


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112122\
Data File : BF131307.D
Acq On : 21 Nov 2022 08:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 22 01:17:52 2022

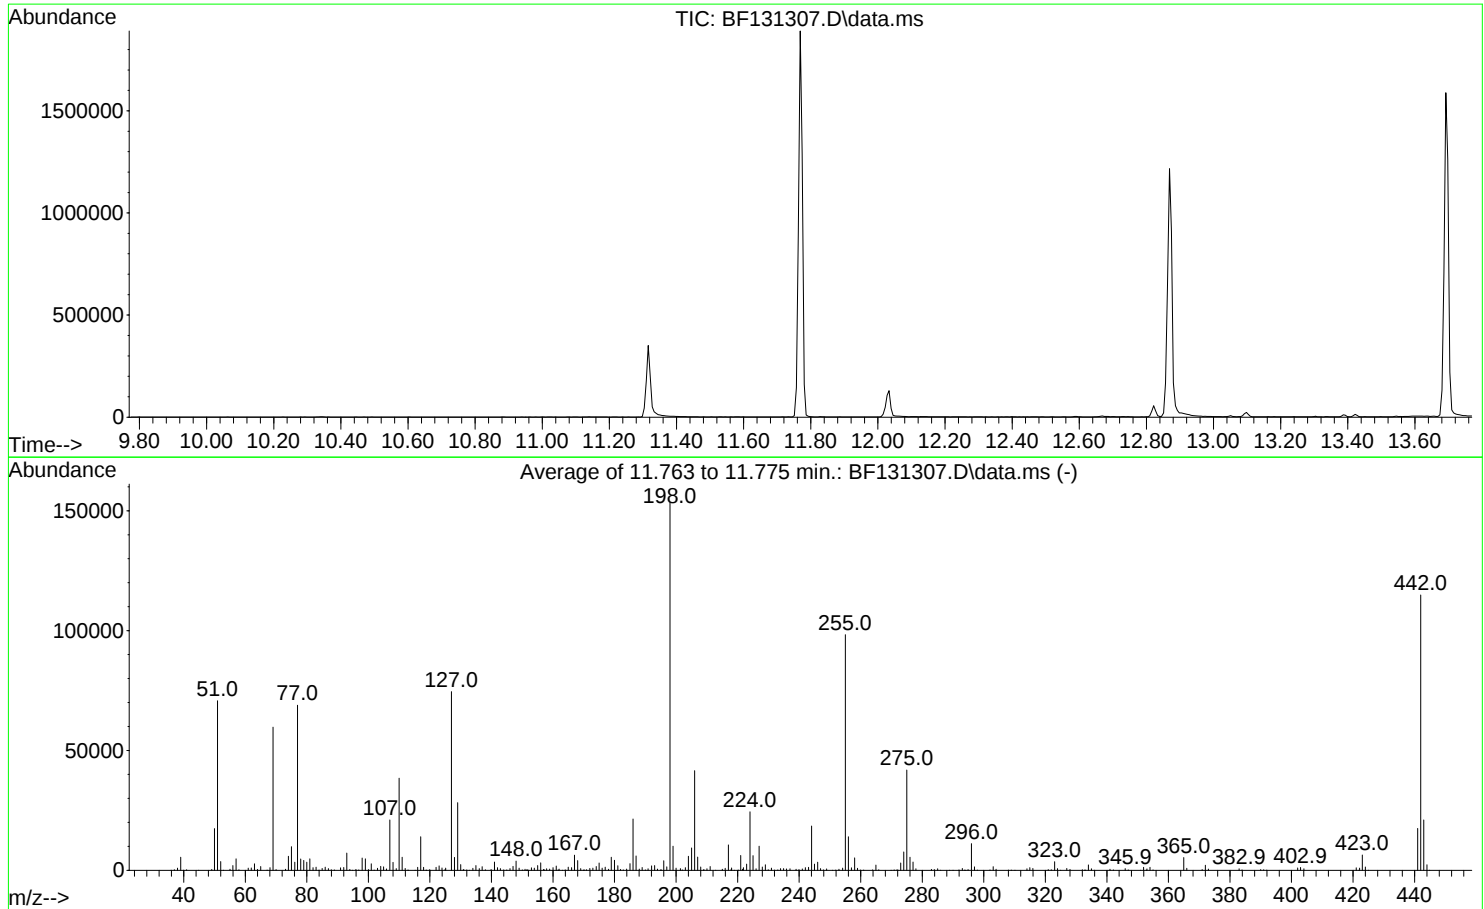




AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1640

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	70749	PASS
68	69	0.00	2	1.8	1081	PASS
69	198	0.00	100	38.9	59723	PASS
70	69	0.00	2	0.5	275	PASS
127	198	10	80	48.6	74576	PASS
197	198	0.00	2	1.0	1470	PASS
198	198	100	100	100.0	153493	PASS
199	198	5	9	6.6	10073	PASS
275	198	10	60	27.3	41845	PASS
365	198	1	100	3.5	5335	PASS
441	198	0.01	100	11.4	17484	PASS
442	442	50	100	100.0	114891	PASS
443	442	15	24	18.3	20971	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112122\
Data File : BF131307.D
Acq On : 21 Nov 2022 08:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 22 06:05:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 01:17:52 2022
Response via : Initial Calibration

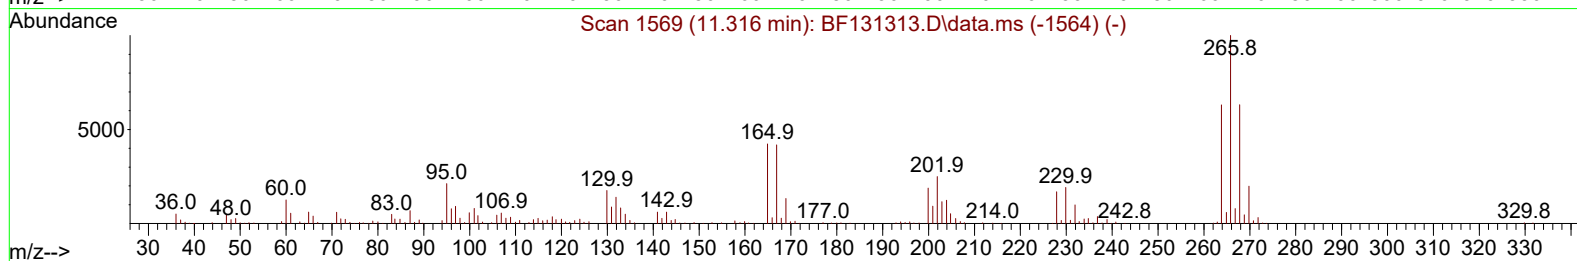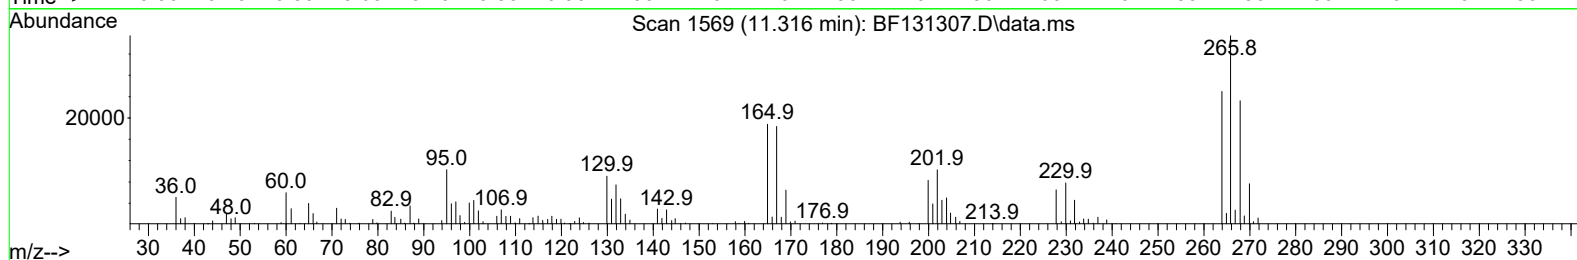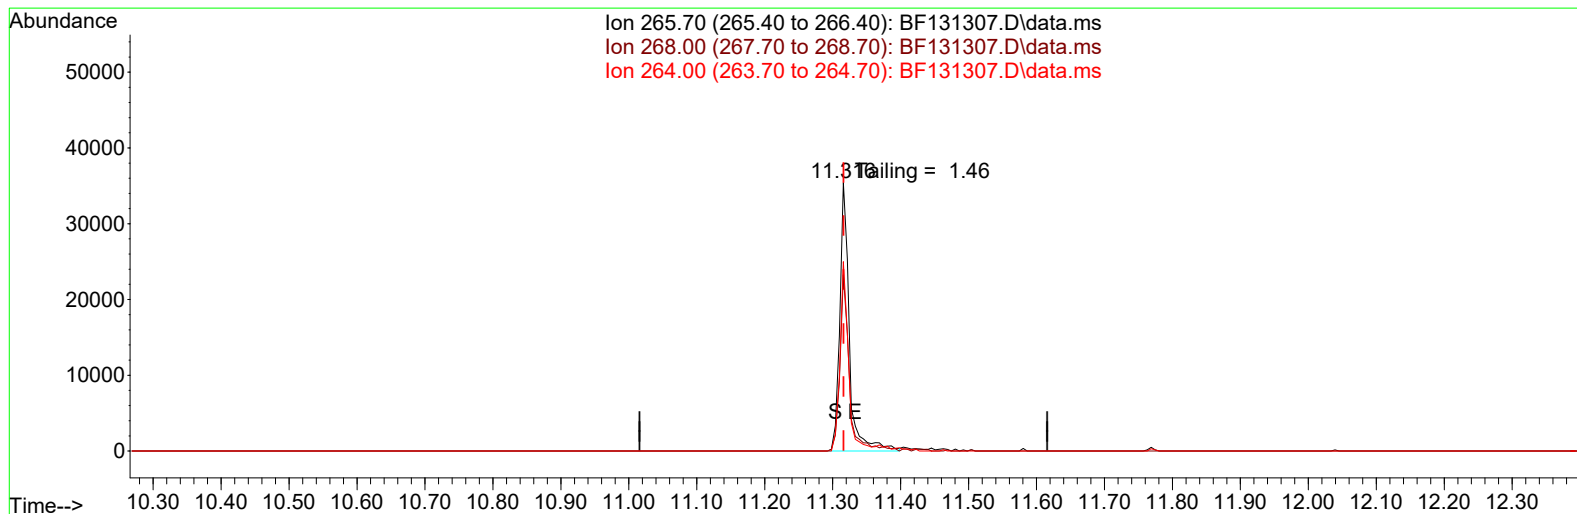

TIC: BF131307.D\data.ms

(70) Pentachlorophenol (C)

11.316min (-0.000) 7989.25 ng




response 34834

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	65.63
264.00	63.00	70.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112122\
Data File : BF131307.D
Acq On : 21 Nov 2022 08:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 22 06:05:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 01:17:52 2022
Response via : Initial Calibration

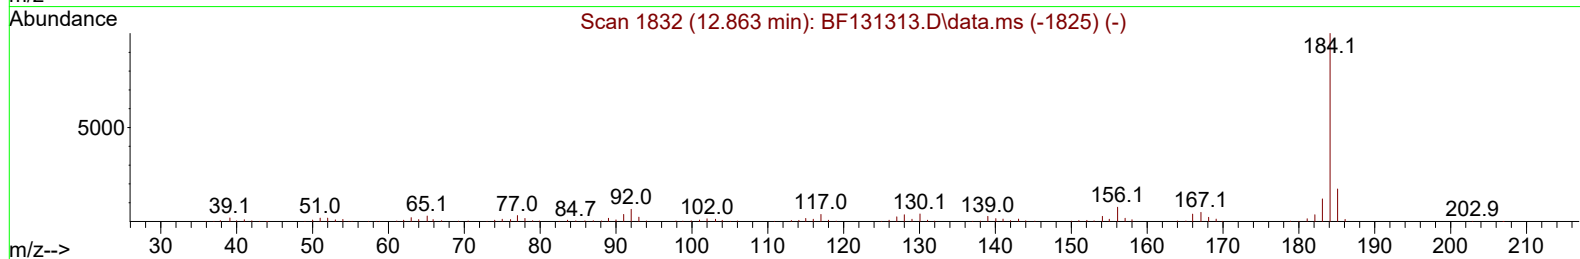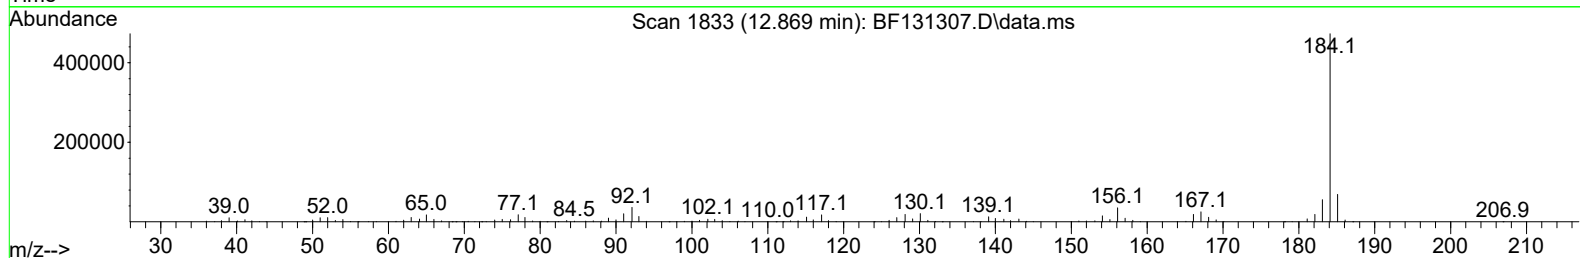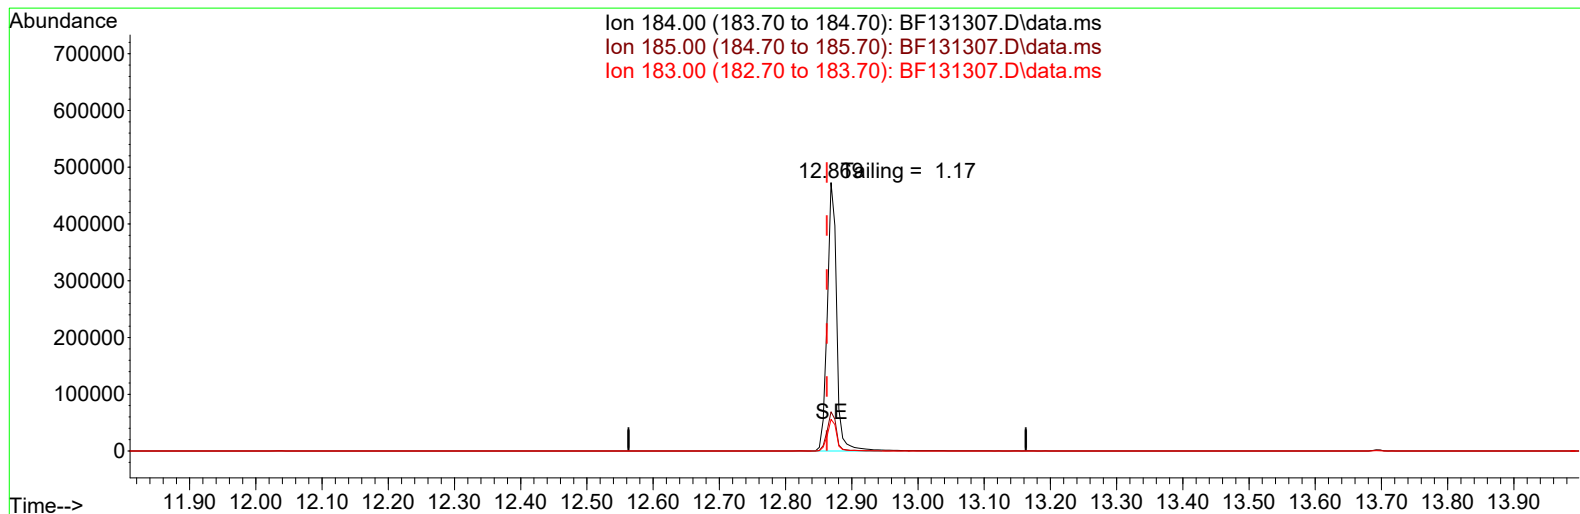

TIC: BF131307.D\data.ms

(77) Benzidine

12.869min (+ 0.006) 0.00 ng

response 467344

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	14.61
183.00	12.00	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/21/2022	BNA_F	<u>BF131307.D</u>
Compound Name	Response	Retention Time
DDT	167853	13.692
DDD	2897	13.386
DDE	866	13.051
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3763	171616	2.19

Instrument :
BNA_F
ClientSampleId :
DFTPP