
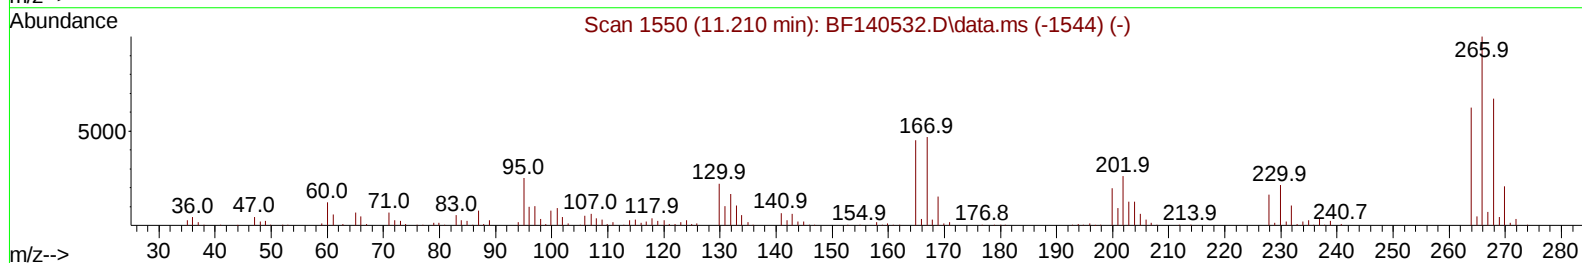
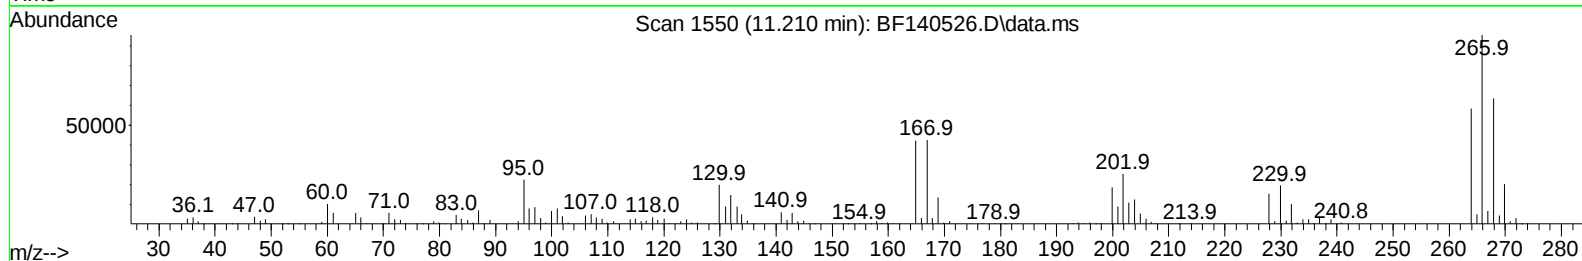


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF-2024\BN-NOV-24\BF112124\
Data File : BF140526.D
Acq On : 21 Nov 2024 10:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 23:23:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

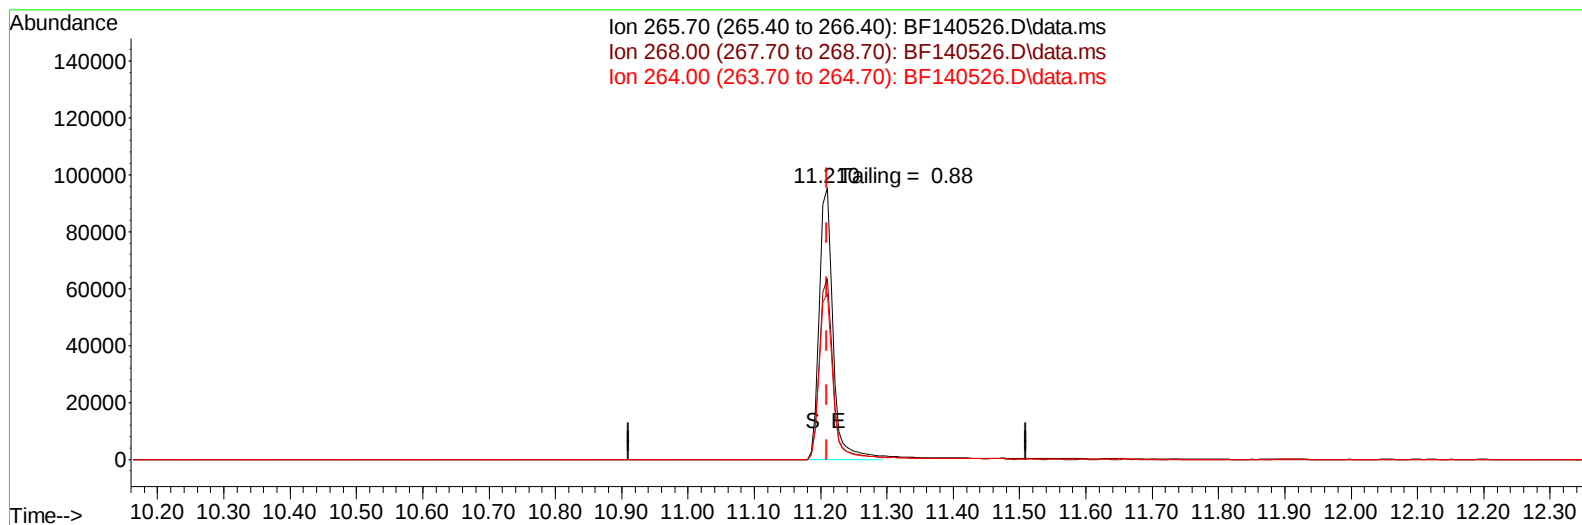




TIC: BF140526.D\data.ms

(70) Pentachlorophenol (C)**11.210min (-0.000) 34448.94 ng****response 138311**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	66.58
264.00	62.30	61.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112124\
Data File : BF140526.D
Acq On : 21 Nov 2024 10:17
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 15:24:39 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

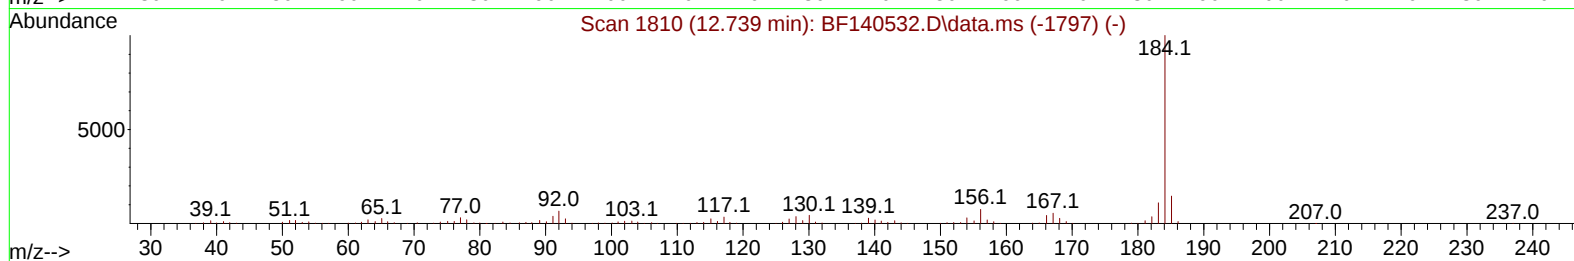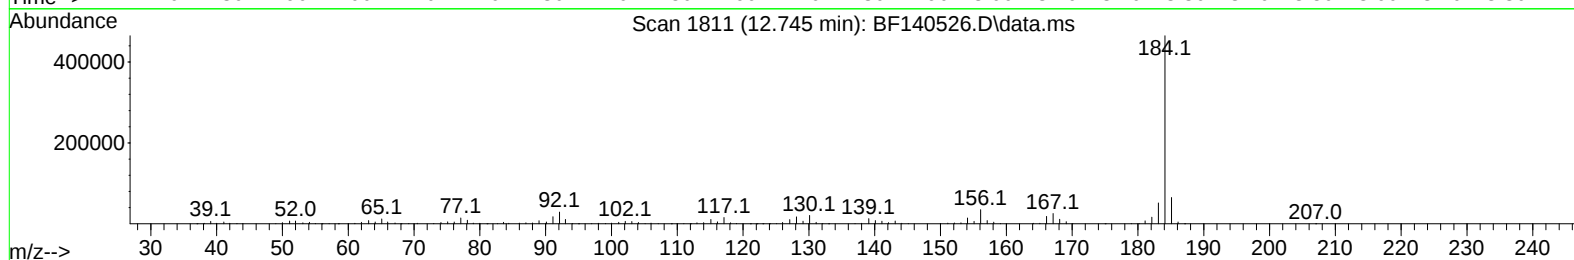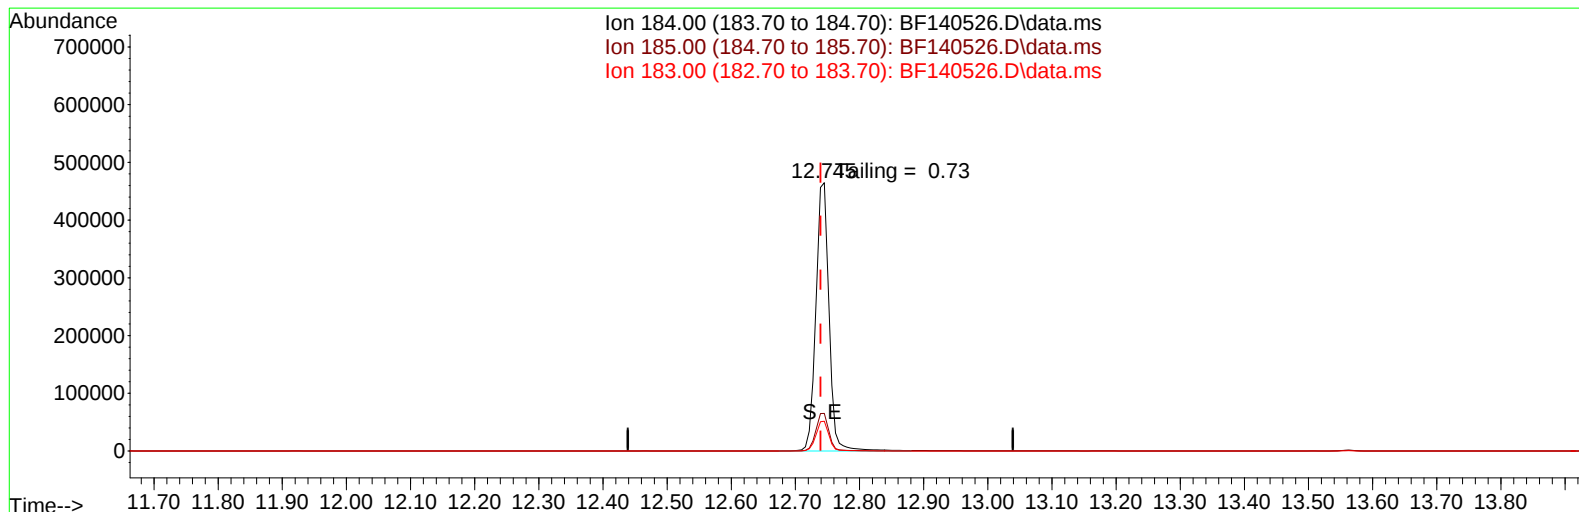

TIC: BF140526.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 32779.12 ng

response 668077

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.02
183.00	11.00	11.11
0.00	0.00	0.00