
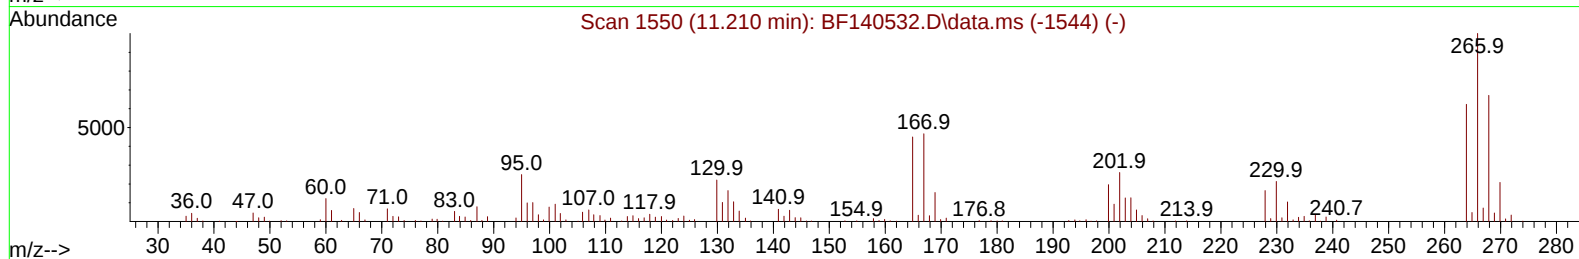
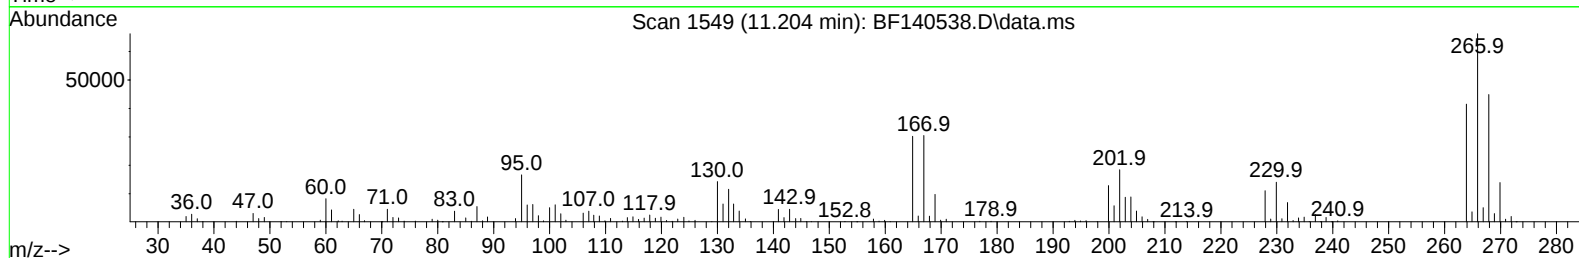


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112124\
Data File : BF140538.D
Acq On : 21 Nov 2024 16:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 16:59:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

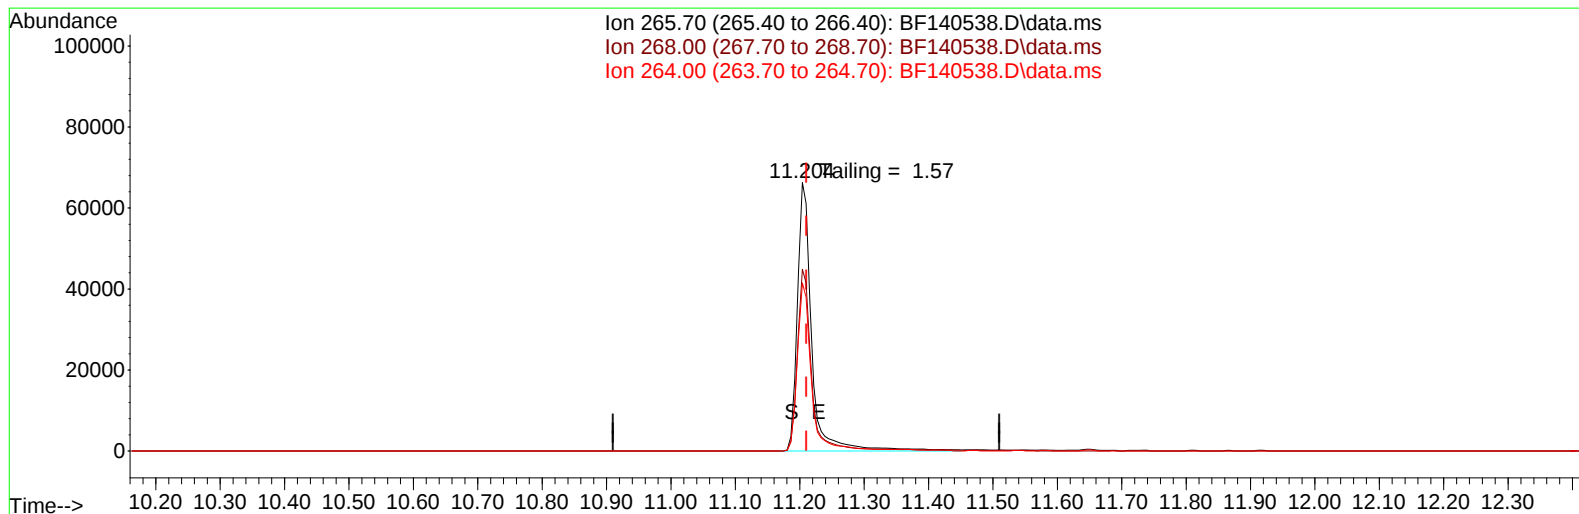

TIC: BF140538.D\data.ms

(70) Pentachlorophenol (C)




11.204min (-0.006) 29910.91 ng

response 102823

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	67.75
264.00	62.30	62.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112124\
Data File : BF140538.D
Acq On : 21 Nov 2024 16:27
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 21 16:59:21 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

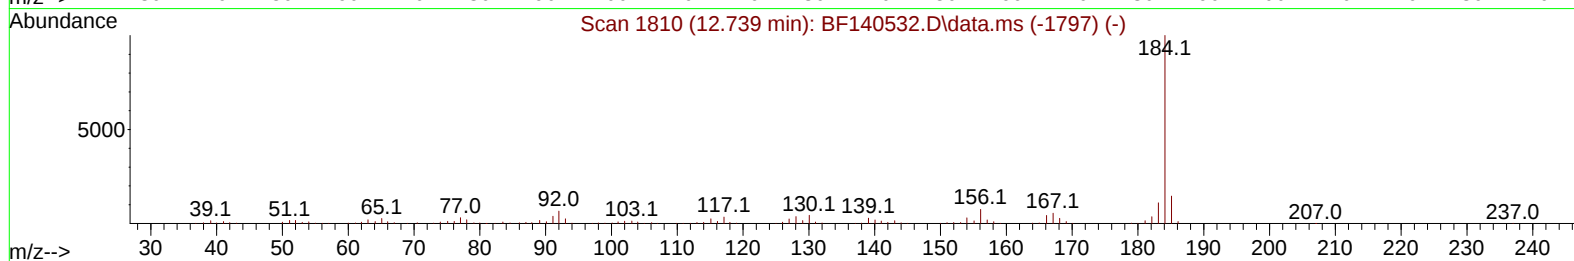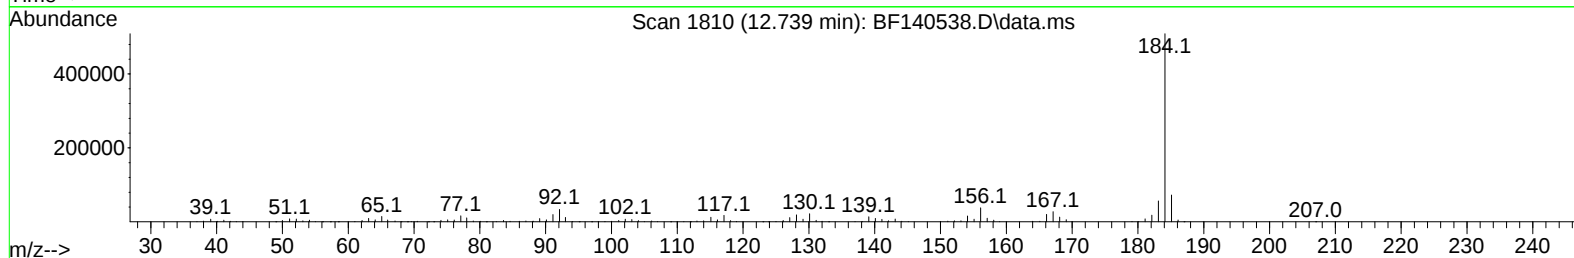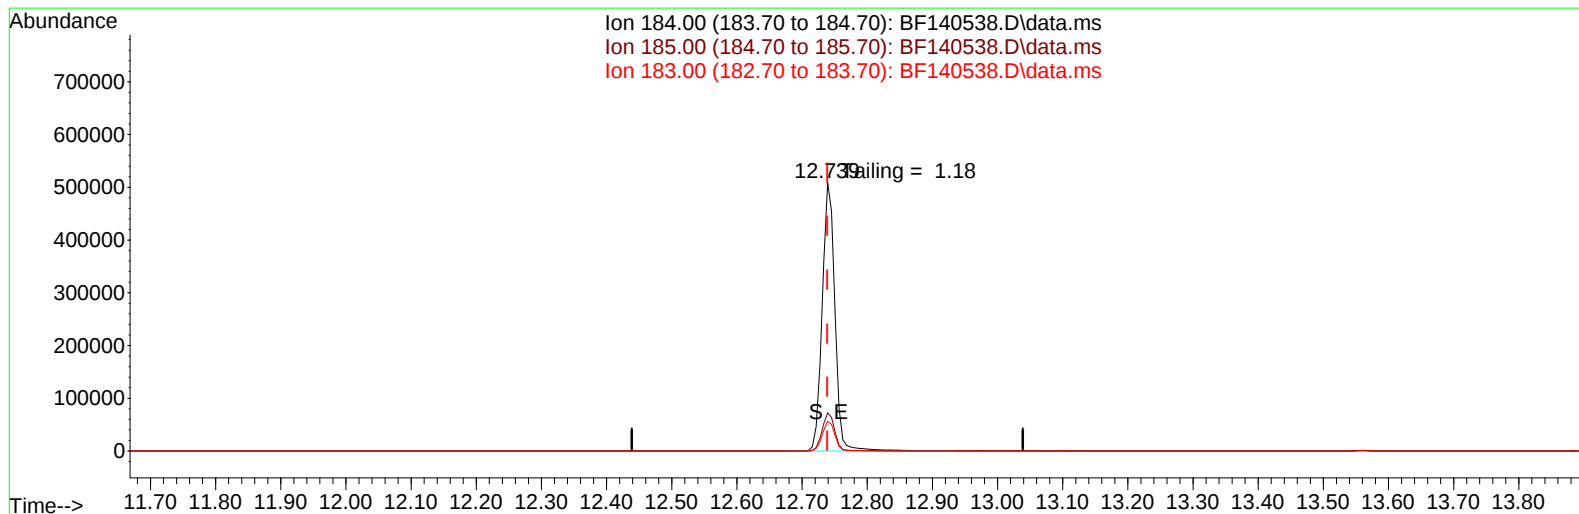

TIC: BF140538.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 64322.88 ng

response 691956

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.28
183.00	11.00	11.13
0.00	0.00	0.00