

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112124\
 Data File : BF140553.D
 Acq On : 21 Nov 2024 23:10
 Operator : RC/JU
 Sample : P4887-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MH-739

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140553.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.493	573	578	600	rBV	565472	748924	81.81%	10.797%
2	6.504	744	750	772	rBV	564756	780604	85.27%	11.253%
3	6.869	807	812	820	rBV	342042	416417	45.49%	6.003%
4	7.428	902	907	931	rBV	371834	491723	53.71%	7.089%
5	7.692	948	952	964	rVB6	5576	16131	1.76%	0.233%
6	8.151	1025	1030	1044	rBV	397454	516986	56.47%	7.453%
7	9.222	1207	1212	1233	rBV	696917	915452	100.00%	13.197%
8	9.904	1323	1328	1339	rBV	409496	557106	60.86%	8.031%
9	9.998	1339	1344	1350	rVB	19603	28767	3.14%	0.415%
10	10.622	1445	1450	1458	rBV	52594	69878	7.63%	1.007%
11	10.698	1458	1463	1481	rVV	345771	469302	51.26%	6.765%
12	11.398	1577	1582	1591	rBV	400709	525058	57.36%	7.569%
13	11.922	1666	1671	1681	rBV	6572	12591	1.38%	0.182%
14	12.980	1846	1851	1864	rBV	559983	709325	77.48%	10.226%
15	14.045	2026	2032	2044	rBV	276790	384466	42.00%	5.542%
16	15.527	2278	2284	2297	rVB	173846	293972	32.11%	4.238%




Sum of corrected areas: 6936702

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112124\
Data File : BF140553.D
Acq On : 21 Nov 2024 23:10
Operator : RC/JU
Sample : P4887-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-739

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

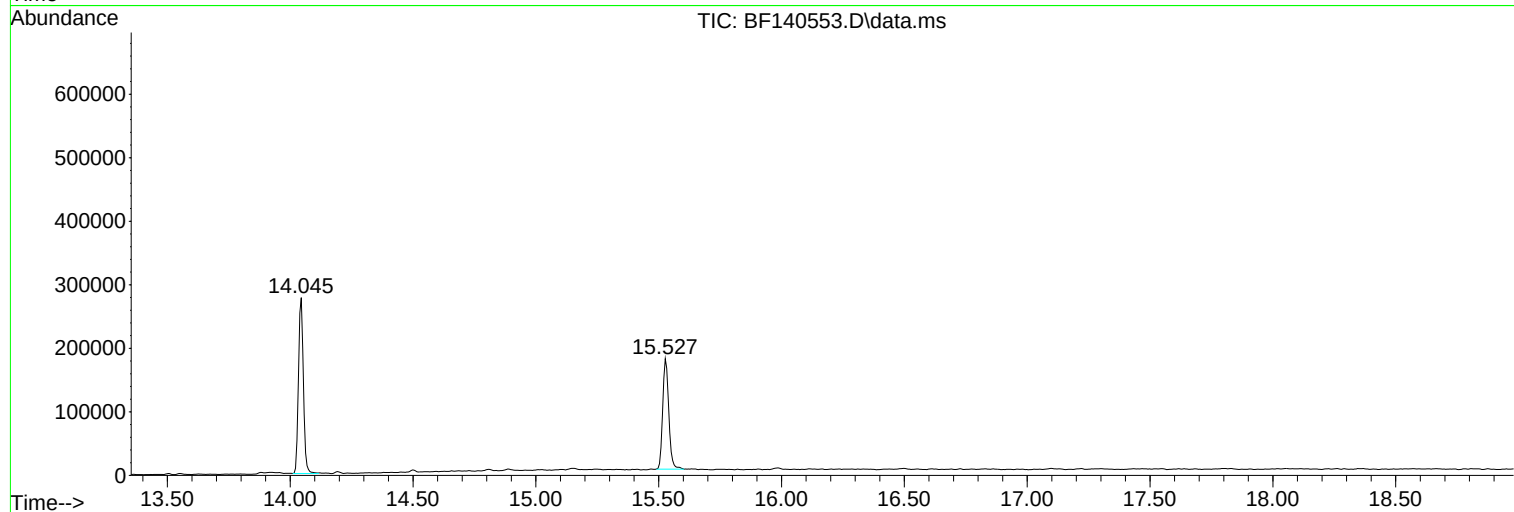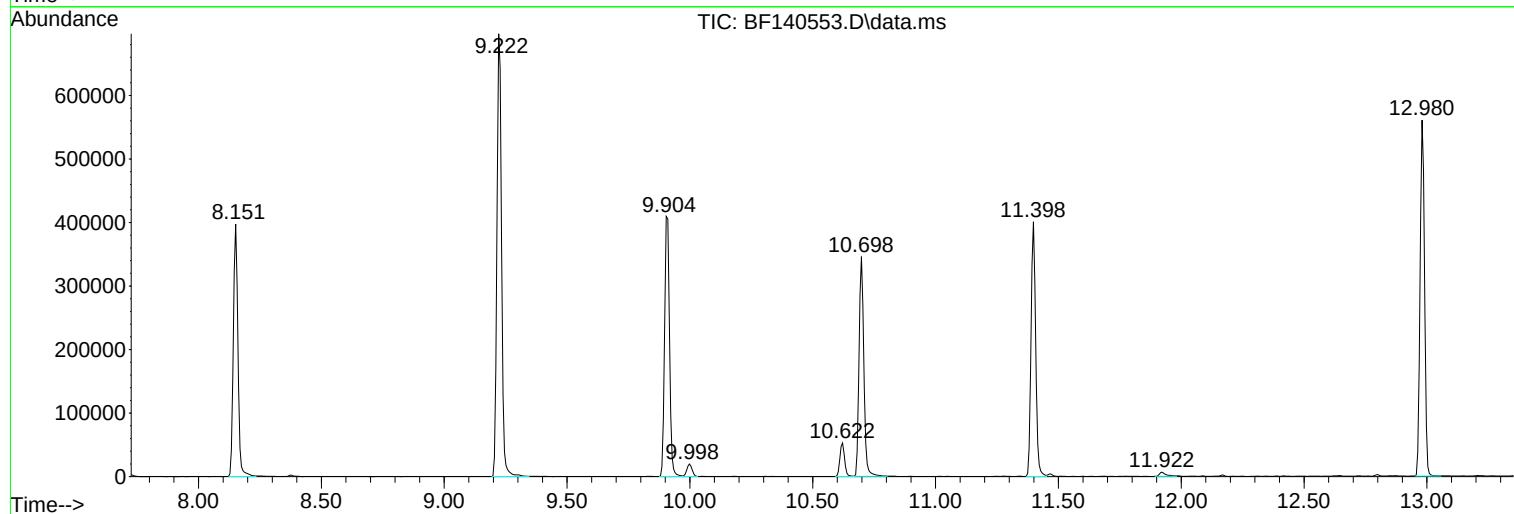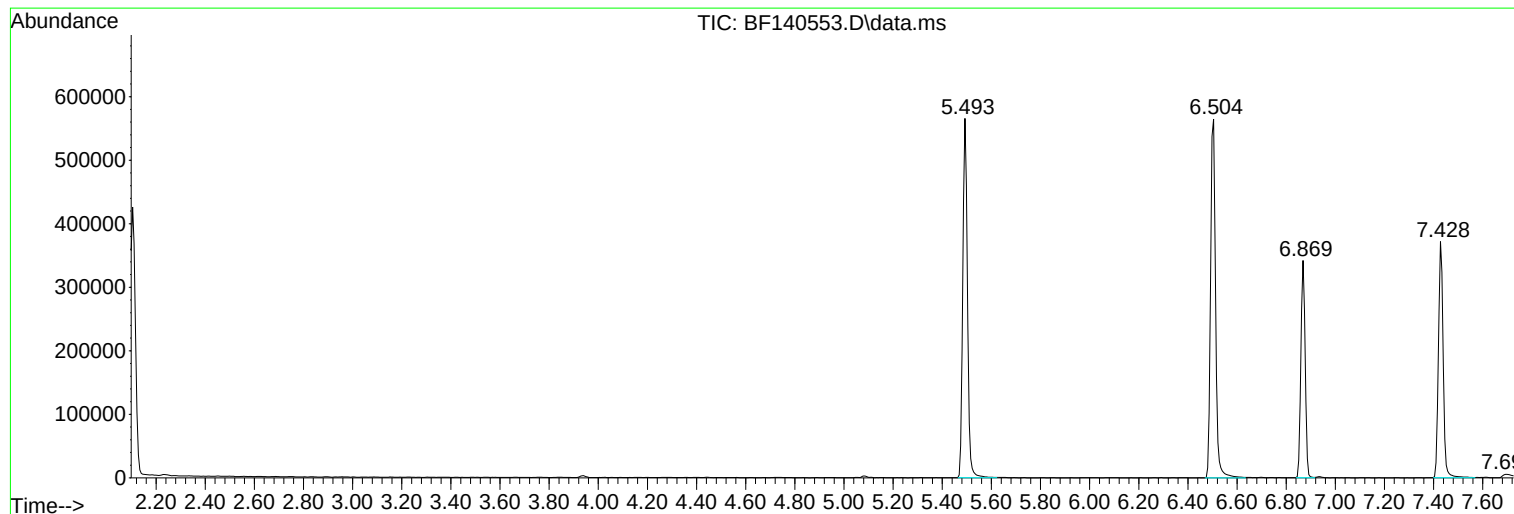

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112124\
Data File : BF140553.D
Acq On : 21 Nov 2024 23:10
Operator : RC/JU
Sample : P4887-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-739










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzophenone Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.622	2.51 ng	69878	Acenaphthene-d10	9.904

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzophenone	182	C13H10O	000119-61-9	96
2			Benzenecarbothioic acid, S-methy...	152	C8H8OS	005925-68-8	52
3			Benzenecarbothioic acid	138	C7H6OS	000098-91-9	47
4			N-Methylbenzamide, N-pentafluoro...	281	C11H8F5NO2	1000446-98-1	47
5			Benzenebutanoic acid, .gamma.-oxo-	178	C10H10O3	002051-95-8	47

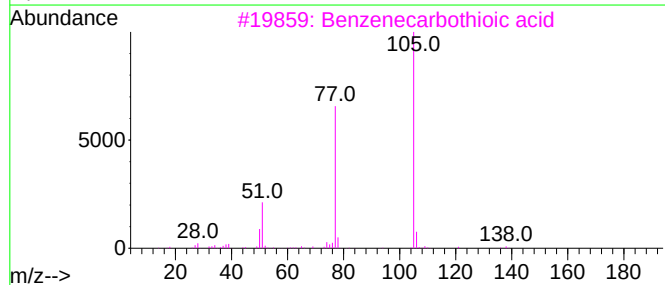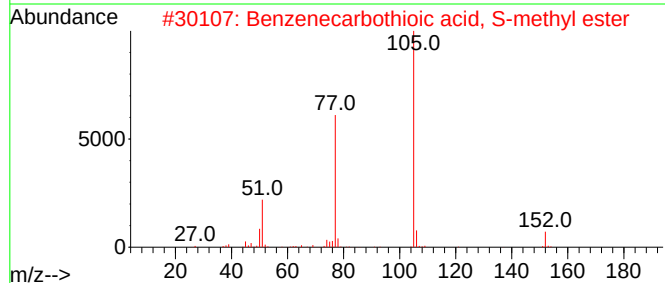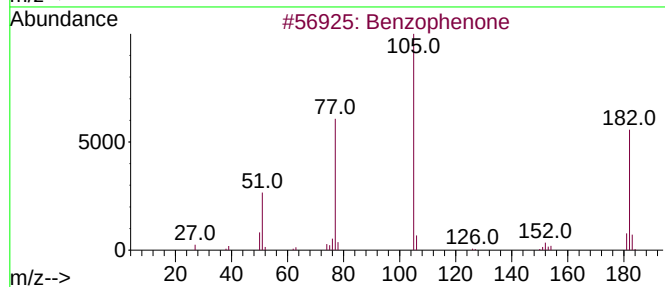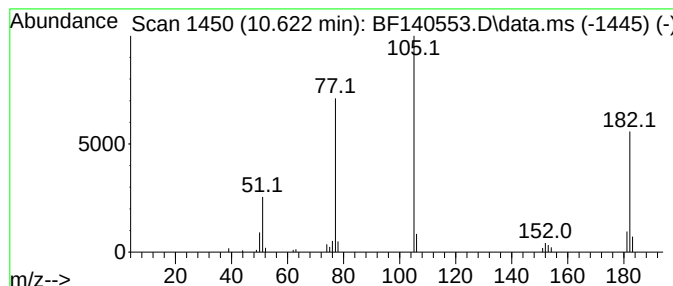

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112124\
Data File : BF140553.D
Acq On : 21 Nov 2024 23:10
Operator : RC/JU
Sample : P4887-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-739

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzophenone	10.622	2.5	ng	69878	3	9.904	557106	20.0