

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112215\
 Data File : BF083192.D
 Acq On : 23 Nov 2015 7:27
 Operator : UM/IZ
 Sample : G4437-05
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-25

Quant Time: Nov 23 17:12:56 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 22 09:22:46 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.65	152	212574	20.00	ng	-0.01
21) Naphthalene-d8	7.94	136	757689	20.00	ng	-0.01
38) Acenaphthene-d10	9.68	164	341997	20.00	ng	-0.02
63) Phenanthrene-d10	11.15	188	574295	20.00	ng	-0.02
75) Chrysene-d12	13.78	240	509356	20.00	ng	-0.02
86) Perylene-d12	15.15	264	394214	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.26	112	971766	69.11	ng	-0.02
7) Phenol-d6	6.31	99	800525	44.00	ng	-0.03
23) Nitrobenzene-d5	7.22	82	1606075	96.86	ng	-0.01
41) 2,4,6-Tribromophenol	10.48	330	472924	135.17	ng	-0.01
44) 2-Fluorobiphenyl	9.02	172	2353490	95.96	ng	-0.01
78) Terphenyl-d14	12.75	244	2024648	93.60	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112215\
Data File : BF083192.D
Acq On : 23 Nov 2015 7:27
Operator : UM/IZ
Sample : G4437-05
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-25

Quant Time: Nov 23 17:12:56 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 09:22:46 2015
Response via : Initial Calibration

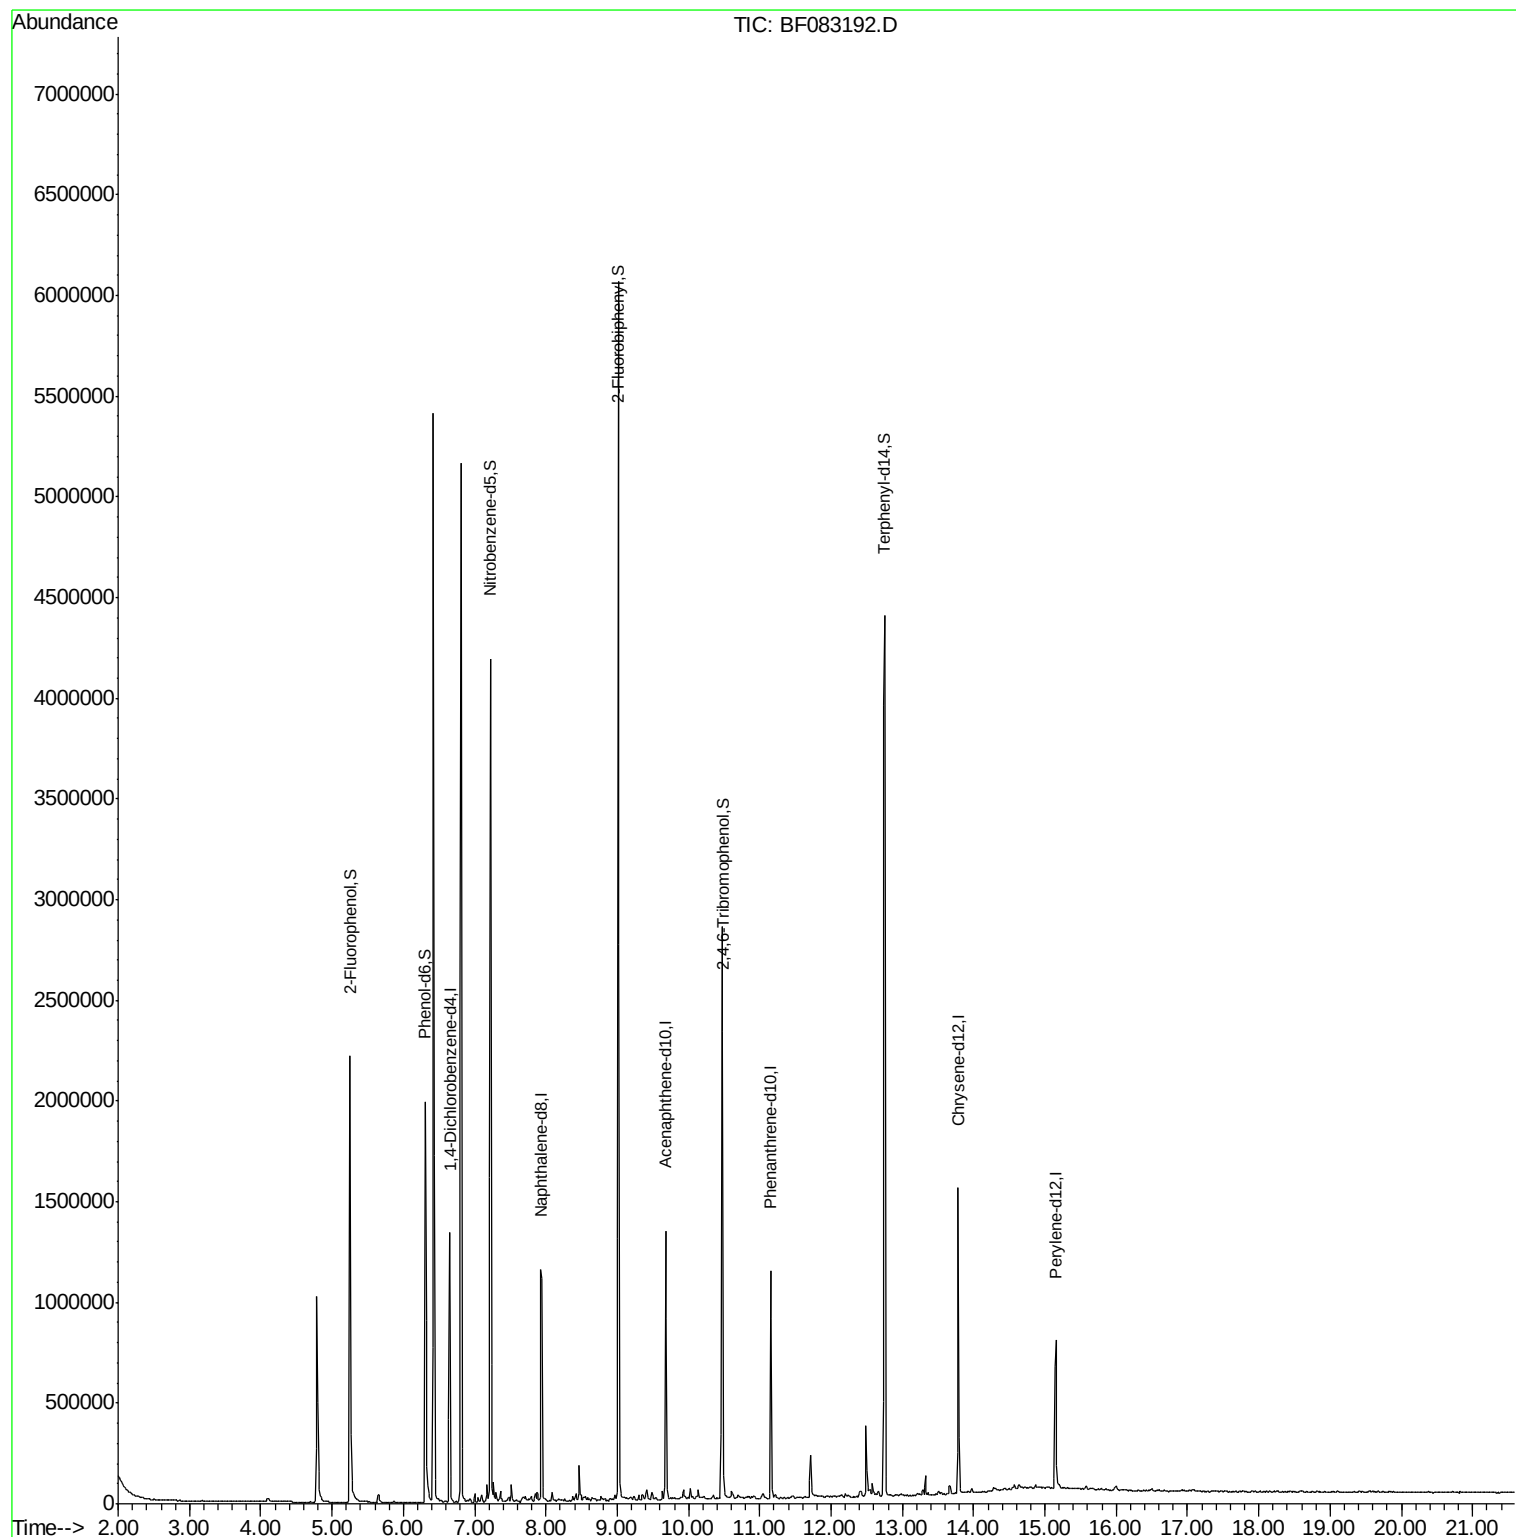

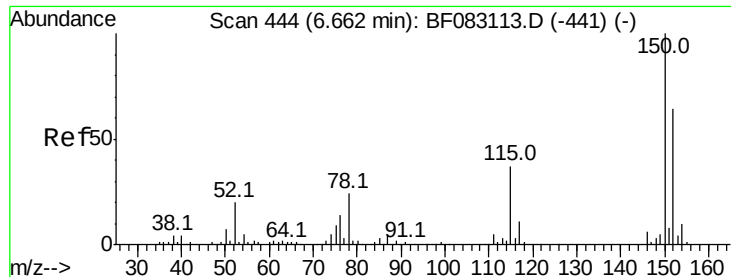

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.65 min Scan# 408

Delta R.T. -0.01 min

Lab File: BF083192.D

Acq: 23 Nov 2015 7:27

Instrument :

BNA_F

ClientSampleId :

MW-25


Tot Ion:152 Resp: 212574

Ion Ratio Lower Upper

152 100

150 155.7 125.8 188.8




115 59.1 46.9 70.3

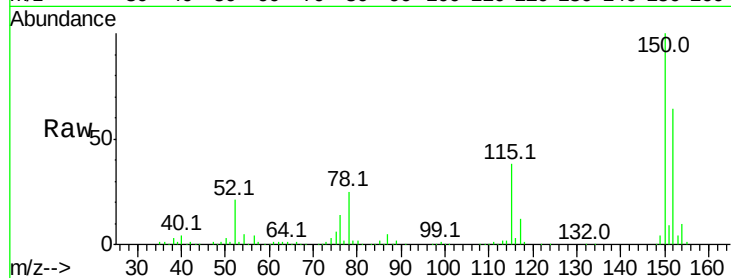

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

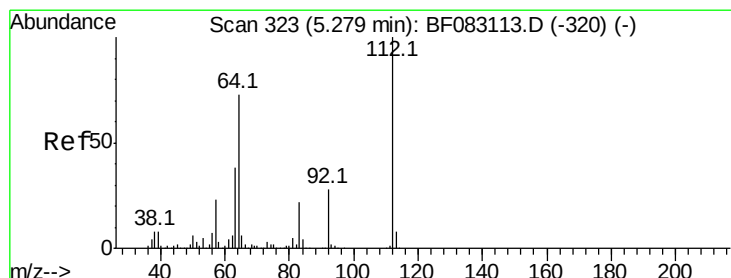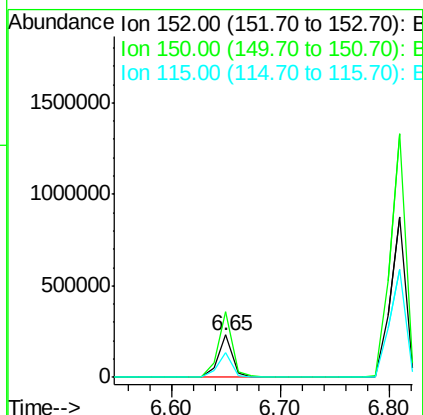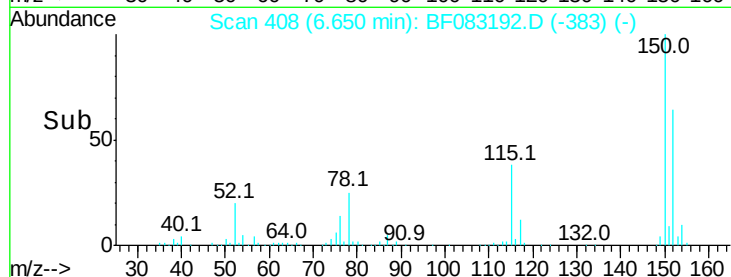

#5

2-Fluorophenol

Concen: 69.11 ng

RT: 5.26 min Scan# 286

Delta R.T. -0.02 min

Lab File: BF083192.D

Acq: 23 Nov 2015 7:27


Tgt Ion:112 Resp: 971766

Ion Ratio Lower Upper

112 100

64 56.7 58.4 87.6#



63 27.8 30.0 45.0#

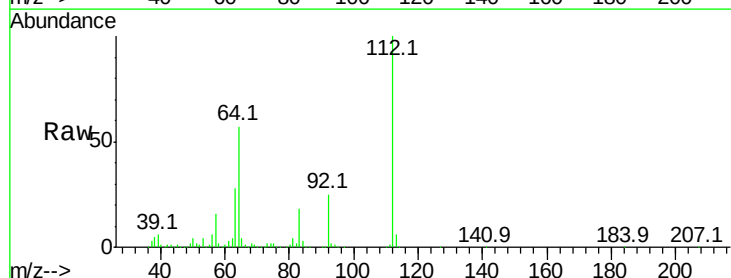


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

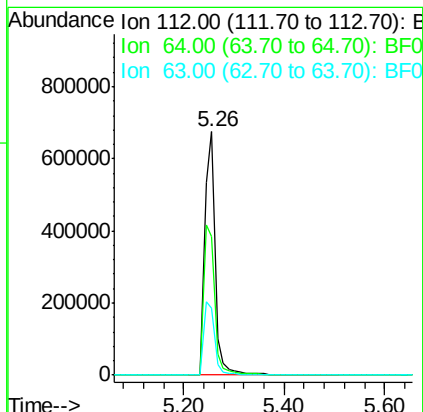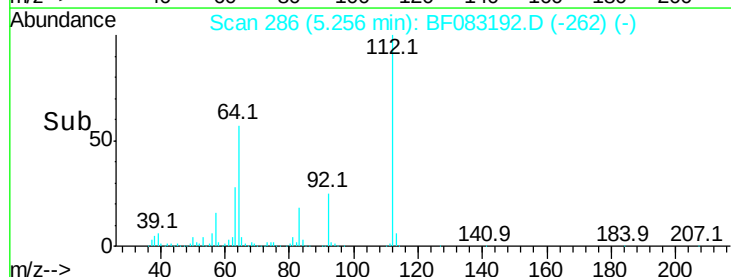

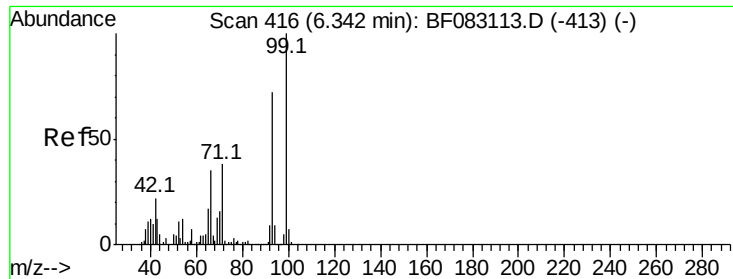

#7

Phenol-d6

Concen: 44.00 ng

RT: 6.31 min Scan# 378

Delta R.T. -0.03 min

Lab File: BF083192.D

Acq: 23 Nov 2015 7:27

Instrument :

BNA_F

ClientSampleId :

MW-25


Tot Ion: 99 Resp: 800525

Ion Ratio Lower Upper

99 100

42 22.4 17.7 26.5




71 34.2 30.2 45.4

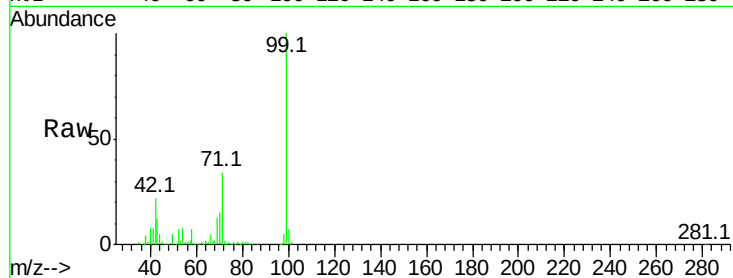

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

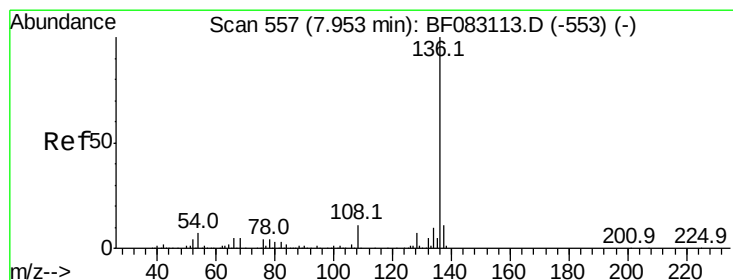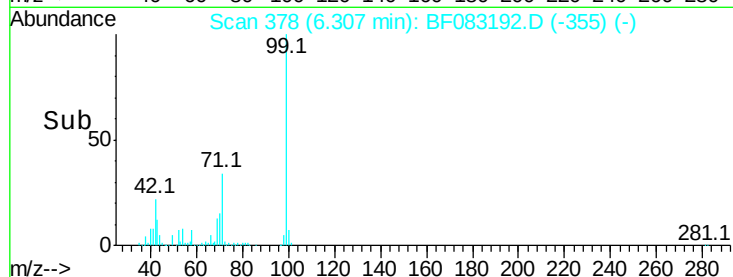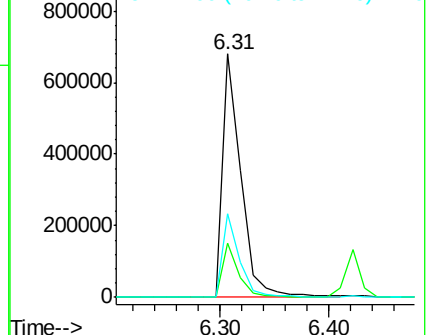

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.94 min Scan# 521

Delta R.T. -0.01 min

Lab File: BF083192.D

Acq: 23 Nov 2015 7:27

Tgt Ion: 136 Resp: 757689


Ion Ratio Lower Upper

136 100

137 10.6 8.7 13.1

54 7.5 5.8 8.6

68 5.4 3.8 5.8


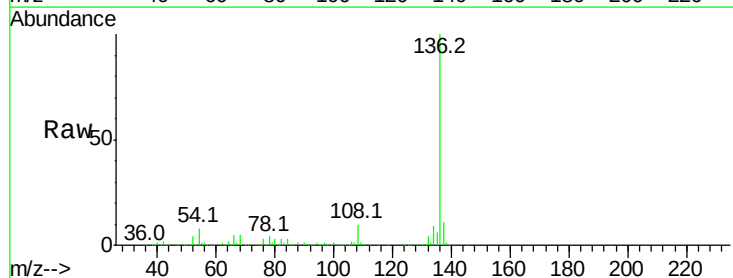



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

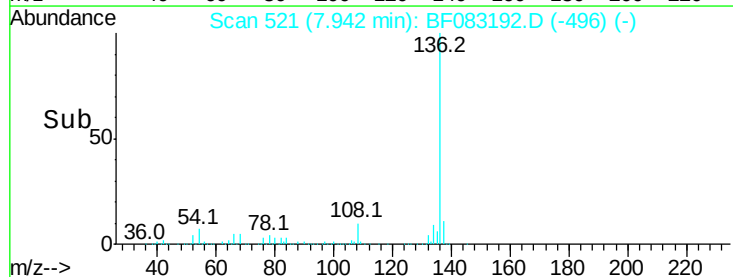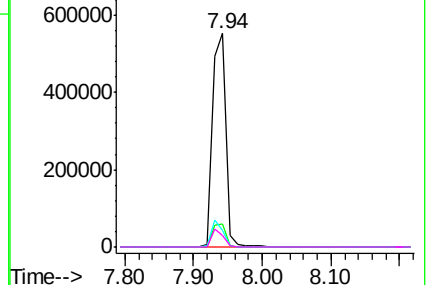

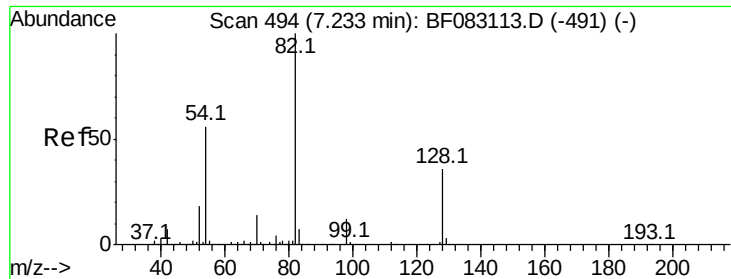


#23
 Nitrobenzene-d5
 Concen: 96.86 ng
 RT: 7.22 min Scan# 458
 Delta R.T. -0.01 min
 Lab File: BF083192.D
 Acq: 23 Nov 2015 7:27




Instrument :
 BNA_F
 ClientSampleId :
 MW-25

Tot Ion: 82 Resp: 1606075

Ion	Ratio	Lower	Upper
82	100		
128	37.9	28.5	42.7
54	54.9	44.6	67.0

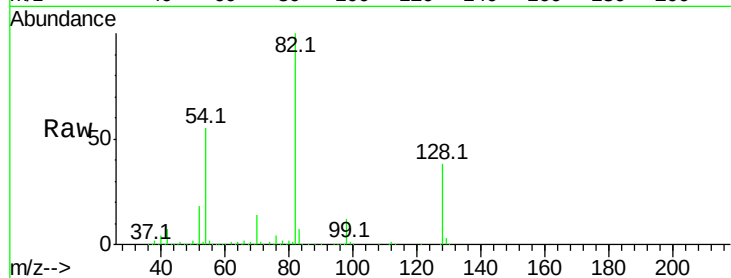


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

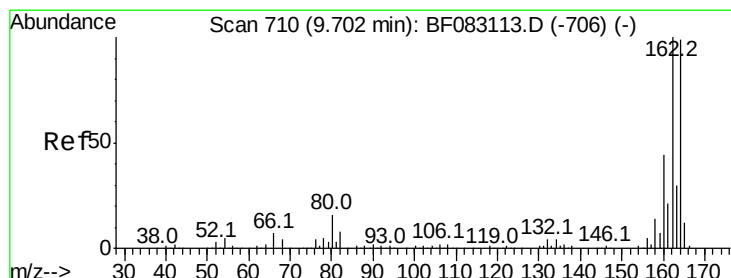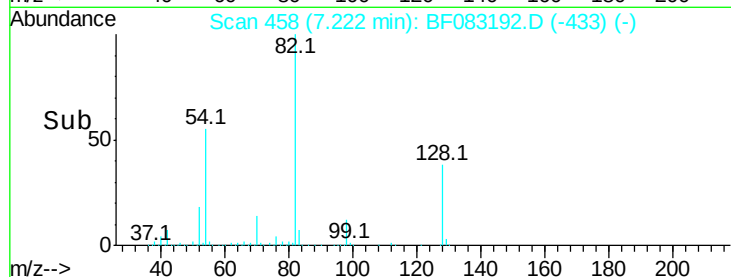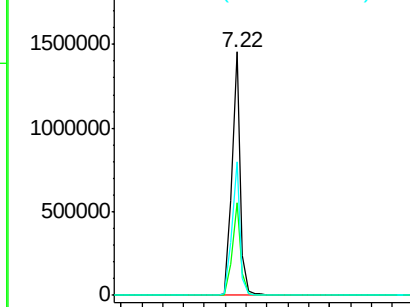



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.68 min Scan# 673
 Delta R.T. -0.02 min
 Lab File: BF083192.D
 Acq: 23 Nov 2015 7:27


Tgt Ion:164 Resp: 341997

Ion	Ratio	Lower	Upper
164	100		
162	100.2	81.2	121.8
160	41.1	35.6	53.4

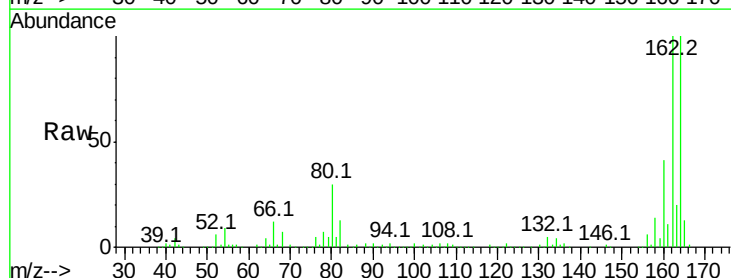

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

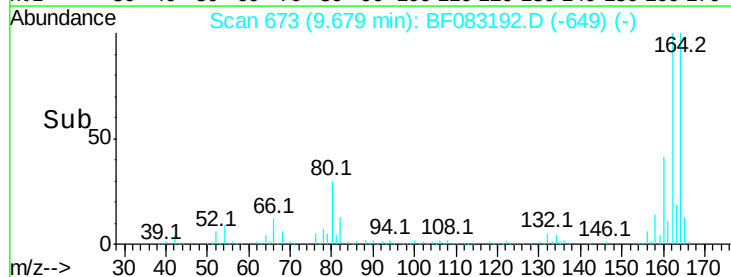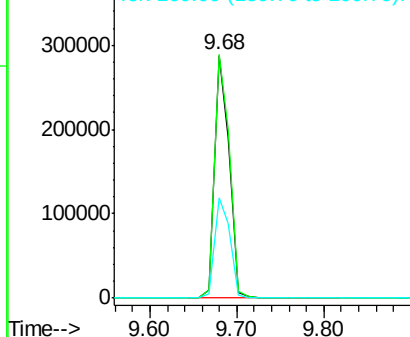


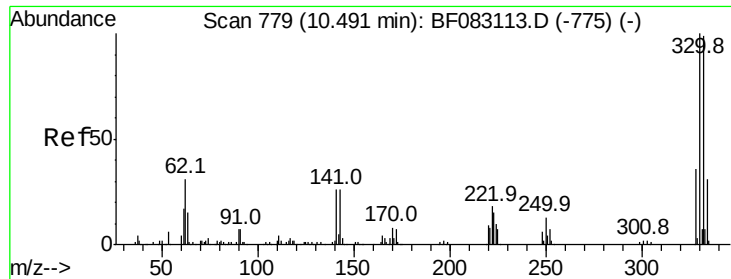




#41
 2,4,6-Tribromophenol
 Concen: 135.17 ng
 RT: 10.48 min Scan# 743
 Delta R.T. -0.01 min
 Lab File: BF083192.D
 Acq: 23 Nov 2015 7:27

Instrument :
 BNA_F
 ClientSampled :
 MW-25

Tot Ion:330 Resp: 472924
 Ion Ratio Lower Upper
 330 100
 332 97.3 77.7 116.5
 141 34.5 29.7 44.5

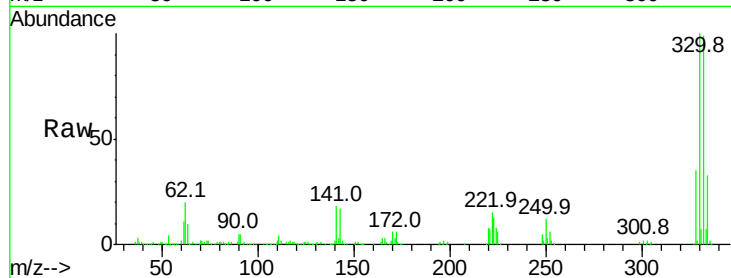


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

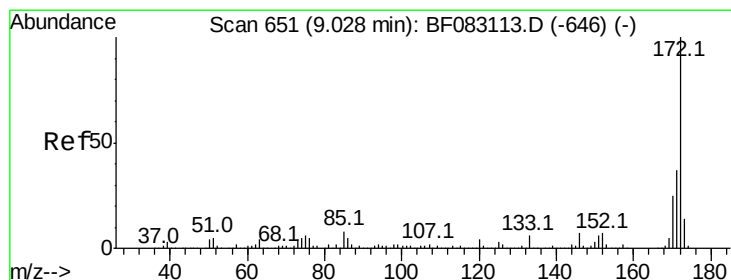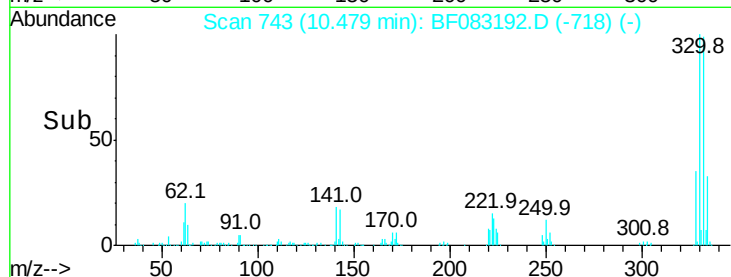
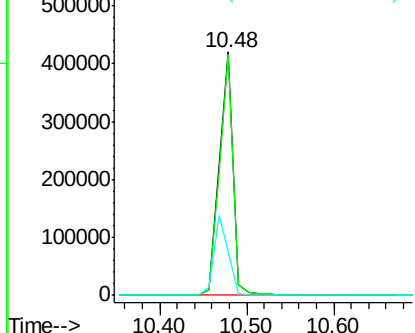



#44
 2-Fluorobiphenyl
 Concen: 95.96 ng
 RT: 9.02 min Scan# 615
 Delta R.T. -0.01 min
 Lab File: BF083192.D
 Acq: 23 Nov 2015 7:27

Tgt Ion:172 Resp: 2353490
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.5 44.3
 170 24.9 19.9 29.9

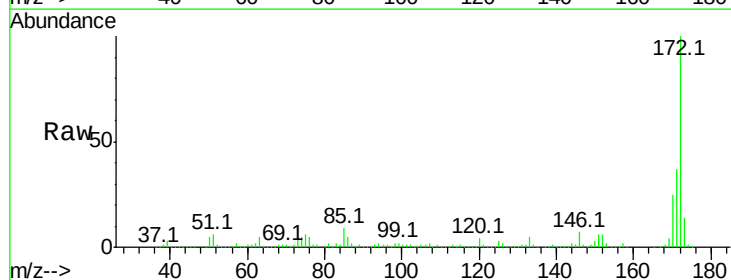

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



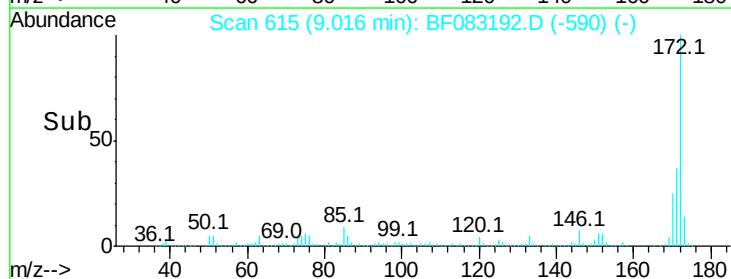
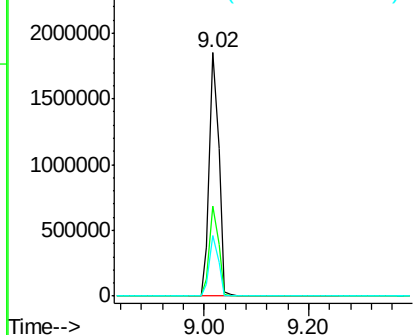


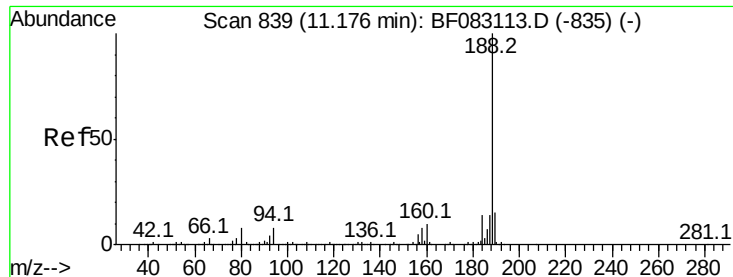

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.15 min Scan# 802
Delta R.T. -0.02 min
Lab File: BF083192.D
Acq: 23 Nov 2015 7:27




Instrument :
BNA_F
ClientSampled :
MW-25


Tot Ion:188 Resp: 574295
Ion Ratio Lower Upper
188 100
94 14.0 6.0 9.0#
80 16.7 6.7 10.1#

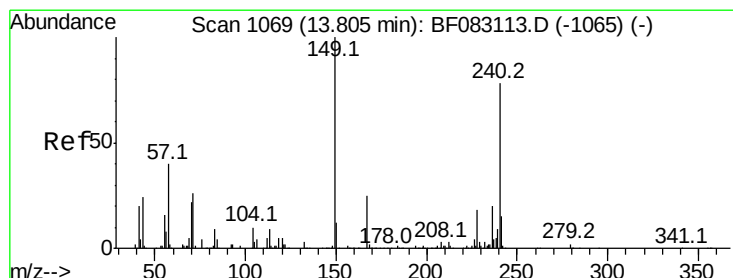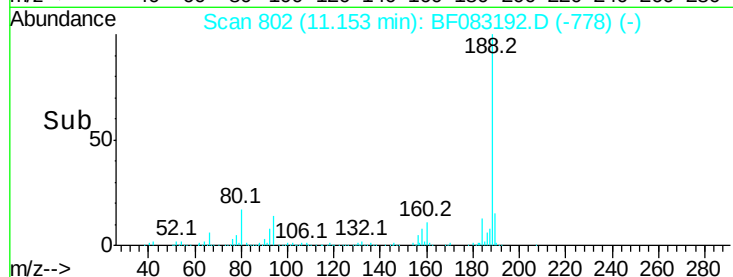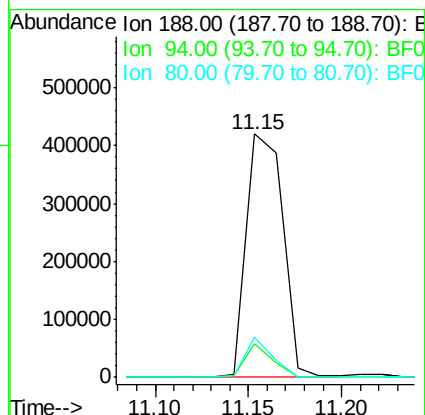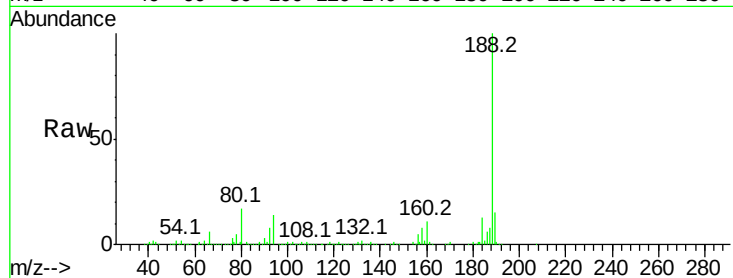

#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.78 min Scan# 1032
Delta R.T. -0.02 min
Lab File: BF083192.D
Acq: 23 Nov 2015 7:27

Tgt Ion:240 Resp: 509356
Ion Ratio Lower Upper
240 100
120 11.8 5.4 8.2#
236 25.8 20.6 31.0

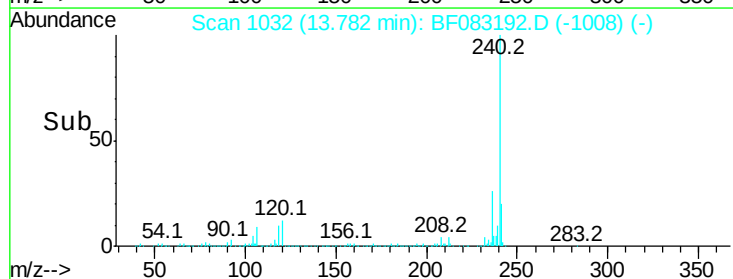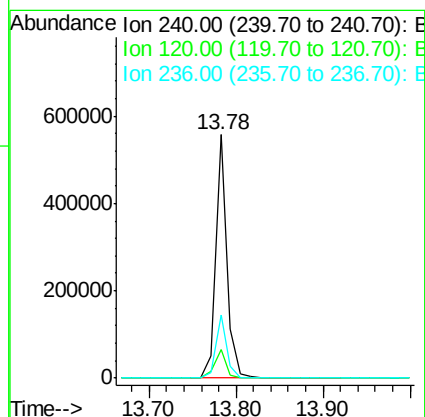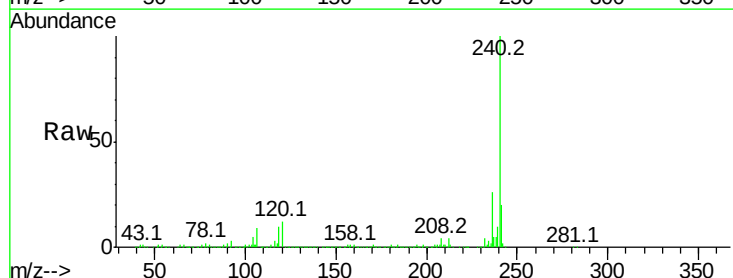

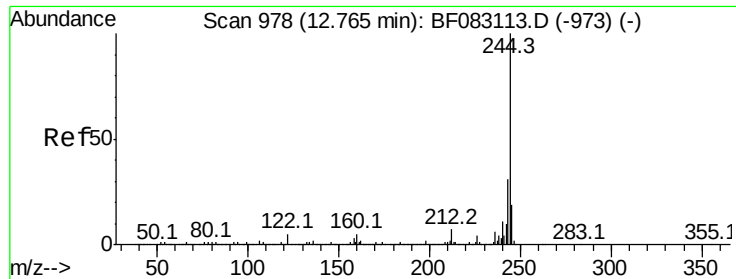

#78

Terphenyl-d14

Concen: 93.60 ng

RT: 12.75 min Scan# 942

Delta R.T. -0.01 min

Lab File: BF083192.D

Acq: 23 Nov 2015 7:27

Instrument :

BNA_F

ClientSampleId :

MW-25


Tot Ion:244 Resp: 2024648

Ion Ratio Lower Upper

244 100

212 7.1 5.4 8.2




122 7.6 4.3 6.5#

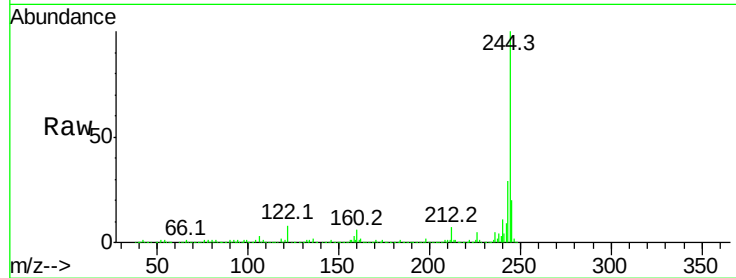

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

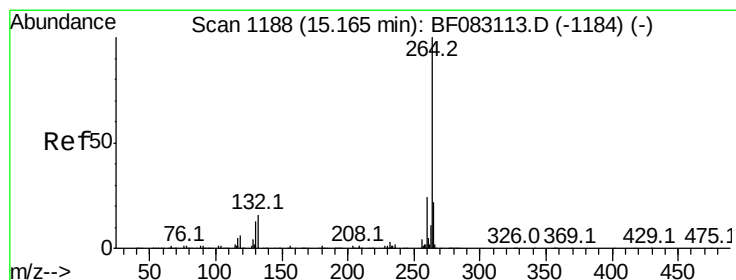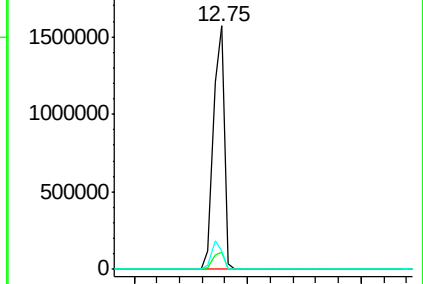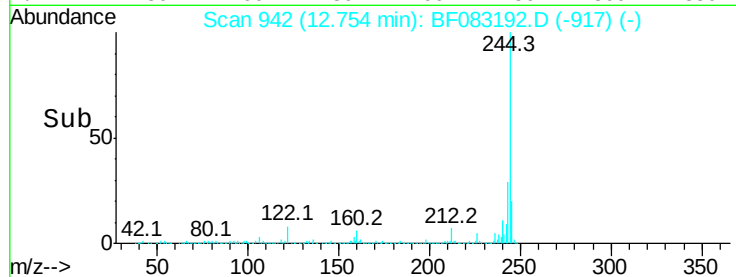

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.15 min Scan# 1152

Delta R.T. -0.01 min

Lab File: BF083192.D

Acq: 23 Nov 2015 7:27


Tgt Ion:264 Resp: 394214

Ion Ratio Lower Upper

264 100

260 22.9 19.1 28.7

265 21.0 18.2 27.4

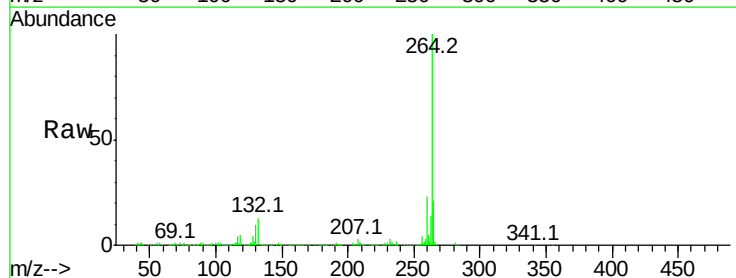

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

