


Data Path : Z:\HPCHEM1\BNA F\Data\BF112215\
 Data File : BF083150.D
 Acq On : 22 Nov 2015 10:54
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Nov 22 09:22:46 2015

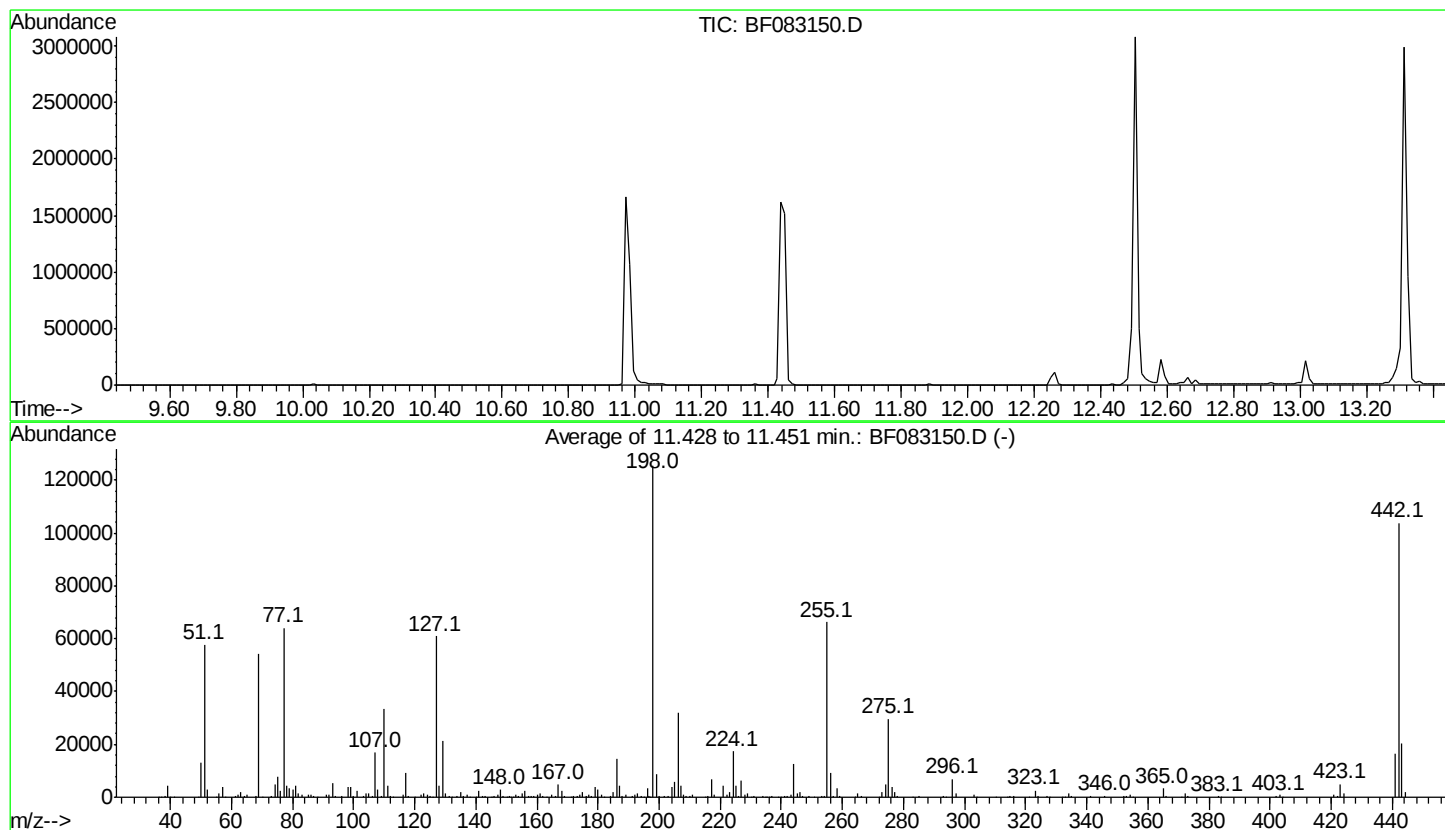

AutoFind: Scans 826, 827, 828; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.0	57662	PASS
68	69	0.00	2	1.3	723	PASS
69	198	0.00	100	43.4	54469	PASS
70	69	0.00	2	0.3	162	PASS
127	198	10	80	48.5	60835	PASS
197	198	0.00	2	0.3	397	PASS
198	198	100	100	100.0	125464	PASS
199	198	5	9	6.8	8556	PASS
275	198	10	60	23.7	29767	PASS
365	198	1	100	2.6	3265	PASS
441	442	0.01	24	16.0	16588	PASS
442	198	50	100	82.7	103801	PASS
443	442	15	24	19.4	20136	PASS