


Data Path : Z:\HPCHEM1\BNA F\DATA\BF112215\
 Data File : BF083174.D
 Acq On : 22 Nov 2015 22:38
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Nov 22 09:22:46 2015

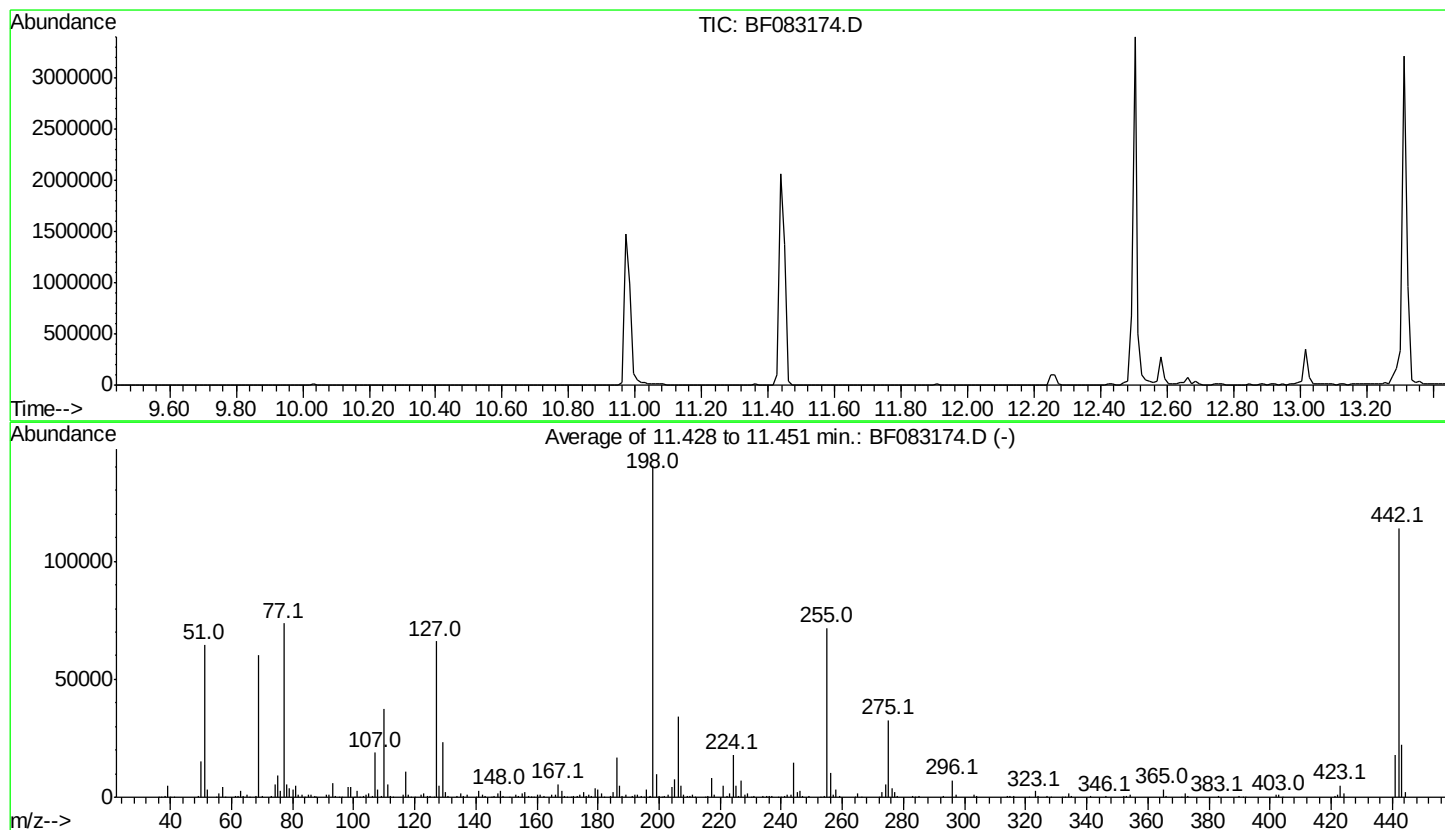

AutoFind: Scans 826, 827, 828; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	64739	PASS
68	69	0.00	2	1.1	672	PASS
69	198	0.00	100	42.9	60296	PASS
70	69	0.00	2	0.5	303	PASS
127	198	10	80	46.9	65972	PASS
197	198	0.00	2	0.4	630	PASS
198	198	100	100	100.0	140550	PASS
199	198	5	9	6.8	9531	PASS
275	198	10	60	23.2	32585	PASS
365	198	1	100	2.4	3333	PASS
441	442	0.01	24	15.7	17870	PASS
442	198	50	100	81.2	114140	PASS
443	442	15	24	19.6	22345	PASS