
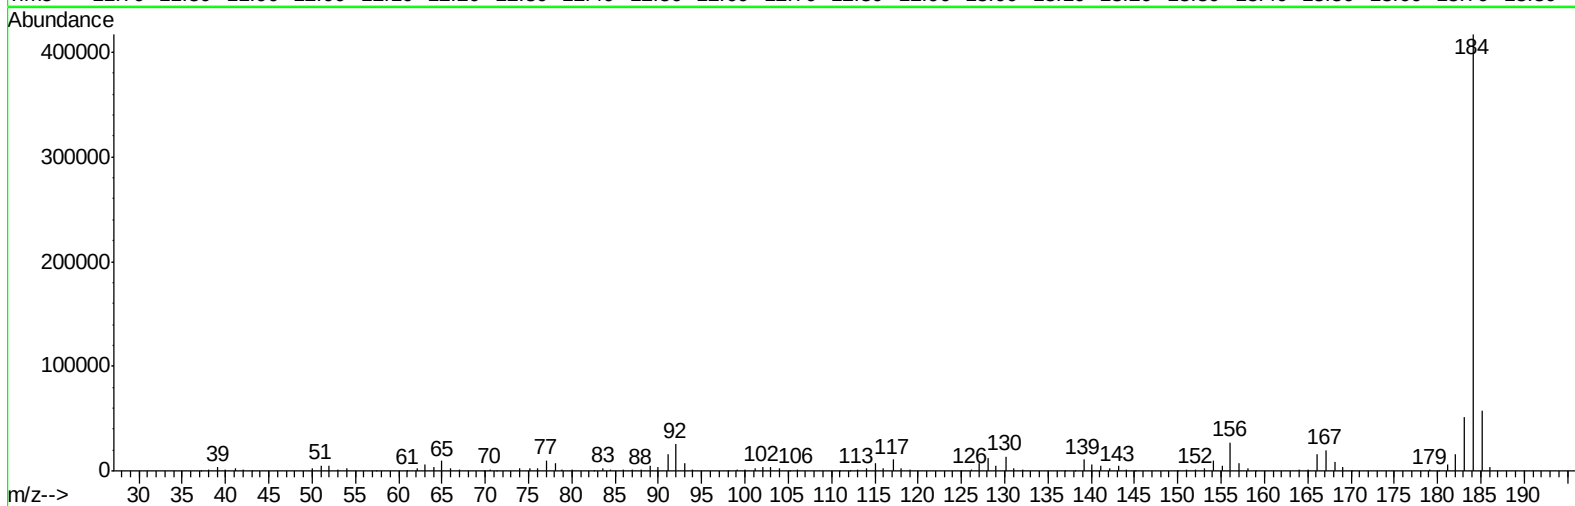


Data Path : Z:\HPCHEM1\BNA F\Data\BF112217\
Data File : BF100812.D
Acq On : 22 Nov 2017 8:44
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 23:56:18 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

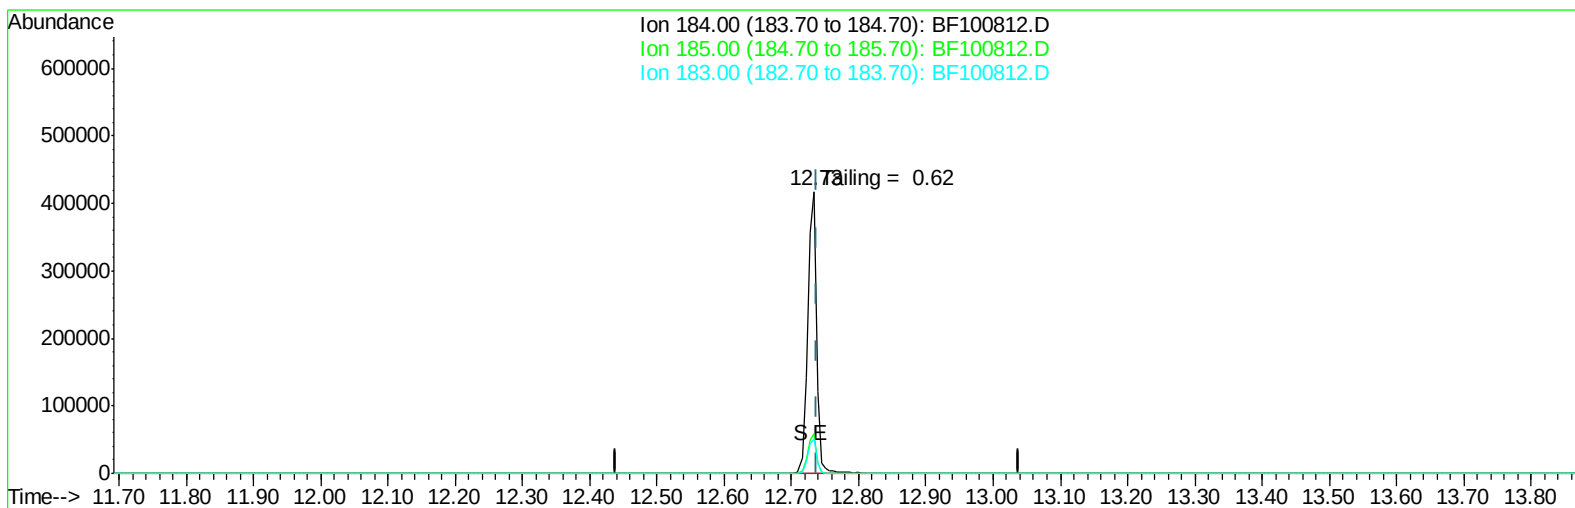

TIC: BF100812.D

(76) Benzidine


12.733min (-0.006) 0.00ng

response 391290

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.89
183.00	11.60	12.26
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA F\Data\BF112217\  
Data File : BF100812.D  
Acq On    : 22 Nov 2017    8:44  
Operator  : SJ/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Nov 26 23:56:18 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

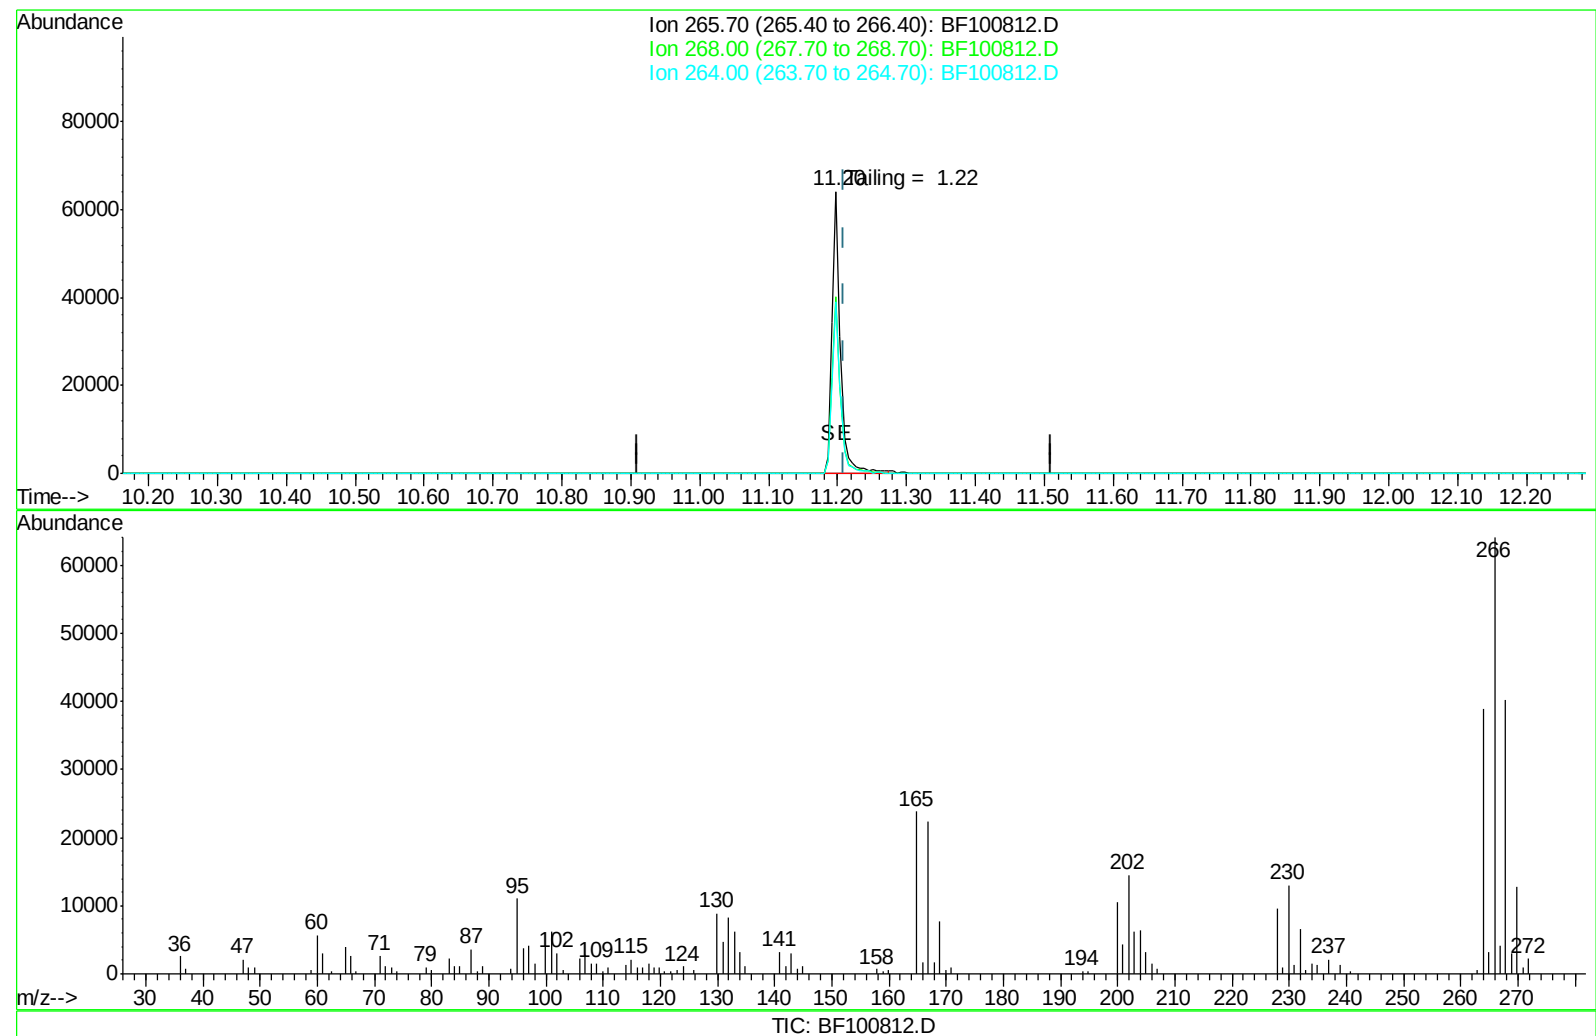

(69) Pentachlorophenol (C)

11.198min (-0.012) 56243.55ng

response 54712

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.85
264.00	61.90	60.80
0.00	0.00	0.00