
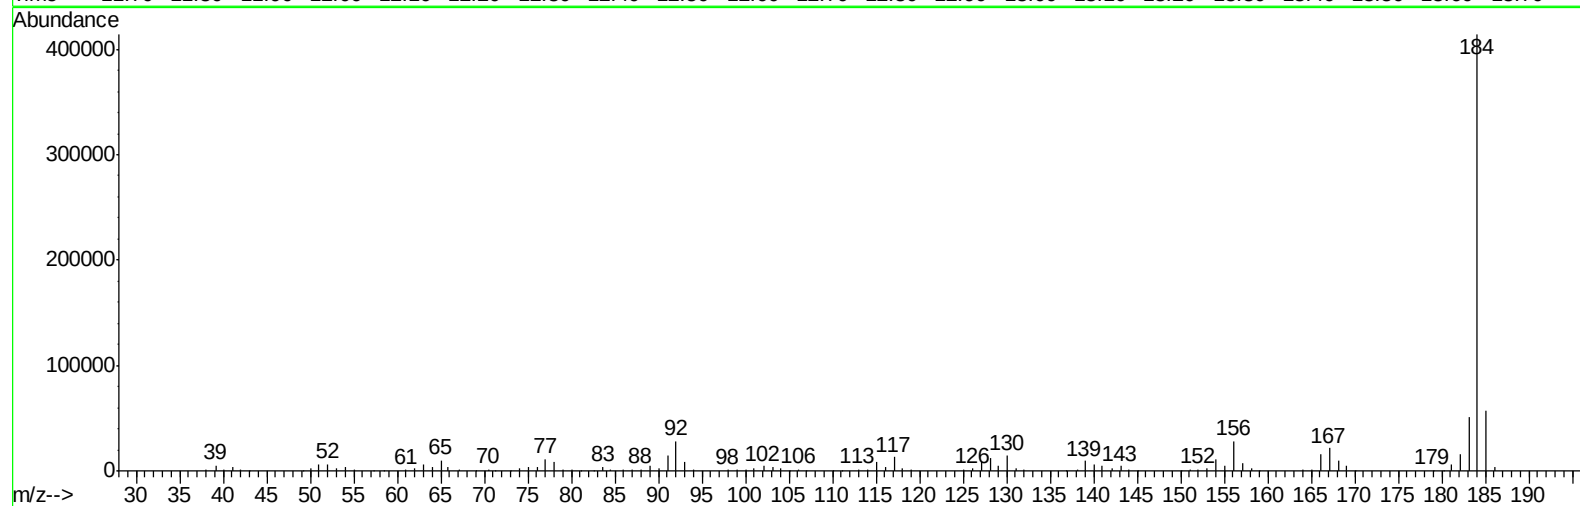


Data Path : Z:\HPCHEM1\BNA F\Data\BF112217\
Data File : BF100828.D
Acq On : 22 Nov 2017 17:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 23:58:32 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

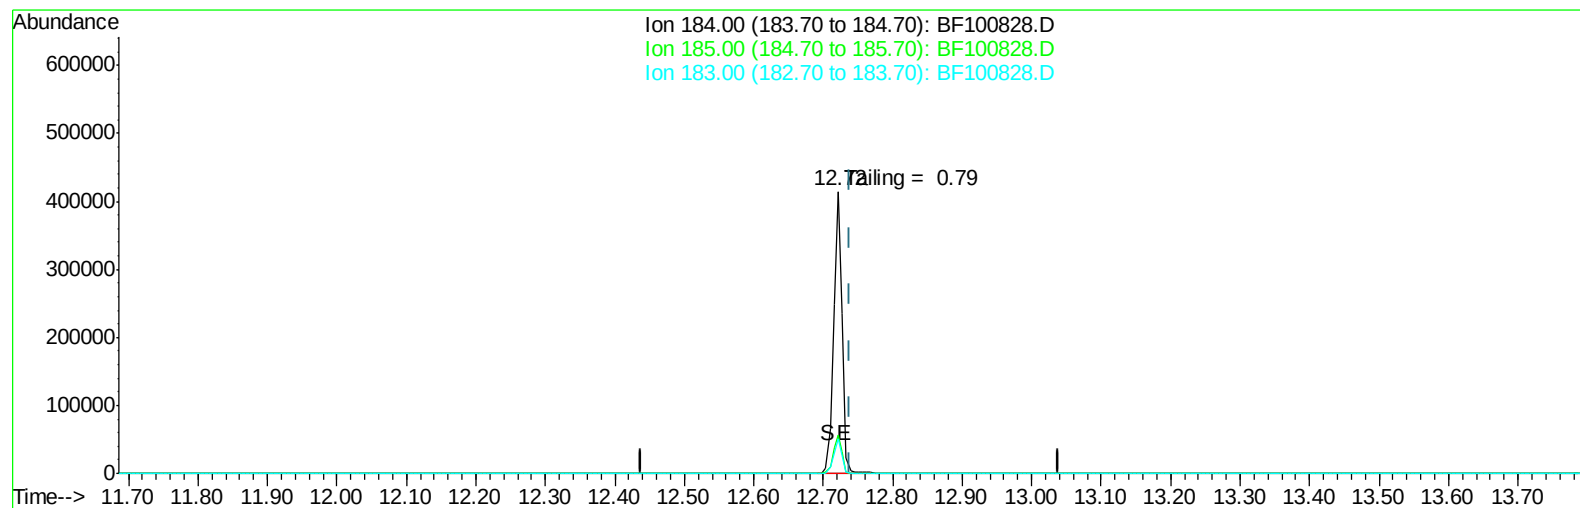

TIC: BF100828.D

(76) Benzidine



12.721min (-0.018) 77398.82ng

response 356460

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.74
183.00	11.60	12.34
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF112217\
Data File : BF100828.D
Acq On : 22 Nov 2017 17:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 23:58:32 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

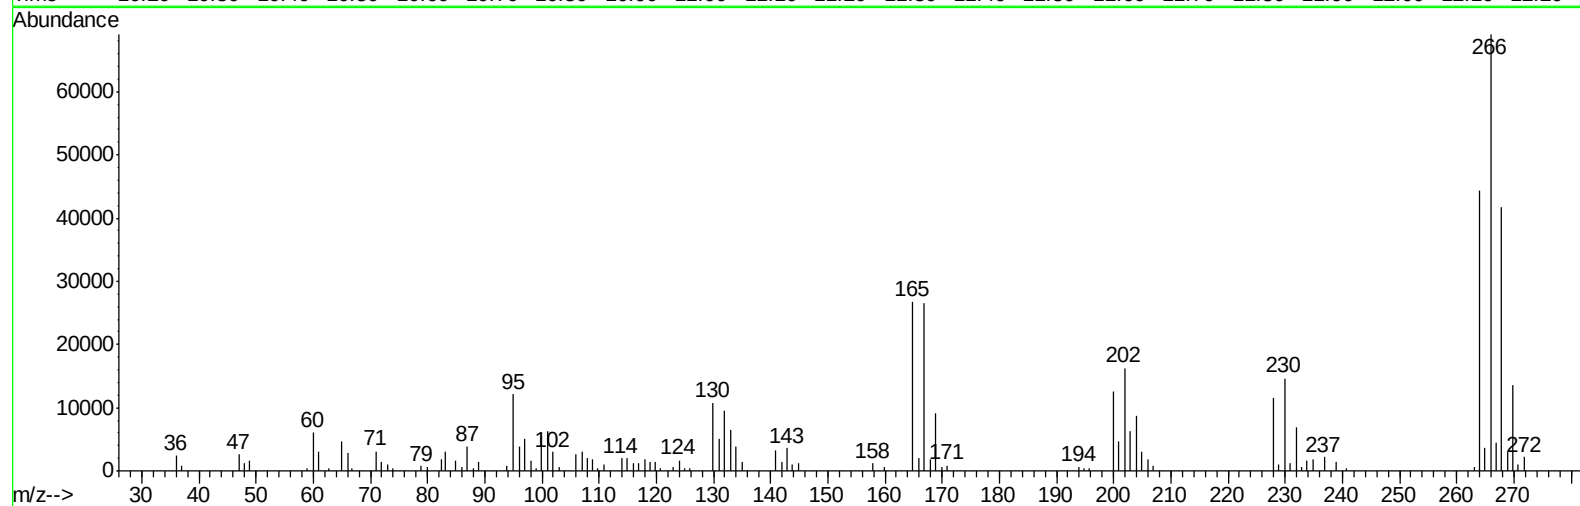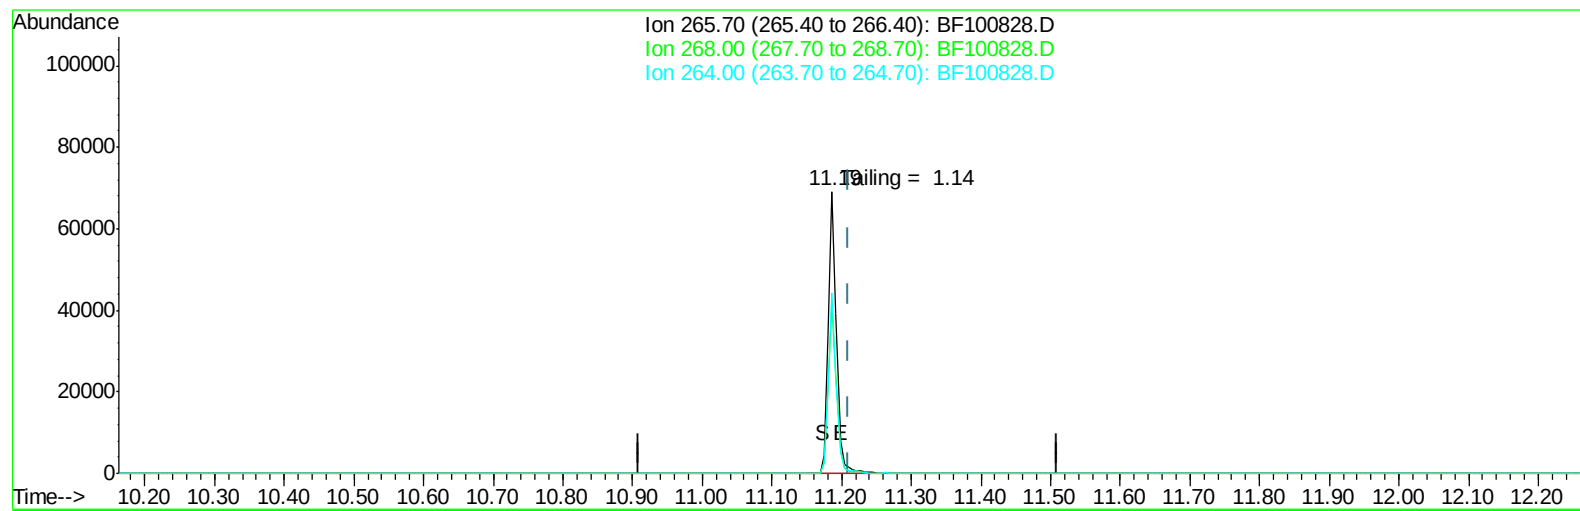

TIC: BF100828.D

(69) Pentachlorophenol (C)

11.186min (-0.024) 0.00ng

response 56978

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.28
264.00	61.90	64.28
0.00	0.00	0.00