

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112217\
 Data File : BF100859.D
 Acq On : 23 Nov 2017 8:01
 Operator : SJ/JU
 Sample : I6541-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 111717-JETT-F-D-B

Quant Time: Nov 24 22:40:32 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 15:22:08 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	69178	20.00	ng	-0.02
21) Naphthalene-d8	8.14	136	262563	20.00	ng	-0.03
38) Acenaphthene-d10	9.90	164	123878	20.00	ng	-0.02
63) Phenanthrene-d10	11.38	188	210131	20.00	ng	-0.02
75) Chrysene-d12	14.02	240	135021	20.00	ng	-0.02
86) Perylene-d12	15.49	264	151847	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	165807	38.42	ng	-0.02
7) Phenol-d6	6.48	99	125233	23.53	ng	-0.03
23) Nitrobenzene-d5	7.42	82	399063	100.48	ng	-0.03
41) 2,4,6-Tribromophenol	10.69	330	105981	83.96	ng	-0.02
44) 2-Fluorobiphenyl	9.22	172	778722	95.72	ng	-0.02
78) Terphenyl-d14	12.97	244	546139	92.94	ng	-0.02


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112217\
Data File : BF100859.D
Acq On : 23 Nov 2017 8:01
Operator : SJ/JU
Sample : I6541-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
111717-JETT-F-D-B

Quant Time: Nov 24 22:40:32 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

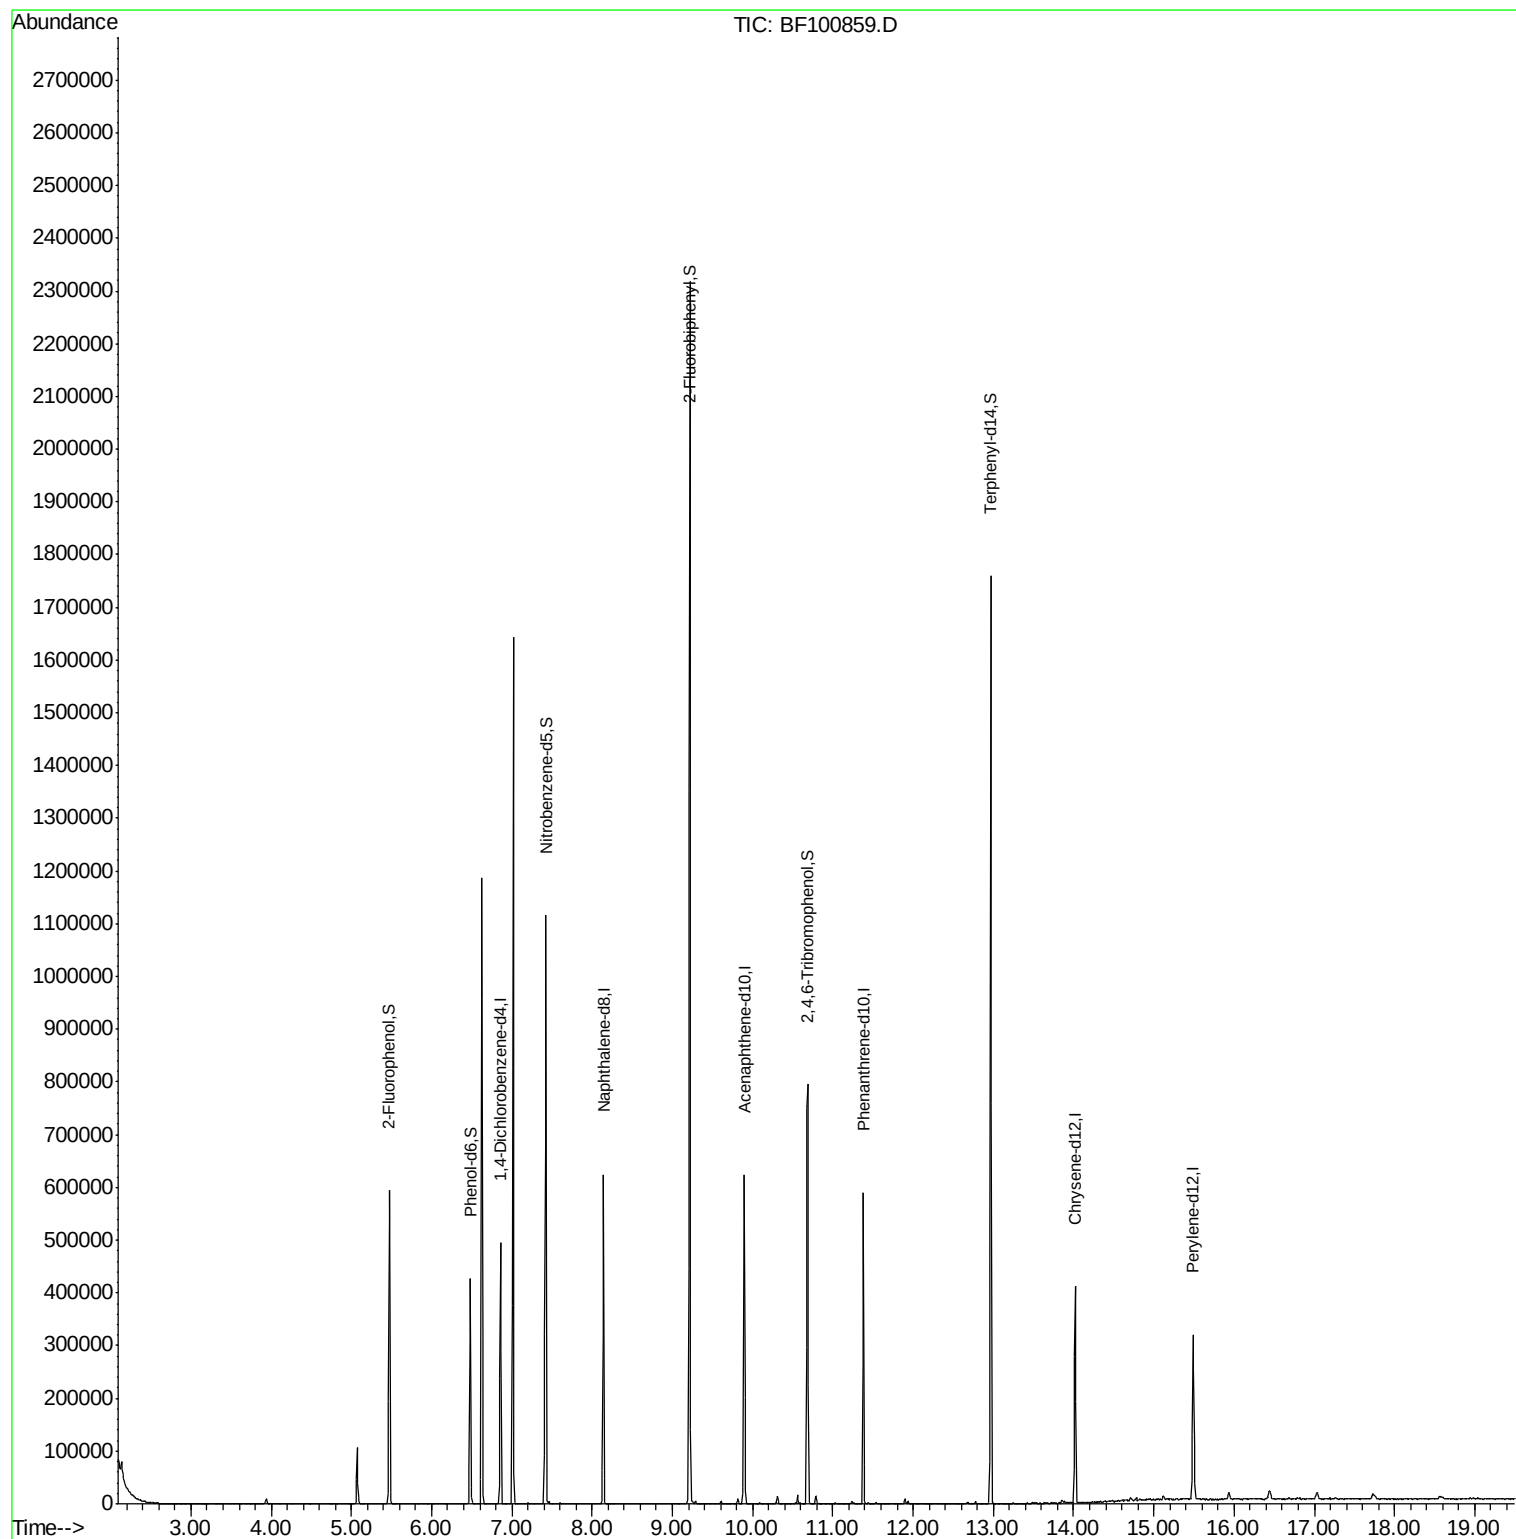

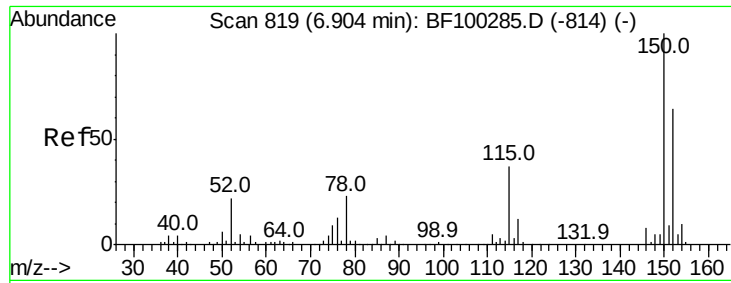


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.86 min Scan# 811
Delta R.T. -0.02 min
Lab File: BF100859.D
Acq: 23 Nov 2017 8:01

Instrument :
BNA_F
ClientSampleId :
111717-JETT-F-D-B

Tot Ion:152 Resp: 69178
Ion Ratio Lower Upper
152 100
150 150.9 124.6 186.8
115 57.4 50.1 75.1

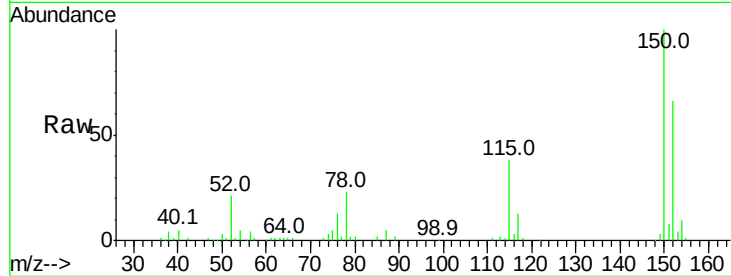


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

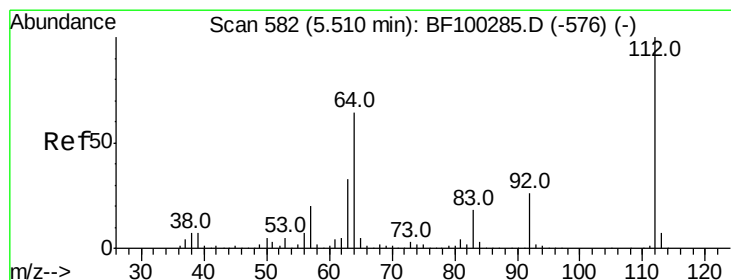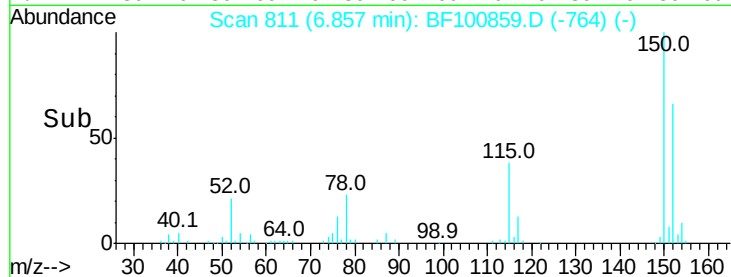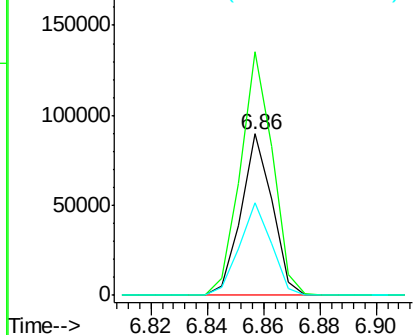



#5


2-Fluorophenol
Concen: 38.421 ng
RT: 5.47 min Scan# 576
Delta R.T. -0.02 min
Lab File: BF100859.D
Acq: 23 Nov 2017 8:01

Tgt Ion:112 Resp: 165807
Ion Ratio Lower Upper
112 100
64 56.3 47.9 71.9
63 28.8 23.7 35.5

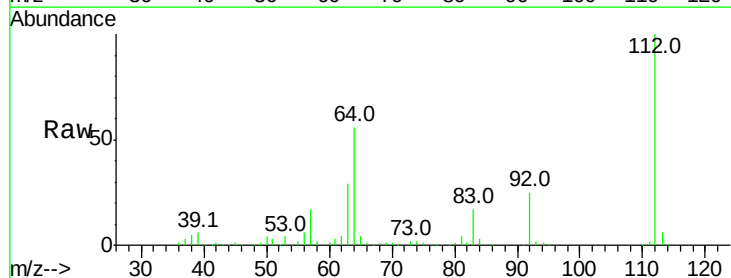

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

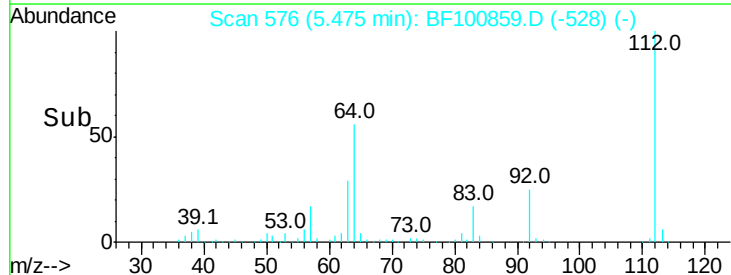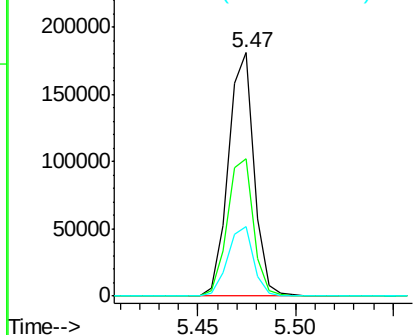

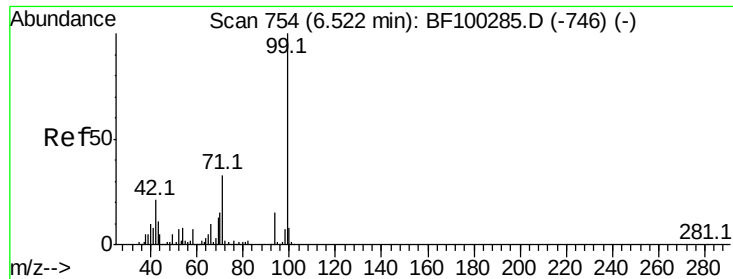

#7

Phenol-d6

Concen: 23.533 ng

RT: 6.48 min Scan# 747

Delta R.T. -0.03 min

Lab File: BF100859.D

Acq: 23 Nov 2017 8:01

Instrument :

BNA_F

ClientSampleId :

111717-JETT-F-D-B


Tot Ion: 99 Resp: 125233

Ion Ratio Lower Upper

99 100

42 17.5 14.5 21.7




71 31.8 25.4 38.0

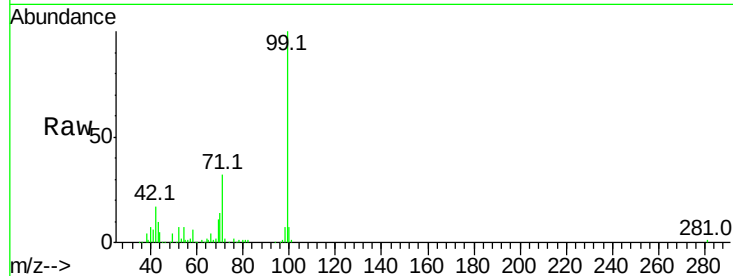

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

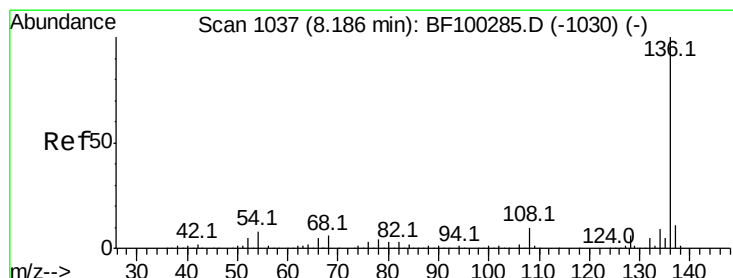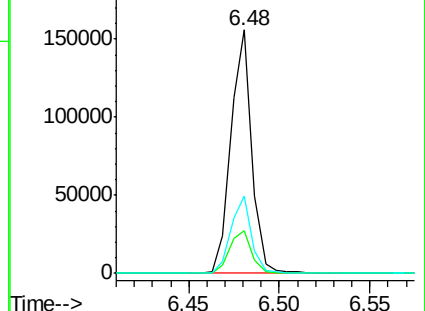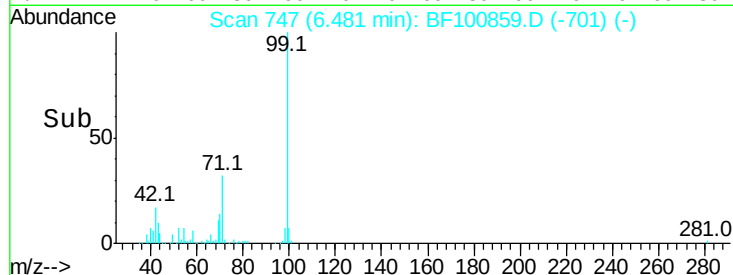

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.14 min Scan# 1029

Delta R.T. -0.03 min

Lab File: BF100859.D

Acq: 23 Nov 2017 8:01

Tgt Ion: 136 Resp: 262563


Ion Ratio Lower Upper

136 100

137 11.3 8.9 13.3

54 7.8 6.6 9.8

68 5.3 5.0 7.4


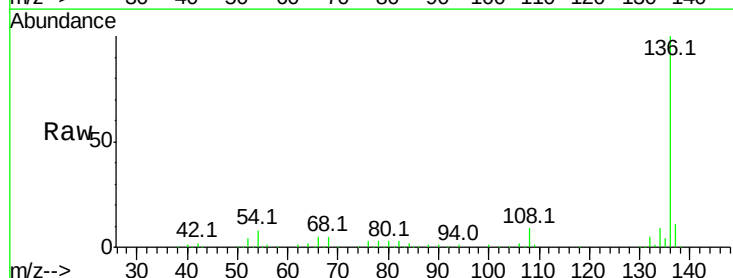



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1



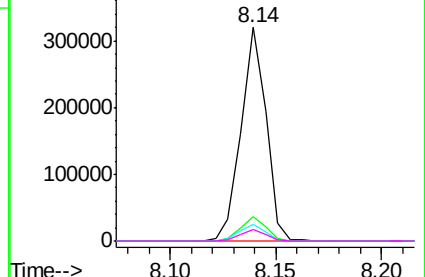
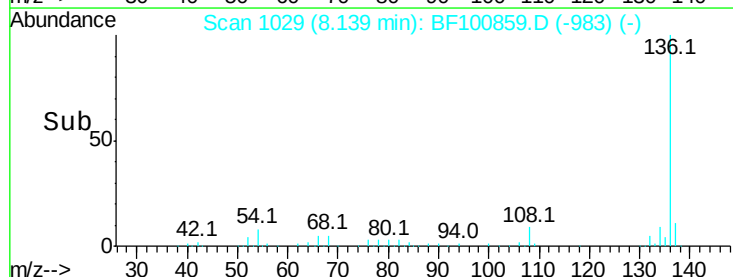


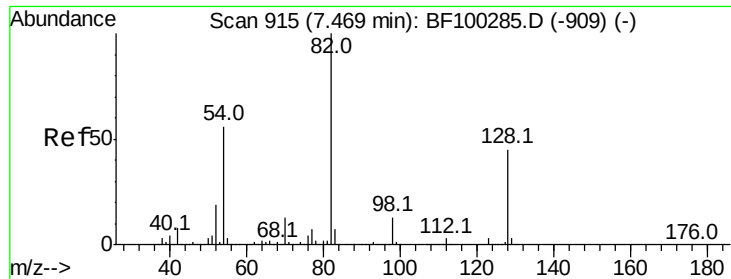

#23
Nitrobenzene-d5
Concen: 100.484 ng
RT: 7.42 min Scan# 907
Delta R.T. -0.03 min
Lab File: BF100859.D
Acq: 23 Nov 2017 8:01




Instrument :
BNA_F
ClientSampleId :
111717-JETT-F-D-B


Tot Ion: 82 Resp: 399063
Ion Ratio Lower Upper
82 100
128 46.2 36.1 54.1
54 54.0 41.4 62.2

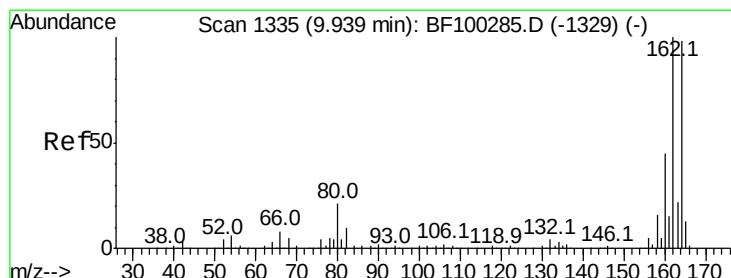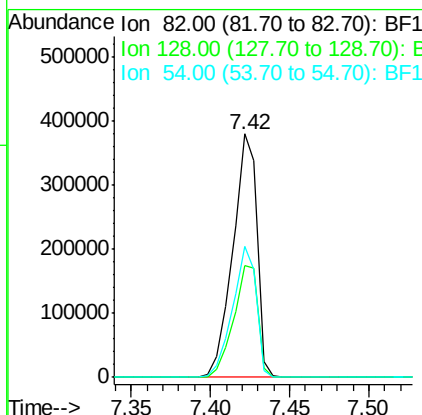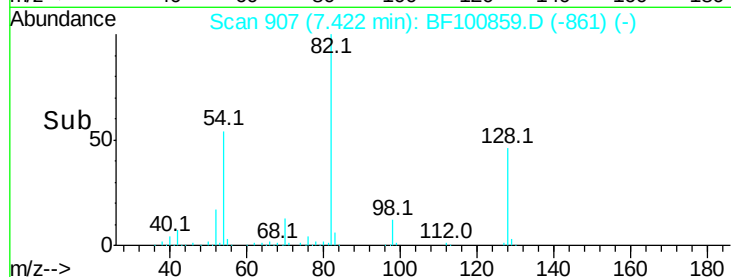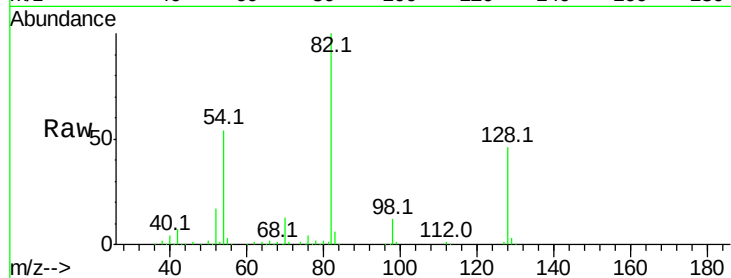

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.90 min Scan# 1328
Delta R.T. -0.02 min
Lab File: BF100859.D
Acq: 23 Nov 2017 8:01

Tgt Ion: 164 Resp: 123878
Ion Ratio Lower Upper
164 100
162 104.2 86.1 129.1
160 47.8 38.3 57.5


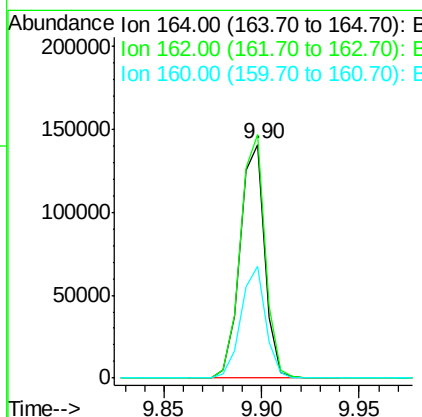
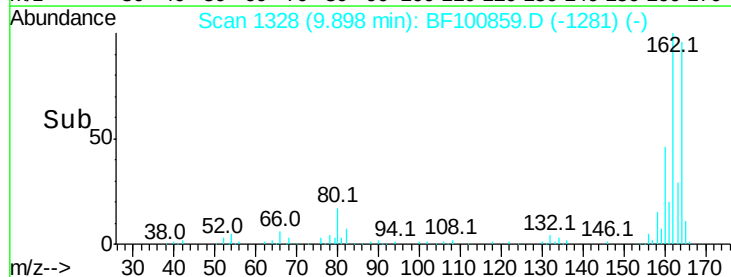
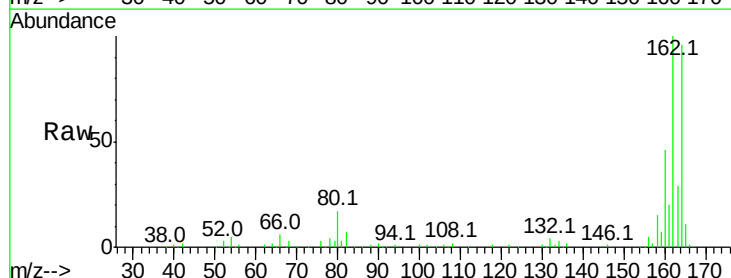


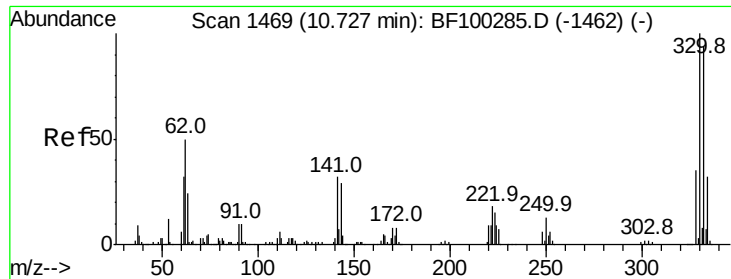

#41
 2,4,6-Tribromophenol
 Concen: 83.958 ng
 RT: 10.69 min Scan# 1462
 Delta R.T. -0.02 min
 Lab File: BF100859.D
 Acq: 23 Nov 2017 8:01




Instrument :
 BNA_F
 ClientSampleId :
 111717-JETT-F-D-B


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.7	77.0	115.6
141	28.9	29.9	44.9#

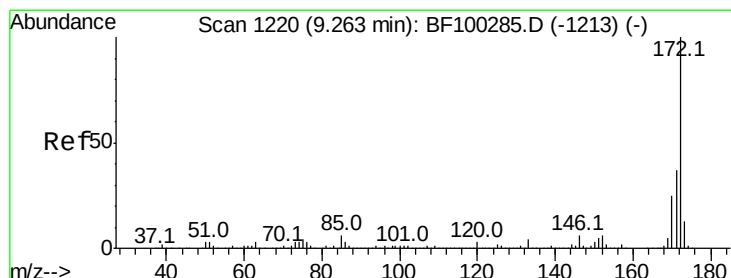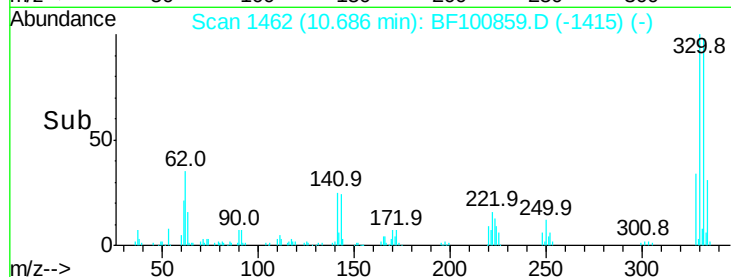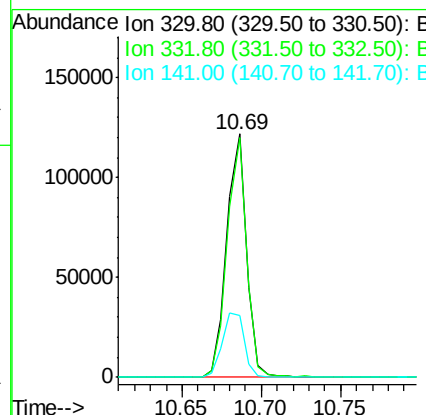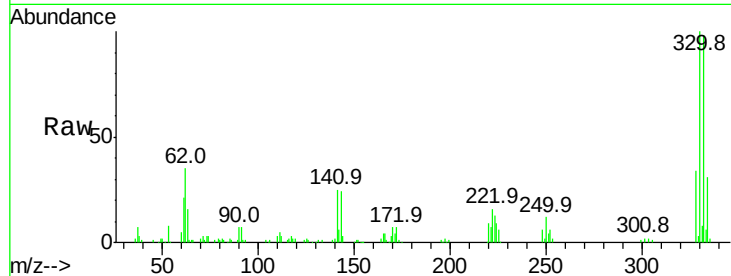

#44
 2-Fluorobiphenyl
 Concen: 95.721 ng
 RT: 9.22 min Scan# 1212
 Delta R.T. -0.02 min
 Lab File: BF100859.D
 Acq: 23 Nov 2017 8:01

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.8	29.7	44.5
170	24.2	19.6	29.4


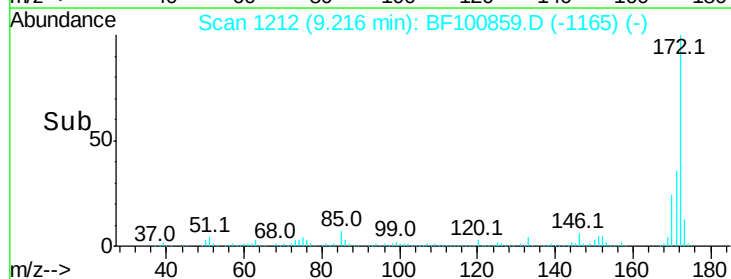
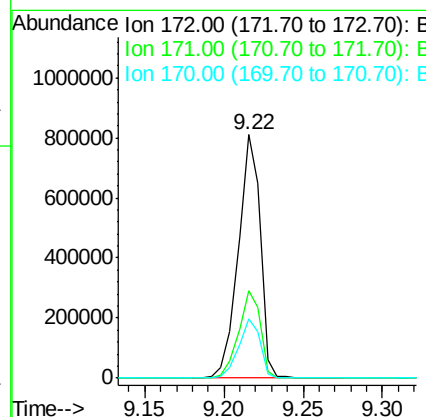
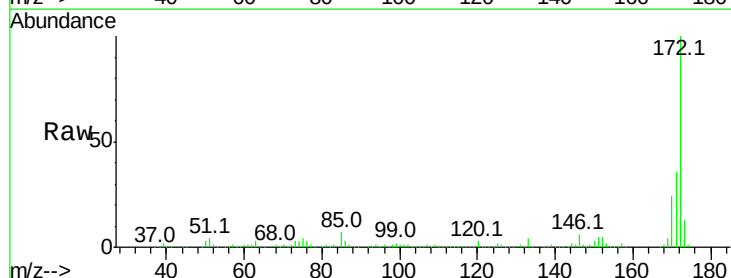


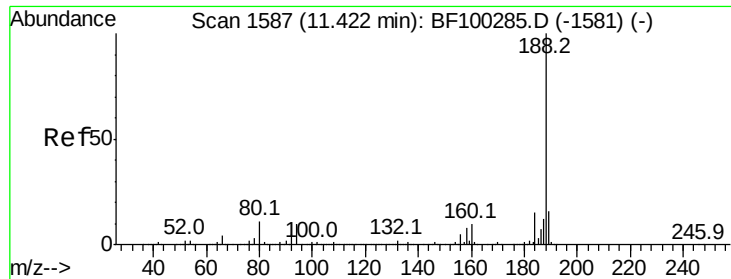

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.38 min Scan# 1580
Delta R.T. -0.02 min
Lab File: BF100859.D
Acq: 23 Nov 2017 8:01




Instrument :
BNA_F
ClientSampleId :
111717-JETT-F-D-B


Tot Ion:188 Resp: 210131
Ion Ratio Lower Upper
188 100
94 9.0 8.5 12.7
80 9.6 9.2 13.8

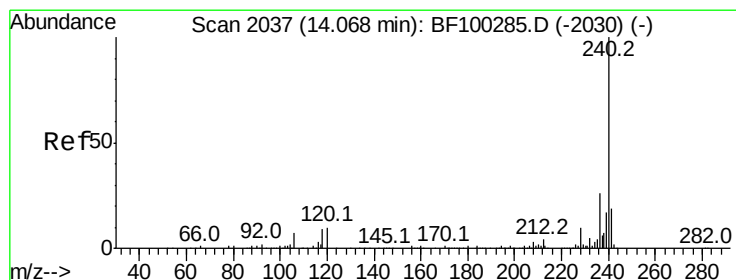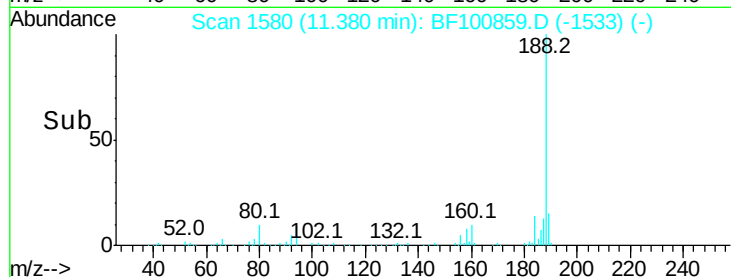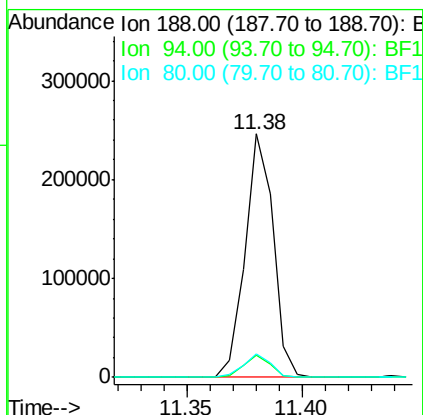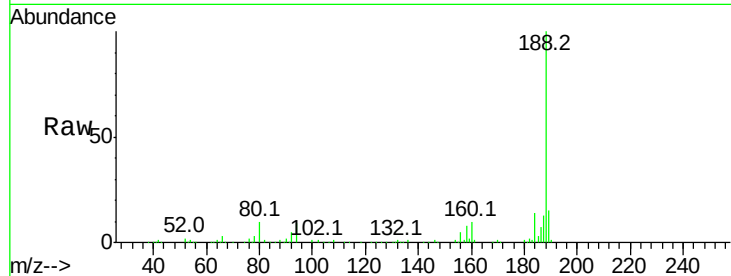

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.02 min Scan# 2029
Delta R.T. -0.02 min
Lab File: BF100859.D
Acq: 23 Nov 2017 8:01

Tgt Ion:240 Resp: 135021
Ion Ratio Lower Upper
240 100
120 9.6 9.5 14.3
236 25.5 20.7 31.1

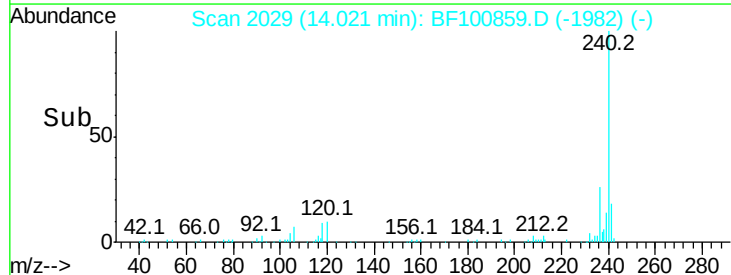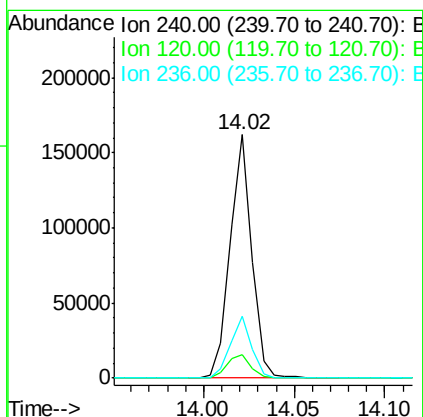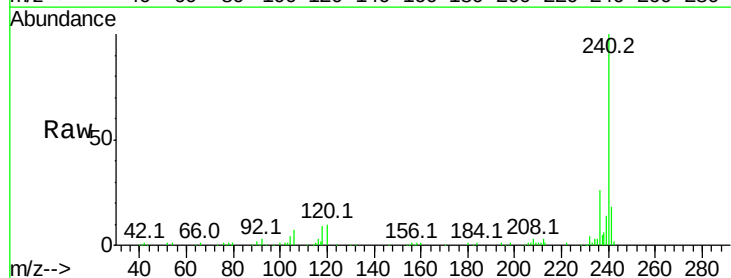

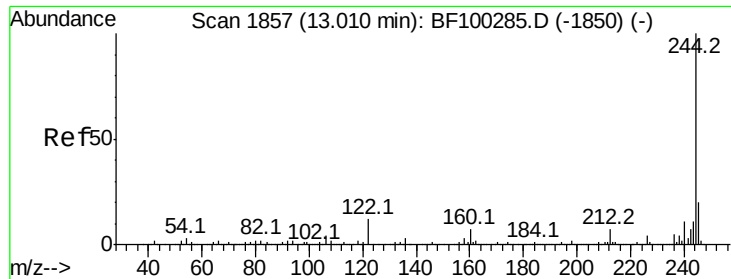

#78

Terphenyl-d14

Concen: 92.939 ng

RT: 12.97 min Scan# 1850

Delta R.T. -0.02 min

Lab File: BF100859.D

Acq: 23 Nov 2017 8:01

Instrument :

BNA_F

ClientSampleId :

111717-JETT-F-D-B


Tot Ion:244 Resp: 546139

Ion Ratio Lower Upper

244 100

212 6.7 5.4 8.0




122 10.7 11.0 16.4#

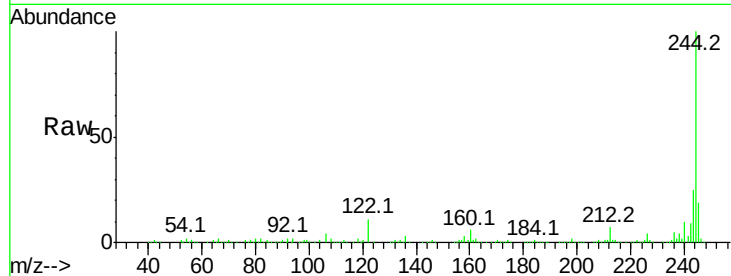

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

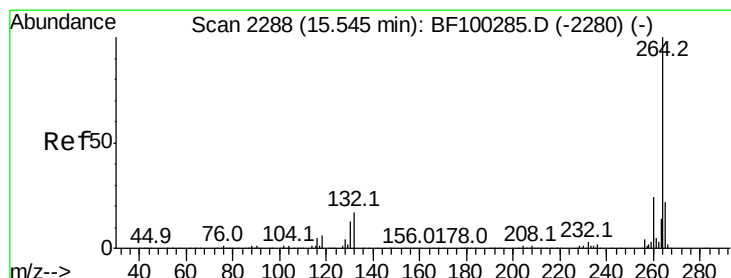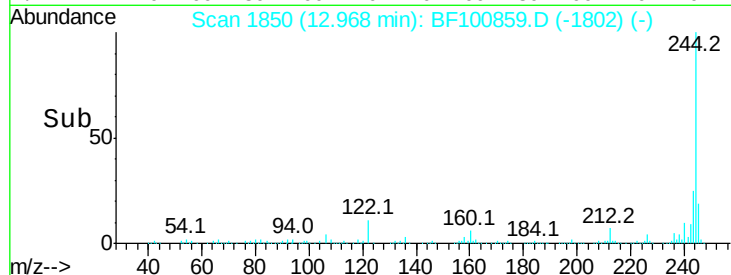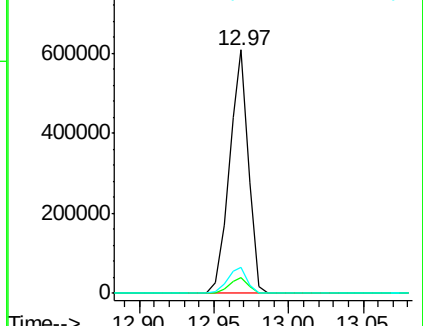

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.49 min Scan# 2279

Delta R.T. -0.02 min

Lab File: BF100859.D

Acq: 23 Nov 2017 8:01


Tgt Ion:264 Resp: 151847

Ion Ratio Lower Upper

264 100

260 23.0 19.2 28.8

265 20.5 17.5 26.3

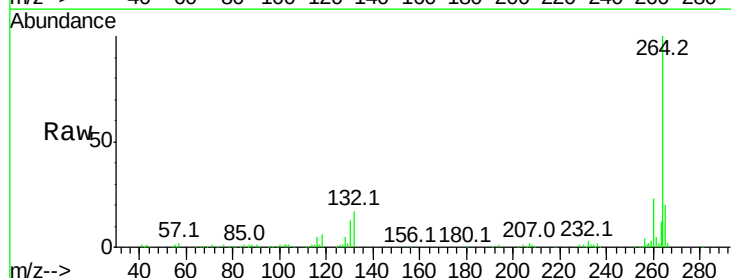

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

