

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112217\
 Data File : BF100846.D
 Acq On : 23 Nov 2017 1:41
 Operator : SJ/JU
 Sample : I6548-08 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SAU-4-E(0-1)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.069	505	507	512	rVB	9102	8946	1.50%	0.156%
2	5.469	572	575	583	rBB	140607	119703	20.02%	2.086%
3	6.481	744	747	752	rBV	153357	125883	21.06%	2.194%
4	6.622	768	771	775	rBV	152950	132387	22.15%	2.307%
5	6.857	807	811	815	rBB	538055	430921	72.09%	7.509%
6	7.010	834	837	841	rBB	126547	105556	17.66%	1.839%
7	7.416	903	906	910	rBV	101442	77679	12.99%	1.354%
8	8.139	1025	1029	1033	rBV	671909	565675	94.63%	9.857%
9	9.210	1208	1211	1215	rBV	199182	159829	26.74%	2.785%
10	9.604	1276	1278	1281	rBB	8665	7052	1.18%	0.123%
11	9.816	1307	1314	1320	rBV3	9075	15974	2.67%	0.278%
12	9.898	1324	1328	1331	rVV	704876	597779	100.00%	10.417%
13	9.927	1331	1333	1336	rVB	10819	8183	1.37%	0.143%
14	10.304	1393	1397	1403	rVB2	9830	16406	2.74%	0.286%
15	10.445	1417	1421	1424	rBB	8658	7446	1.25%	0.130%
16	10.680	1458	1461	1465	rVB	92286	72202	12.08%	1.258%
17	10.792	1477	1480	1484	rBB2	5838	7812	1.31%	0.136%
18	11.280	1558	1563	1566	rVB3	5394	6727	1.13%	0.117%
19	11.386	1577	1581	1583	rBV	600708	573720	95.98%	9.997%
20	11.404	1583	1584	1588	rVB	136705	96298	16.11%	1.678%
21	11.457	1591	1593	1596	rVB	26668	20544	3.44%	0.358%
22	11.674	1625	1630	1633	rVB3	5271	7739	1.29%	0.135%
23	11.886	1663	1666	1668	rBV	23790	24159	4.04%	0.421%
24	11.910	1668	1670	1673	rVV	33600	26209	4.38%	0.457%
25	11.957	1676	1678	1681	rVV	10618	9223	1.54%	0.161%
26	11.998	1681	1685	1687	rVV2	38611	42585	7.12%	0.742%
27	12.016	1687	1688	1691	rVB	20114	14241	2.38%	0.248%
28	12.180	1712	1716	1718	rBV	14836	12801	2.14%	0.223%
29	12.204	1718	1720	1724	rVB2	9319	8058	1.35%	0.140%
30	12.433	1753	1759	1761	rBV	17788	18491	3.09%	0.322%
31	12.468	1761	1765	1767	rVV4	12559	17130	2.87%	0.298%
32	12.515	1771	1773	1778	rVB3	12170	14746	2.47%	0.257%
33	12.598	1783	1787	1790	rBV	195746	177414	29.68%	3.092%
34	12.827	1820	1826	1832	rBV	180131	201121	33.64%	3.505%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112217\
 Data File : BF100846.D
 Acq On : 23 Nov 2017 1:41
 Operator : SJ/JU
 Sample : I6548-08 10X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SAU-4-E(0-1)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.874	1832	1834	1838	rVB2	9158	11353	1.90%	0.198%
36	12.963	1846	1849	1852	rBV	142645	101807	17.03%	1.774%
37	13.039	1856	1862	1866	rBV4	16579	26527	4.44%	0.462%
38	13.127	1874	1877	1878	rBV2	12252	10599	1.77%	0.185%
39	13.151	1878	1881	1884	rVB	27731	29919	5.01%	0.521%
40	13.215	1890	1892	1895	rBV2	15283	12673	2.12%	0.221%
41	13.257	1895	1899	1901	rBV2	20410	20281	3.39%	0.353%
42	13.351	1912	1915	1918	rBV2	12130	13288	2.22%	0.232%
43	13.380	1918	1920	1923	rVB	13539	12088	2.02%	0.211%
44	13.662	1965	1968	1971	rVB	14821	15007	2.51%	0.262%
45	13.768	1982	1986	1989	rBV3	13627	17919	3.00%	0.312%
46	13.798	1989	1991	1993	rVV	16019	13774	2.30%	0.240%
47	13.821	1993	1995	1997	rVV2	11118	12942	2.17%	0.226%
48	13.862	1998	2002	2004	rVV2	16896	27032	4.52%	0.471%
49	13.886	2004	2006	2012	rVB	15434	14188	2.37%	0.247%
50	13.933	2012	2014	2017	rBV4	6118	6910	1.16%	0.120%
51	14.021	2021	2029	2032	rBV2	497635	532004	89.00%	9.270%
52	14.045	2032	2033	2039	rVB	82624	64582	10.80%	1.125%
53	14.127	2044	2047	2050	rBV2	16547	15442	2.58%	0.269%
54	14.409	2092	2095	2098	rVB	19639	16691	2.79%	0.291%
55	14.439	2098	2100	2103	rBV	15662	16680	2.79%	0.291%
56	14.533	2113	2116	2118	rBV3	16145	16831	2.82%	0.293%
57	15.062	2202	2206	2213	rBV	80953	154030	25.77%	2.684%
58	15.168	2222	2224	2229	rVB	14947	18070	3.02%	0.315%
59	15.368	2254	2258	2263	rVB	48585	63818	10.68%	1.112%
60	15.427	2264	2268	2274	rBV	70293	85676	14.33%	1.493%
61	15.492	2274	2279	2283	rBV	353978	463772	77.58%	8.081%
62	15.627	2300	2302	2309	rBV8	13106	22142	3.70%	0.386%
63	16.192	2394	2398	2403	rVB7	24154	42162	7.05%	0.735%
64	16.962	2524	2529	2538	rVB3	31874	72409	12.11%	1.262%
65	17.209	2568	2571	2578	rVB9	18024	34230	5.73%	0.596%
66	17.409	2601	2605	2611	rBV2	21912	43275	7.24%	0.754%


Sum of corrected areas: 5738760

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112217\
Data File : BF100846.D
Acq On : 23 Nov 2017 1:41
Operator : SJ/JU
Sample : I6548-08 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SAU-4-E(0-1)

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

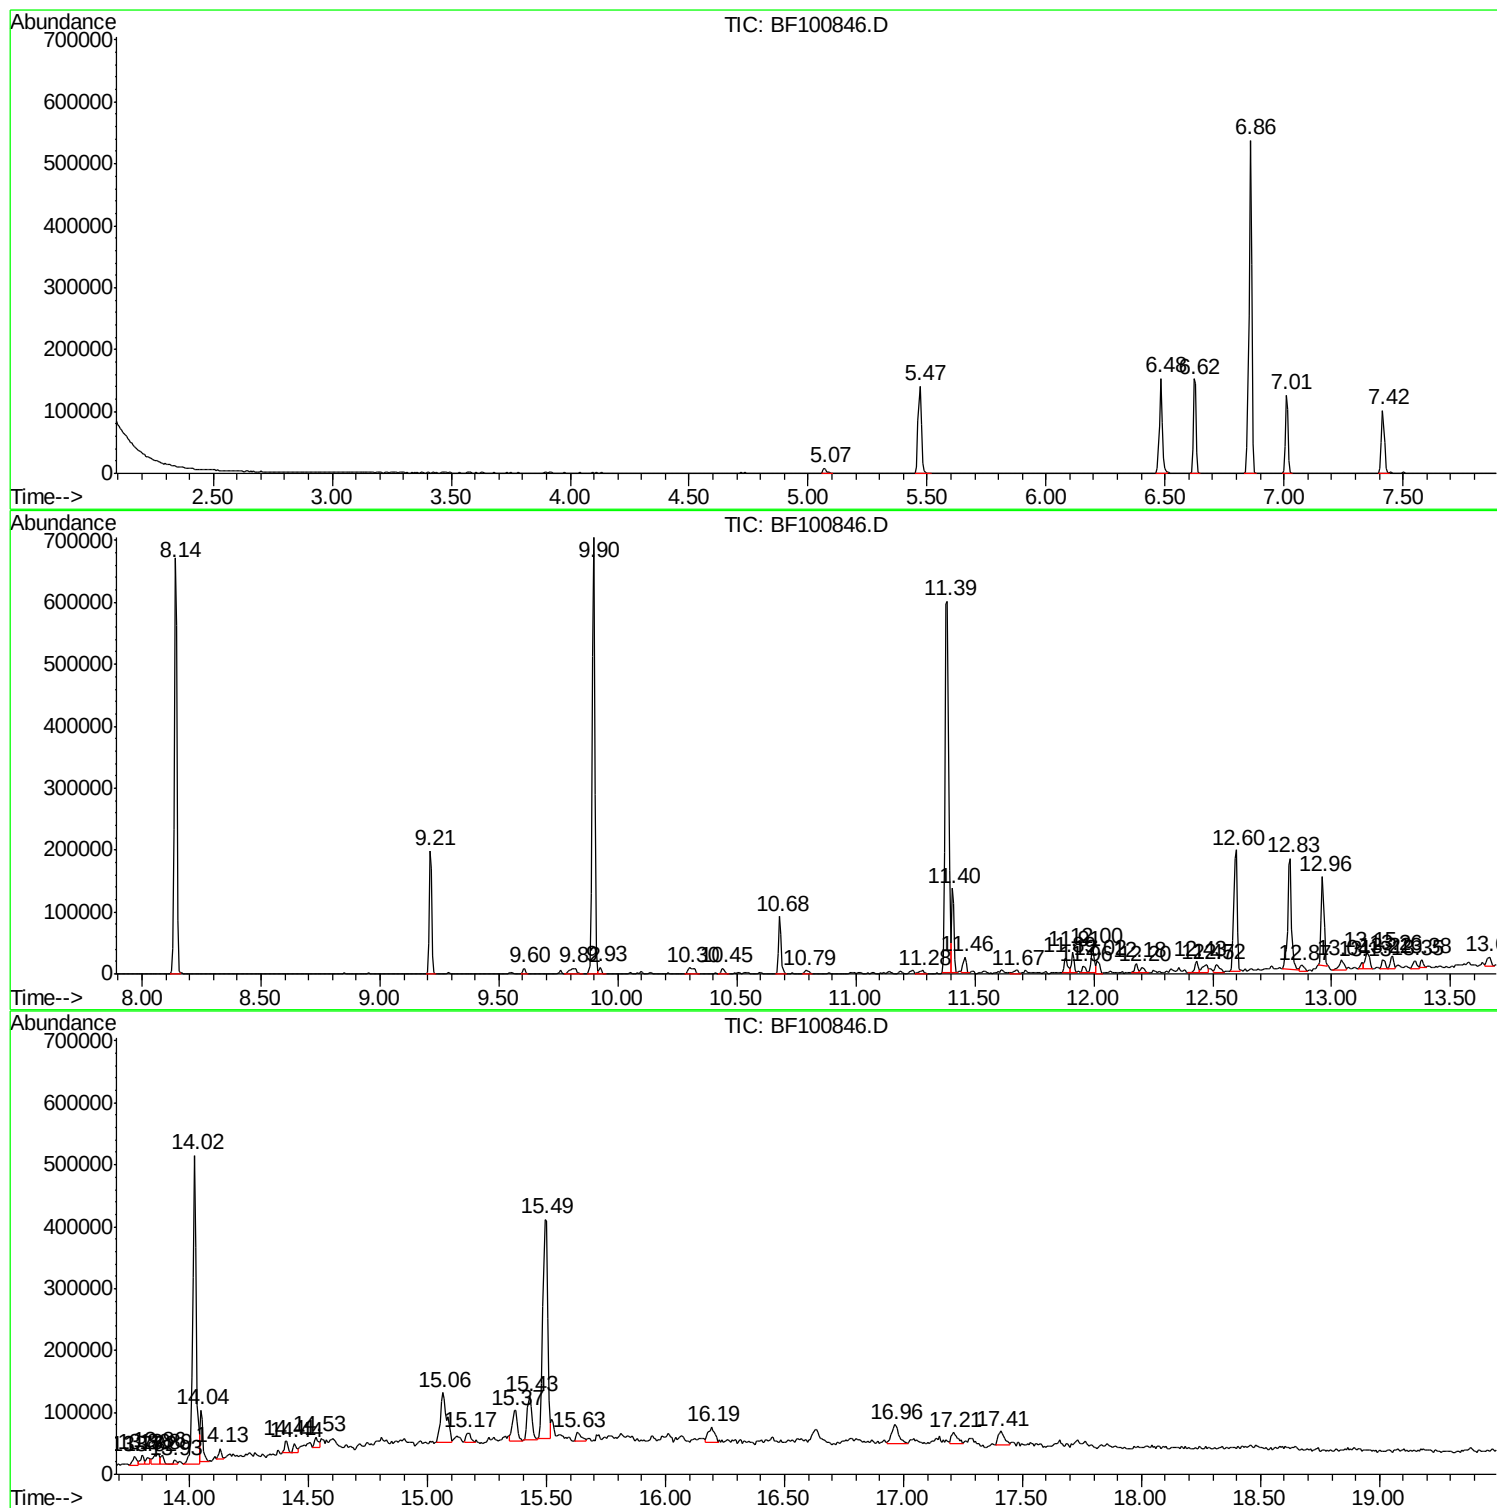

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112217\
Data File : BF100846.D
Acq On : 23 Nov 2017 1:41
Operator : SJ/JU
Sample : I6548-08 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SAU-4-E(0-1)










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.62 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.62	6.14 ng	132387	1,4-Dichlorobenzene-d4	6.86

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,3-Cyclopentanedione, 2-chloro-	132	C5H5ClO2	014203-19-1	23
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		5-Aminoindole	132	C8H8N2	005192-03-0	10
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	10

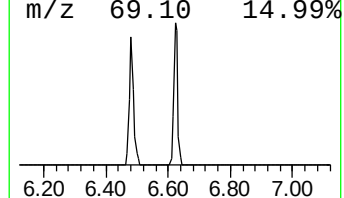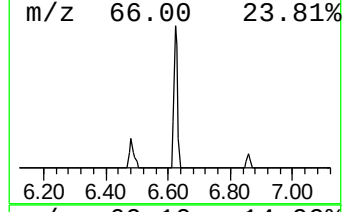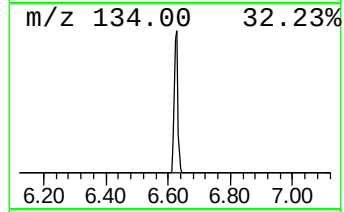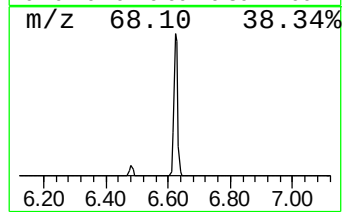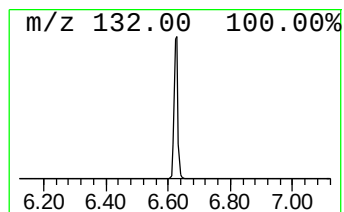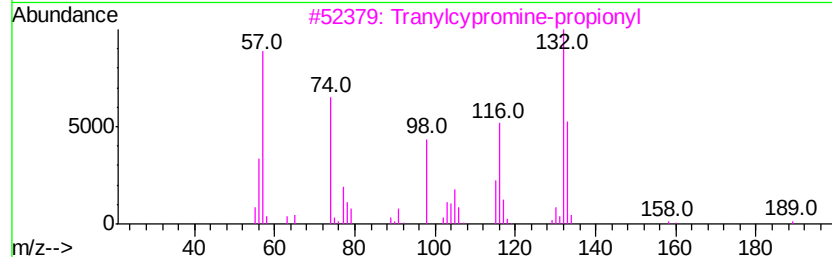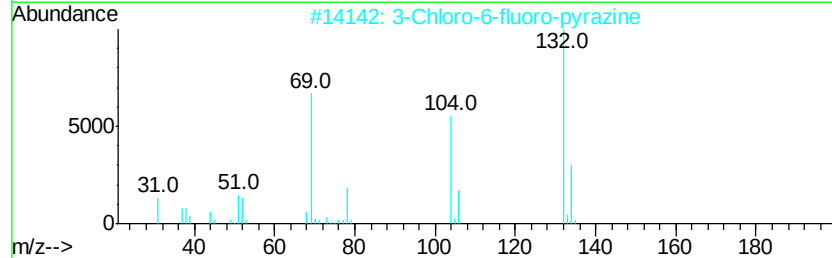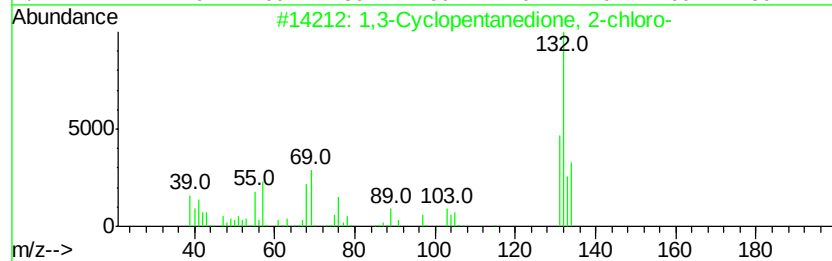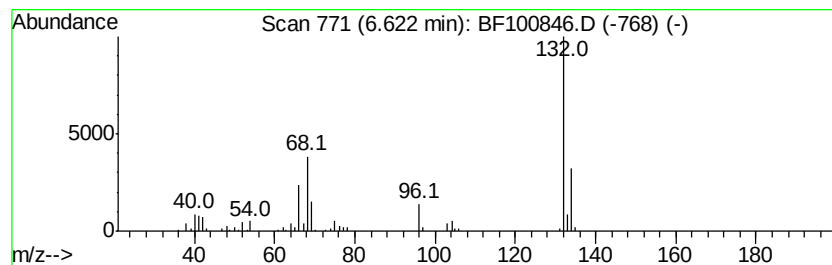

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112217\
Data File : BF100846.D
Acq On : 23 Nov 2017 1:41
Operator : SJ/JU
Sample : I6548-08 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SAU-4-E(0-1)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.62	6.62	6.1	ng	132387	1	6.86	430921	20.0