

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112217\  
 Data File : BF100849.D  
 Acq On : 23 Nov 2017 3:01  
 Operator : SJ/JU  
 Sample : I6548-03 5X  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 SAU-1-E(3-4)

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0  
 Filtering: 5  
 Min Area: 3 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF110817.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

| peak # | R.T. min | first scan | max scan | last scan | PK TY | peak height | corr. area | corr. % max. | % of total |
|--------|----------|------------|----------|-----------|-------|-------------|------------|--------------|------------|
| 1      | 5.069    | 504        | 507      | 514       | rBB   | 29080       | 29833      | 4.82%        | 0.325%     |
| 2      | 5.469    | 571        | 575      | 583       | rBB   | 388292      | 326676     | 52.82%       | 3.563%     |
| 3      | 6.481    | 743        | 747      | 756       | rBV   | 415711      | 343302     | 55.51%       | 3.744%     |
| 4      | 6.622    | 768        | 771      | 775       | rBV   | 396650      | 356349     | 57.62%       | 3.886%     |
| 5      | 6.857    | 807        | 811      | 815       | rBV   | 534264      | 432557     | 69.95%       | 4.717%     |
| 6      | 7.010    | 834        | 837      | 841       | rBV   | 323348      | 292430     | 47.29%       | 3.189%     |
| 7      | 7.416    | 902        | 906      | 910       | rBV   | 271191      | 213192     | 34.47%       | 2.325%     |
| 8      | 8.139    | 1025       | 1029     | 1032      | rBV   | 658630      | 563827     | 91.17%       | 6.149%     |
| 9      | 9.216    | 1208       | 1212     | 1215      | rBV   | 531446      | 425925     | 68.87%       | 4.645%     |
| 10     | 9.610    | 1275       | 1279     | 1284      | rBB2  | 29639       | 30620      | 4.95%        | 0.334%     |
| 11     | 9.757    | 1301       | 1304     | 1307      | rBV   | 55520       | 41413      | 6.70%        | 0.452%     |
| 12     | 9.816    | 1307       | 1314     | 1319      | rVB2  | 15005       | 20968      | 3.39%        | 0.229%     |
| 13     | 9.898    | 1324       | 1328     | 1331      | rVV   | 736786      | 593420     | 95.96%       | 6.471%     |
| 14     | 9.928    | 1331       | 1333     | 1336      | rVB   | 10918       | 7612       | 1.23%        | 0.083%     |
| 15     | 10.304   | 1390       | 1397     | 1398      | rBV2  | 8422        | 11565      | 1.87%        | 0.126%     |
| 16     | 10.316   | 1398       | 1399     | 1402      | rVB   | 16558       | 11118      | 1.80%        | 0.121%     |
| 17     | 10.439   | 1418       | 1420     | 1428      | rVB   | 5941        | 8597       | 1.39%        | 0.094%     |
| 18     | 10.539   | 1433       | 1437     | 1443      | rBB2  | 4711        | 8444       | 1.37%        | 0.092%     |
| 19     | 10.681   | 1458       | 1461     | 1465      | rBV   | 230573      | 183533     | 29.68%       | 2.002%     |
| 20     | 10.792   | 1476       | 1480     | 1481      | rBV   | 16233       | 12522      | 2.02%        | 0.137%     |
| 21     | 11.186   | 1544       | 1547     | 1552      | rVB2  | 8856        | 7692       | 1.24%        | 0.084%     |
| 22     | 11.239   | 1552       | 1556     | 1558      | rVV2  | 14167       | 13198      | 2.13%        | 0.144%     |
| 23     | 11.280   | 1558       | 1563     | 1567      | rVB3  | 5594        | 8426       | 1.36%        | 0.092%     |
| 24     | 11.386   | 1577       | 1581     | 1583      | rBV   | 611114      | 546111     | 88.31%       | 5.956%     |
| 25     | 11.404   | 1583       | 1584     | 1588      | rVV   | 134782      | 102298     | 16.54%       | 1.116%     |
| 26     | 11.457   | 1591       | 1593     | 1596      | rVB   | 38227       | 28653      | 4.63%        | 0.312%     |
| 27     | 11.616   | 1614       | 1620     | 1623      | rBV3  | 7196        | 11888      | 1.92%        | 0.130%     |
| 28     | 11.669   | 1626       | 1629     | 1634      | rVB3  | 13034       | 18826      | 3.04%        | 0.205%     |
| 29     | 11.886   | 1663       | 1666     | 1668      | rBV   | 26133       | 27676      | 4.48%        | 0.302%     |
| 30     | 11.910   | 1668       | 1670     | 1674      | rVV   | 38842       | 32547      | 5.26%        | 0.355%     |
| 31     | 11.957   | 1676       | 1678     | 1681      | rVB   | 15376       | 12648      | 2.05%        | 0.138%     |
| 32     | 11.992   | 1681       | 1684     | 1687      | rBV2  | 36842       | 44646      | 7.22%        | 0.487%     |
| 33     | 12.016   | 1687       | 1688     | 1692      | rVB   | 25910       | 19494      | 3.15%        | 0.213%     |
| 34     | 12.075   | 1695       | 1698     | 1700      | rBV   | 11529       | 10386      | 1.68%        | 0.113%     |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF112217\  
 Data File : BF100849.D  
 Acq On : 23 Nov 2017 3:01  
 Operator : SJ/JU  
 Sample : I6548-03 5X  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 SAU-1-E(3-4)

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON  
 Sampling : 1  
 Start Thrs: 0.2  
 Stop Thrs : 0

Filtering: 5  
 Min Area: 3 % of largest Peak  
 Max Peaks: 100  
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF110817.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

|    |        |      |      |      |      |        |        |         |        |
|----|--------|------|------|------|------|--------|--------|---------|--------|
| 35 | 12.180 | 1711 | 1716 | 1718 | rVB  | 22293  | 20976  | 3.39%   | 0.229% |
| 36 | 12.204 | 1718 | 1720 | 1725 | rVB2 | 12806  | 11847  | 1.92%   | 0.129% |
| 37 | 12.327 | 1739 | 1741 | 1744 | rVB2 | 14173  | 10346  | 1.67%   | 0.113% |
| 38 | 12.357 | 1744 | 1746 | 1748 | rBV2 | 11327  | 8457   | 1.37%   | 0.092% |
| 39 | 12.433 | 1753 | 1759 | 1762 | rBV  | 32053  | 35539  | 5.75%   | 0.388% |
| 40 | 12.463 | 1762 | 1764 | 1767 | rVV3 | 22296  | 26492  | 4.28%   | 0.289% |
| 41 | 12.492 | 1767 | 1769 | 1771 | rVV2 | 11700  | 9798   | 1.58%   | 0.107% |
| 42 | 12.522 | 1771 | 1774 | 1778 | rVB2 | 23329  | 25674  | 4.15%   | 0.280% |
| 43 | 12.598 | 1783 | 1787 | 1790 | rBV  | 291977 | 244122 | 39.48%  | 2.662% |
| 44 | 12.692 | 1800 | 1803 | 1805 | rBV  | 21593  | 19370  | 3.13%   | 0.211% |
| 45 | 12.827 | 1820 | 1826 | 1831 | rBV  | 312575 | 311377 | 50.35%  | 3.396% |
| 46 | 12.874 | 1831 | 1834 | 1838 | rVB2 | 17114  | 23426  | 3.79%   | 0.255% |
| 47 | 12.963 | 1846 | 1849 | 1852 | rBV  | 353926 | 275909 | 44.62%  | 3.009% |
| 48 | 13.045 | 1857 | 1863 | 1867 | rBV2 | 29240  | 51643  | 8.35%   | 0.563% |
| 49 | 13.098 | 1870 | 1872 | 1874 | rBV3 | 9384   | 9251   | 1.50%   | 0.101% |
| 50 | 13.127 | 1874 | 1877 | 1879 | rBV3 | 22980  | 29947  | 4.84%   | 0.327% |
| 51 | 13.151 | 1879 | 1881 | 1884 | rVB  | 31527  | 26757  | 4.33%   | 0.292% |
| 52 | 13.186 | 1884 | 1887 | 1890 | rBV3 | 10193  | 12650  | 2.05%   | 0.138% |
| 53 | 13.257 | 1895 | 1899 | 1902 | rBV2 | 45277  | 45225  | 7.31%   | 0.493% |
| 54 | 13.322 | 1906 | 1910 | 1912 | rBV2 | 17813  | 21000  | 3.40%   | 0.229% |
| 55 | 13.351 | 1912 | 1915 | 1917 | rVB  | 32189  | 28958  | 4.68%   | 0.316% |
| 56 | 13.380 | 1917 | 1920 | 1923 | rBV  | 29476  | 25718  | 4.16%   | 0.280% |
| 57 | 13.533 | 1942 | 1946 | 1948 | rBV2 | 13310  | 18426  | 2.98%   | 0.201% |
| 58 | 13.657 | 1965 | 1967 | 1972 | rVB  | 41757  | 41247  | 6.67%   | 0.450% |
| 59 | 13.721 | 1976 | 1978 | 1981 | rVV2 | 12443  | 11152  | 1.80%   | 0.122% |
| 60 | 13.769 | 1981 | 1986 | 1989 | rVV3 | 26673  | 45233  | 7.31%   | 0.493% |
| 61 | 13.798 | 1989 | 1991 | 1993 | rVV  | 30340  | 29550  | 4.78%   | 0.322% |
| 62 | 13.821 | 1993 | 1995 | 1997 | rVV  | 29179  | 31182  | 5.04%   | 0.340% |
| 63 | 13.869 | 1999 | 2003 | 2011 | rVB3 | 40214  | 70004  | 11.32%  | 0.763% |
| 64 | 14.021 | 2024 | 2029 | 2032 | rBV2 | 526024 | 618417 | 100.00% | 6.744% |
| 65 | 14.051 | 2032 | 2034 | 2039 | rVB  | 150739 | 137185 | 22.18%  | 1.496% |
| 66 | 14.127 | 2045 | 2047 | 2049 | rBV  | 14639  | 11233  | 1.82%   | 0.123% |
| 67 | 14.169 | 2051 | 2054 | 2060 | rVV4 | 24321  | 35466  | 5.73%   | 0.387% |
| 68 | 14.251 | 2063 | 2068 | 2070 | rBV4 | 17082  | 19547  | 3.16%   | 0.213% |
| 69 | 14.280 | 2070 | 2073 | 2075 | rVB4 | 15008  | 14569  | 2.36%   | 0.159% |
| 70 | 14.304 | 2075 | 2077 | 2079 | rBV2 | 8621   | 7906   | 1.28%   | 0.086% |
| 71 | 14.374 | 2086 | 2089 | 2090 | rBV  | 14164  | 13745  | 2.22%   | 0.150% |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF112217\  
 Data File : BF100849.D  
 Acq On : 23 Nov 2017 3:01  
 Operator : SJ/JU  
 Sample : I6548-03 5X  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 SAU-1-E(3-4)

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF110817.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

|     |        |      |      |      |      |        |        |        |        |
|-----|--------|------|------|------|------|--------|--------|--------|--------|
| 72  | 14.410 | 2090 | 2095 | 2098 | rVB  | 50663  | 53934  | 8.72%  | 0.588% |
| 73  | 14.439 | 2098 | 2100 | 2103 | rBV2 | 29822  | 28202  | 4.56%  | 0.308% |
| 74  | 14.480 | 2104 | 2107 | 2108 | rBV3 | 14300  | 13549  | 2.19%  | 0.148% |
| 75  | 14.533 | 2113 | 2116 | 2118 | rVV2 | 30282  | 33675  | 5.45%  | 0.367% |
| 76  | 14.557 | 2118 | 2120 | 2124 | rVV5 | 27551  | 34089  | 5.51%  | 0.372% |
| 77  | 14.604 | 2125 | 2128 | 2131 | rVB3 | 23904  | 27341  | 4.42%  | 0.298% |
| 78  | 14.716 | 2145 | 2147 | 2150 | rBV3 | 8773   | 7781   | 1.26%  | 0.085% |
| 79  | 14.745 | 2150 | 2152 | 2157 | rVV5 | 9685   | 12419  | 2.01%  | 0.135% |
| 80  | 14.792 | 2157 | 2160 | 2164 | rVV5 | 13042  | 22312  | 3.61%  | 0.243% |
| 81  | 14.827 | 2164 | 2166 | 2169 | rVB4 | 17359  | 13910  | 2.25%  | 0.152% |
| 82  | 14.968 | 2187 | 2190 | 2194 | rBV5 | 13177  | 19641  | 3.18%  | 0.214% |
| 83  | 15.063 | 2201 | 2206 | 2210 | rBV  | 176129 | 297672 | 48.13% | 3.246% |
| 84  | 15.174 | 2221 | 2225 | 2228 | rVB  | 46087  | 51588  | 8.34%  | 0.563% |
| 85  | 15.368 | 2253 | 2258 | 2264 | rVB  | 133601 | 173406 | 28.04% | 1.891% |
| 86  | 15.427 | 2264 | 2268 | 2274 | rVB  | 166559 | 213801 | 34.57% | 2.332% |
| 87  | 15.498 | 2274 | 2280 | 2283 | rBV  | 375548 | 476769 | 77.10% | 5.199% |
| 88  | 15.527 | 2283 | 2285 | 2291 | rVB2 | 50034  | 66528  | 10.76% | 0.726% |
| 89  | 15.810 | 2330 | 2333 | 2338 | rBV4 | 16427  | 24936  | 4.03%  | 0.272% |
| 90  | 15.851 | 2338 | 2340 | 2346 | rVB6 | 13027  | 19024  | 3.08%  | 0.207% |
| 91  | 15.933 | 2350 | 2354 | 2358 | rVB5 | 14622  | 24955  | 4.04%  | 0.272% |
| 92  | 16.015 | 2366 | 2368 | 2372 | rBV5 | 9020   | 9421   | 1.52%  | 0.103% |
| 93  | 16.057 | 2372 | 2375 | 2379 | rVV3 | 13111  | 17774  | 2.87%  | 0.194% |
| 94  | 16.627 | 2469 | 2472 | 2475 | rBV5 | 12614  | 14564  | 2.36%  | 0.159% |
| 95  | 16.780 | 2493 | 2498 | 2499 | rBV4 | 12249  | 17174  | 2.78%  | 0.187% |
| 96  | 16.968 | 2524 | 2530 | 2537 | rVB2 | 75470  | 147123 | 23.79% | 1.604% |
| 97  | 17.145 | 2556 | 2560 | 2563 | rBV4 | 13263  | 17023  | 2.75%  | 0.186% |
| 98  | 17.415 | 2599 | 2606 | 2612 | rBV  | 62535  | 122025 | 19.73% | 1.331% |
| 99  | 17.651 | 2643 | 2646 | 2652 | rVB4 | 11910  | 23219  | 3.75%  | 0.253% |
| 100 | 18.339 | 2759 | 2763 | 2765 | rBV5 | 5465   | 8165   | 1.32%  | 0.089% |


Sum of corrected areas: 9169756

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF112217\  
Data File : BF100849.D  
Acq On : 23 Nov 2017 3:01  
Operator : SJ/JU  
Sample : I6548-03 5X  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampled :  
SAU-1-E(3-4)

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF110817.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

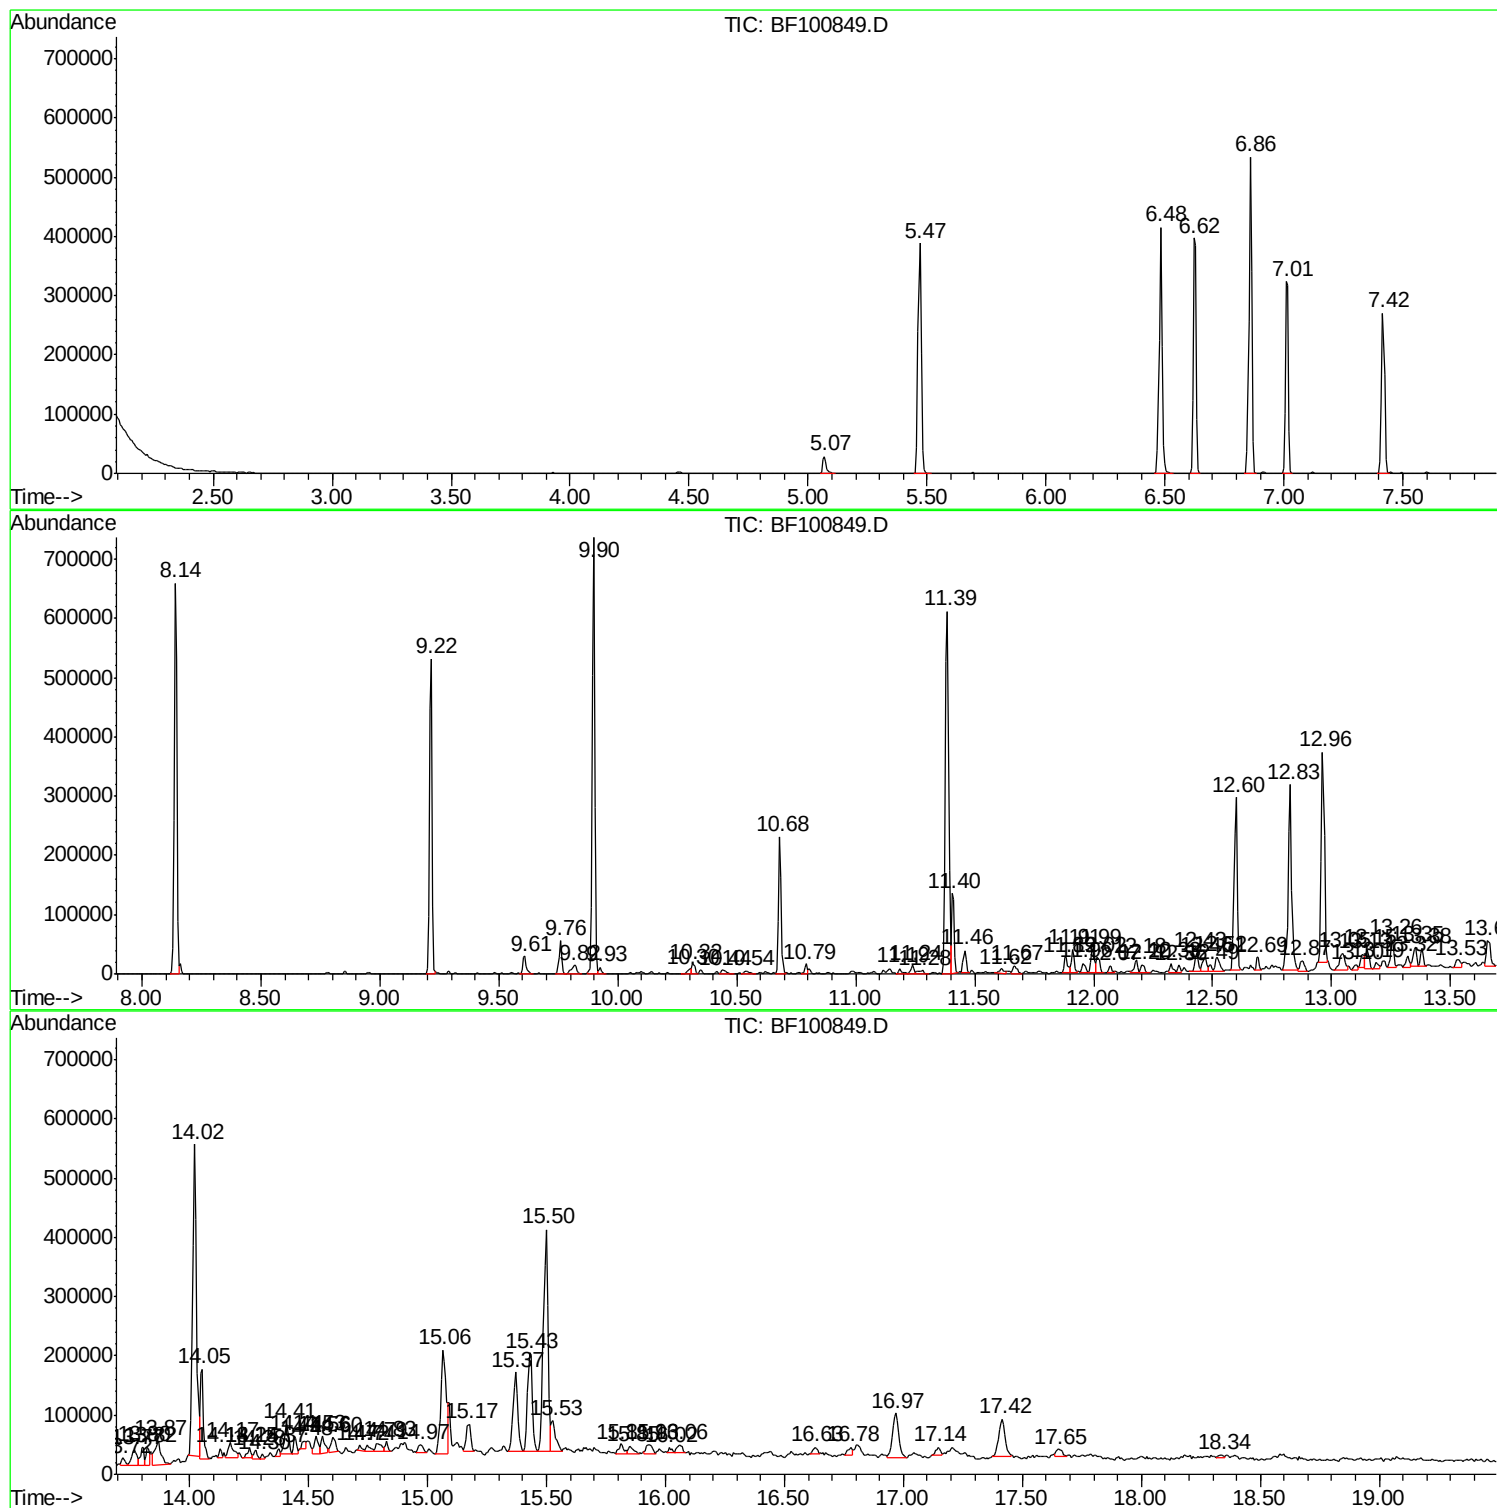

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF112217\  
Data File : BF100849.D  
Acq On : 23 Nov 2017 3:01  
Operator : SJ/JU  
Sample : I6548-03 5X  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SAU-1-E(3-4)

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF110817.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION










TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

\*\*\*\*\*  
Peak Number 1 unknown6.62 Concentration Rank 1

| R.T. | EstConc  | Area   | Relative to ISTD       | R.T. |
|------|----------|--------|------------------------|------|
| 6.62 | 16.48 ng | 356349 | 1,4-Dichlorobenzene-d4 | 6.86 |

| Hit# | of | Tentative ID                   | MW  | MolForm   | CAS#         | Qual |
|------|----|--------------------------------|-----|-----------|--------------|------|
| 1    | 5  | 5-Aminoindole                  | 132 | C8H8N2    | 005192-03-0  | 12   |
| 2    |    | Tranylcypromine-propionyl      | 189 | C12H15NO  | 1000123-86-3 | 10   |
| 3    |    | 5-Fluoro-2-chloropyrimidine    | 132 | C4H2ClFN2 | 062802-42-0  | 9    |
| 4    |    | 4-Methylpyrrolo[1,2-a]pyrazine | 132 | C8H8N2    | 064608-60-2  | 9    |
| 5    |    | 1H-Benzimidazole, 2-methyl-    | 132 | C8H8N2    | 000615-15-6  | 9    |

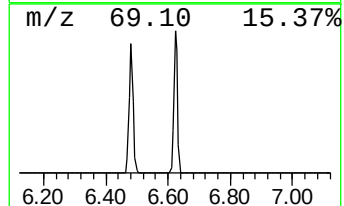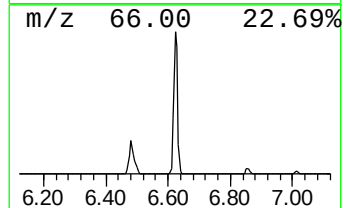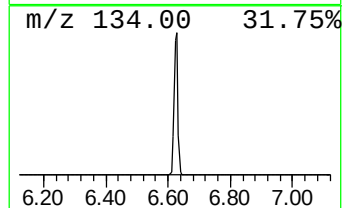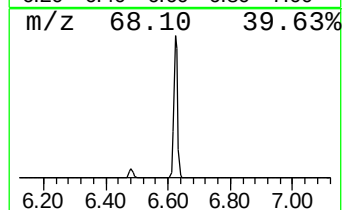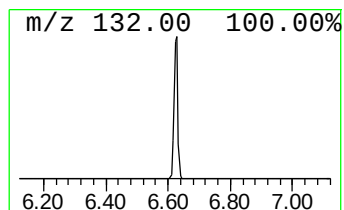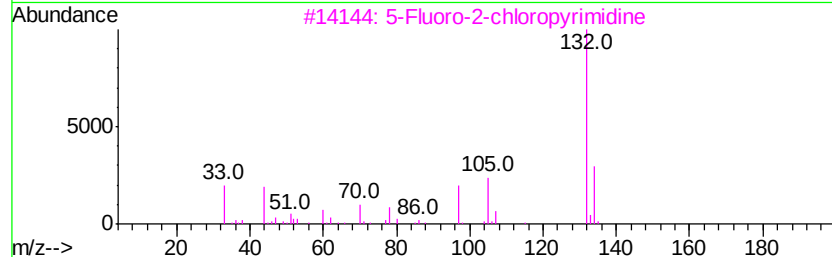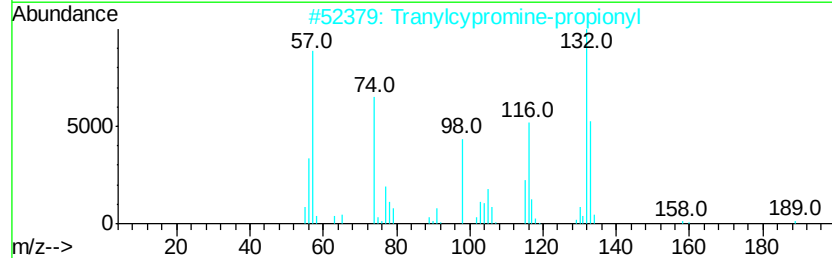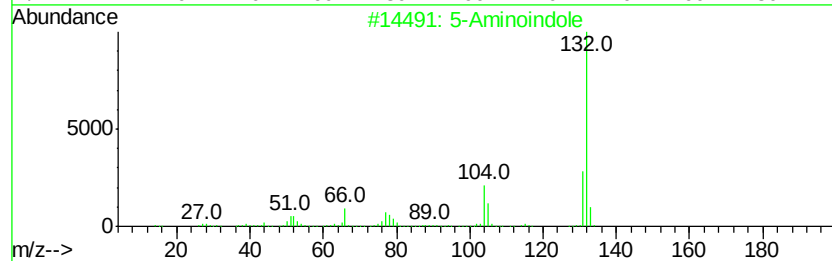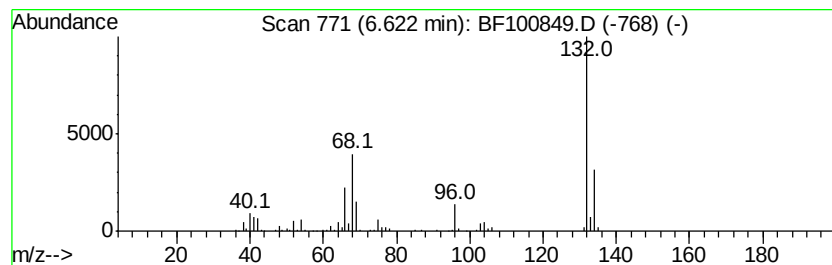

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF112217\  
Data File : BF100849.D  
Acq On : 23 Nov 2017 3:01  
Operator : SJ/JU  
Sample : I6548-03 5X  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SAU-1-E(3-4)










Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF110817.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

\*\*\*\*\*  
Peak Number 3 11H-Benzo[a]fluoren-11-one Concentration Rank 4

| R.T.  | EstConc | Area  | Relative to ISTD | R.T.  |
|-------|---------|-------|------------------|-------|
| 13.87 | 2.26 ng | 70004 | Chrysene-d12     | 14.02 |

| Hit# | of | Tentative ID                        | MW  | MolForm  | CAS#        | Qual |
|------|----|-------------------------------------|-----|----------|-------------|------|
| 1    | 5  | 11H-Benzo[a]fluoren-11-one          | 230 | C17H10O  | 000479-79-8 | 93   |
| 2    |    | 7H-Benz[de]anthracen-7-one          | 230 | C17H10O  | 000082-05-3 | 74   |
| 3    |    | 6H-Benz[de]anthracen-6-one          | 230 | C17H10O  | 080252-14-8 | 58   |
| 4    |    | Pyrene, 1,3-dimethyl-               | 230 | C18H14   | 064401-21-4 | 53   |
| 5    |    | (E)-.alpha.,.alpha.'-Dicyanostil... | 230 | C16H10N2 | 002450-55-7 | 53   |

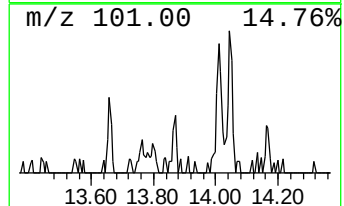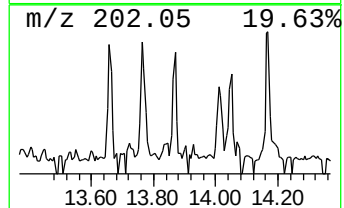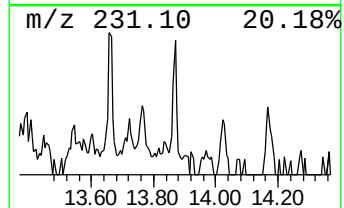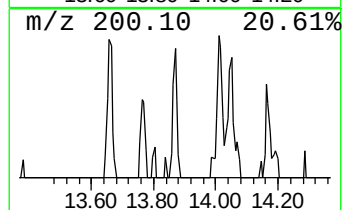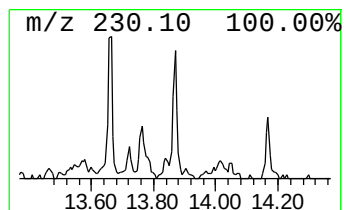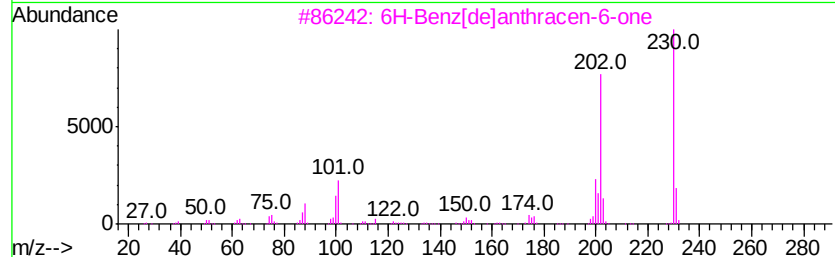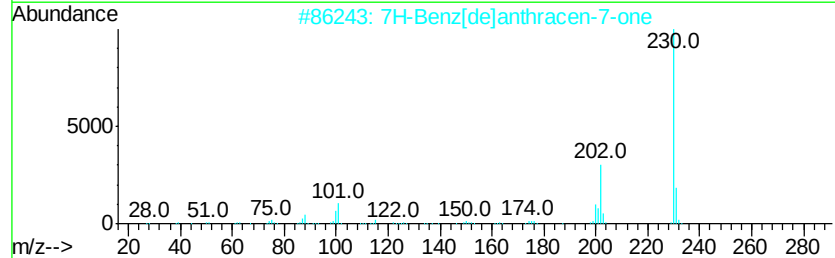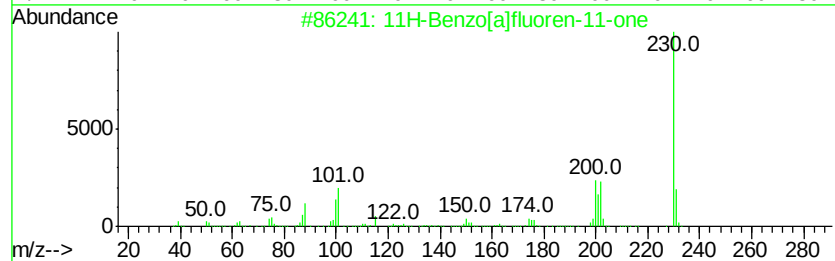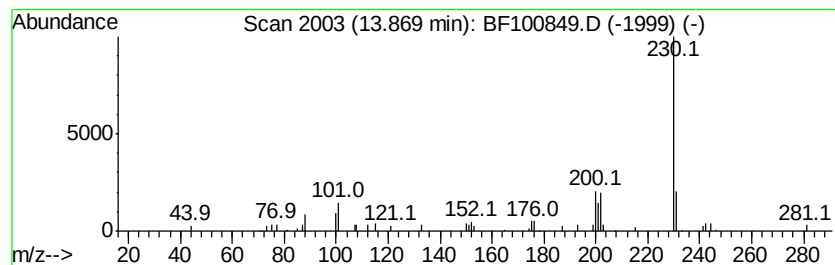

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF112217\  
Data File : BF100849.D  
Acq On : 23 Nov 2017 3:01  
Operator : SJ/JU  
Sample : I6548-03 5X  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SAU-1-E(3-4)

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF110817.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION










TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

\*\*\*\*\*  
Peak Number 4 Benzo[e]pyrene Concentration Rank 5

| R.T.  | EstConc | Area  | Relative to ISTD | R.T.  |
|-------|---------|-------|------------------|-------|
| 15.17 | 2.16 ng | 51588 | Perylene-d12     | 15.50 |

| Hit# of | 5 | Tentative ID              | MW  | MolForm | CAS#        | Qual |
|---------|---|---------------------------|-----|---------|-------------|------|
| 1       |   | Benzo[e]pyrene            | 252 | C20H12  | 000192-97-2 | 95   |
| 2       |   | Benzo[a]pyrene            | 252 | C20H12  | 000050-32-8 | 94   |
| 3       |   | Benzo[k]fluoranthene      | 252 | C20H12  | 000207-08-9 | 93   |
| 4       |   | Benzo[e]acephenanthrylene | 252 | C20H12  | 000205-99-2 | 90   |
| 5       |   | Perylene                  | 252 | C20H12  | 000198-55-0 | 86   |

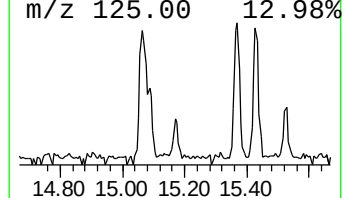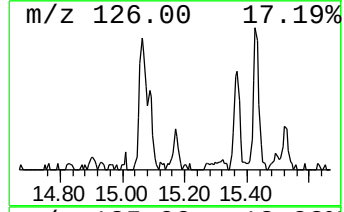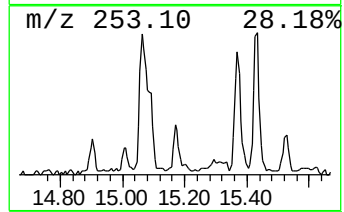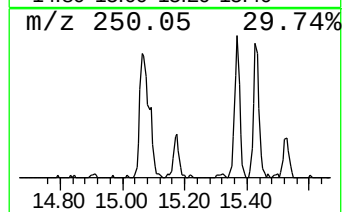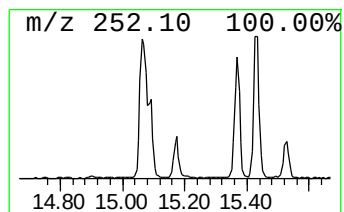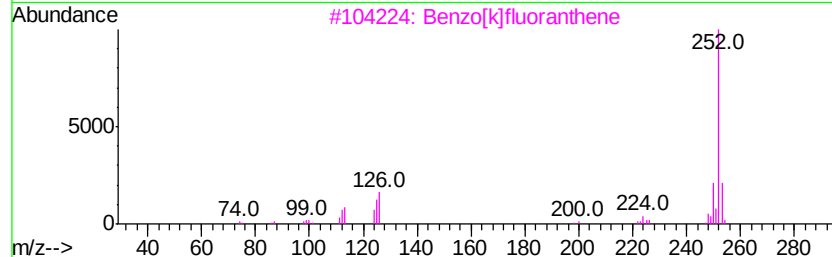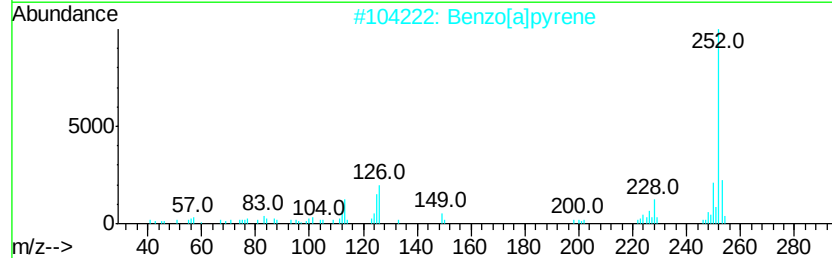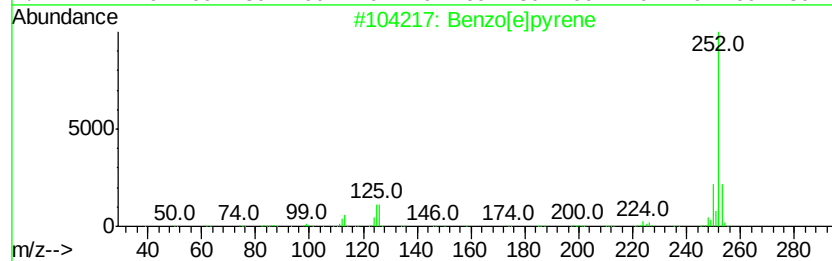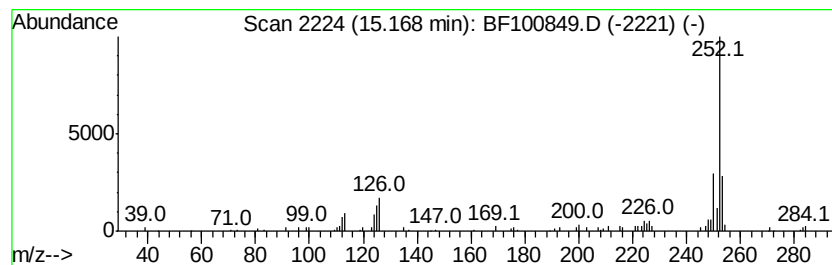

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF112217\  
Data File : BF100849.D  
Acq On : 23 Nov 2017 3:01  
Operator : SJ/JU  
Sample : I6548-03 5X  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SAU-1-E(3-4)

Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF110817.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name     | RT    | EstConc | Units | Response | --Internal Standard-- |       |        |      |
|----------------------|-------|---------|-------|----------|-----------------------|-------|--------|------|
|                      |       |         |       |          | #                     | RT    | Resp   | Conc |
| unknown6.62          | 6.62  | 16.5    | ng    | 356349   | 1                     | 6.86  | 432557 | 20.0 |
| 11H-Benzo[a]fluor... | 13.87 | 2.3     | ng    | 70004    | 5                     | 14.02 | 618417 | 20.0 |
| Benzo[e]pyrene       | 15.17 | 2.2     | ng    | 51588    | 6                     | 15.50 | 476769 | 20.0 |