

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112217\
 Data File : BF100873.D
 Acq On : 23 Nov 2017 14:12
 Operator : SJ/JU
 Sample : I6567-05
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 112017-JETT-F-D-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.075	504	508	516	rBV	124365	133512	5.24%	0.978%
2	5.469	572	575	579	rBV	644537	607800	23.83%	4.451%
3	6.475	743	746	754	rBB	419789	401942	15.76%	2.944%
4	6.628	767	772	775	rBV	1249302	1178551	46.21%	8.631%
5	6.857	807	811	814	rBV	548656	437876	17.17%	3.207%
6	7.016	833	838	841	rBV	1931338	1683196	66.00%	12.327%
7	7.422	901	907	910	rBV	1243141	1407610	55.20%	10.309%
8	8.139	1025	1029	1032	rBV	707280	570710	22.38%	4.180%
9	9.216	1206	1212	1215	rBV	2660198	2550221	100.00%	18.676%
10	9.892	1321	1327	1331	rBV	679127	654319	25.66%	4.792%
11	10.680	1457	1461	1465	rBV	949376	887616	34.81%	6.500%
12	11.380	1576	1580	1583	rBV	702855	559240	21.93%	4.096%
13	12.969	1845	1850	1853	rBV	1911669	1766137	69.25%	12.934%
14	13.851	1996	2000	2004	rBV	30048	31078	1.22%	0.228%
15	14.021	2025	2029	2032	rBV	402011	368930	14.47%	2.702%
16	15.492	2273	2279	2289	rBV	317897	416060	16.31%	3.047%


Sum of corrected areas: 13654798

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112217\
Data File : BF100873.D
Acq On : 23 Nov 2017 14:12
Operator : SJ/JU
Sample : I6567-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
112017-JETT-F-D-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

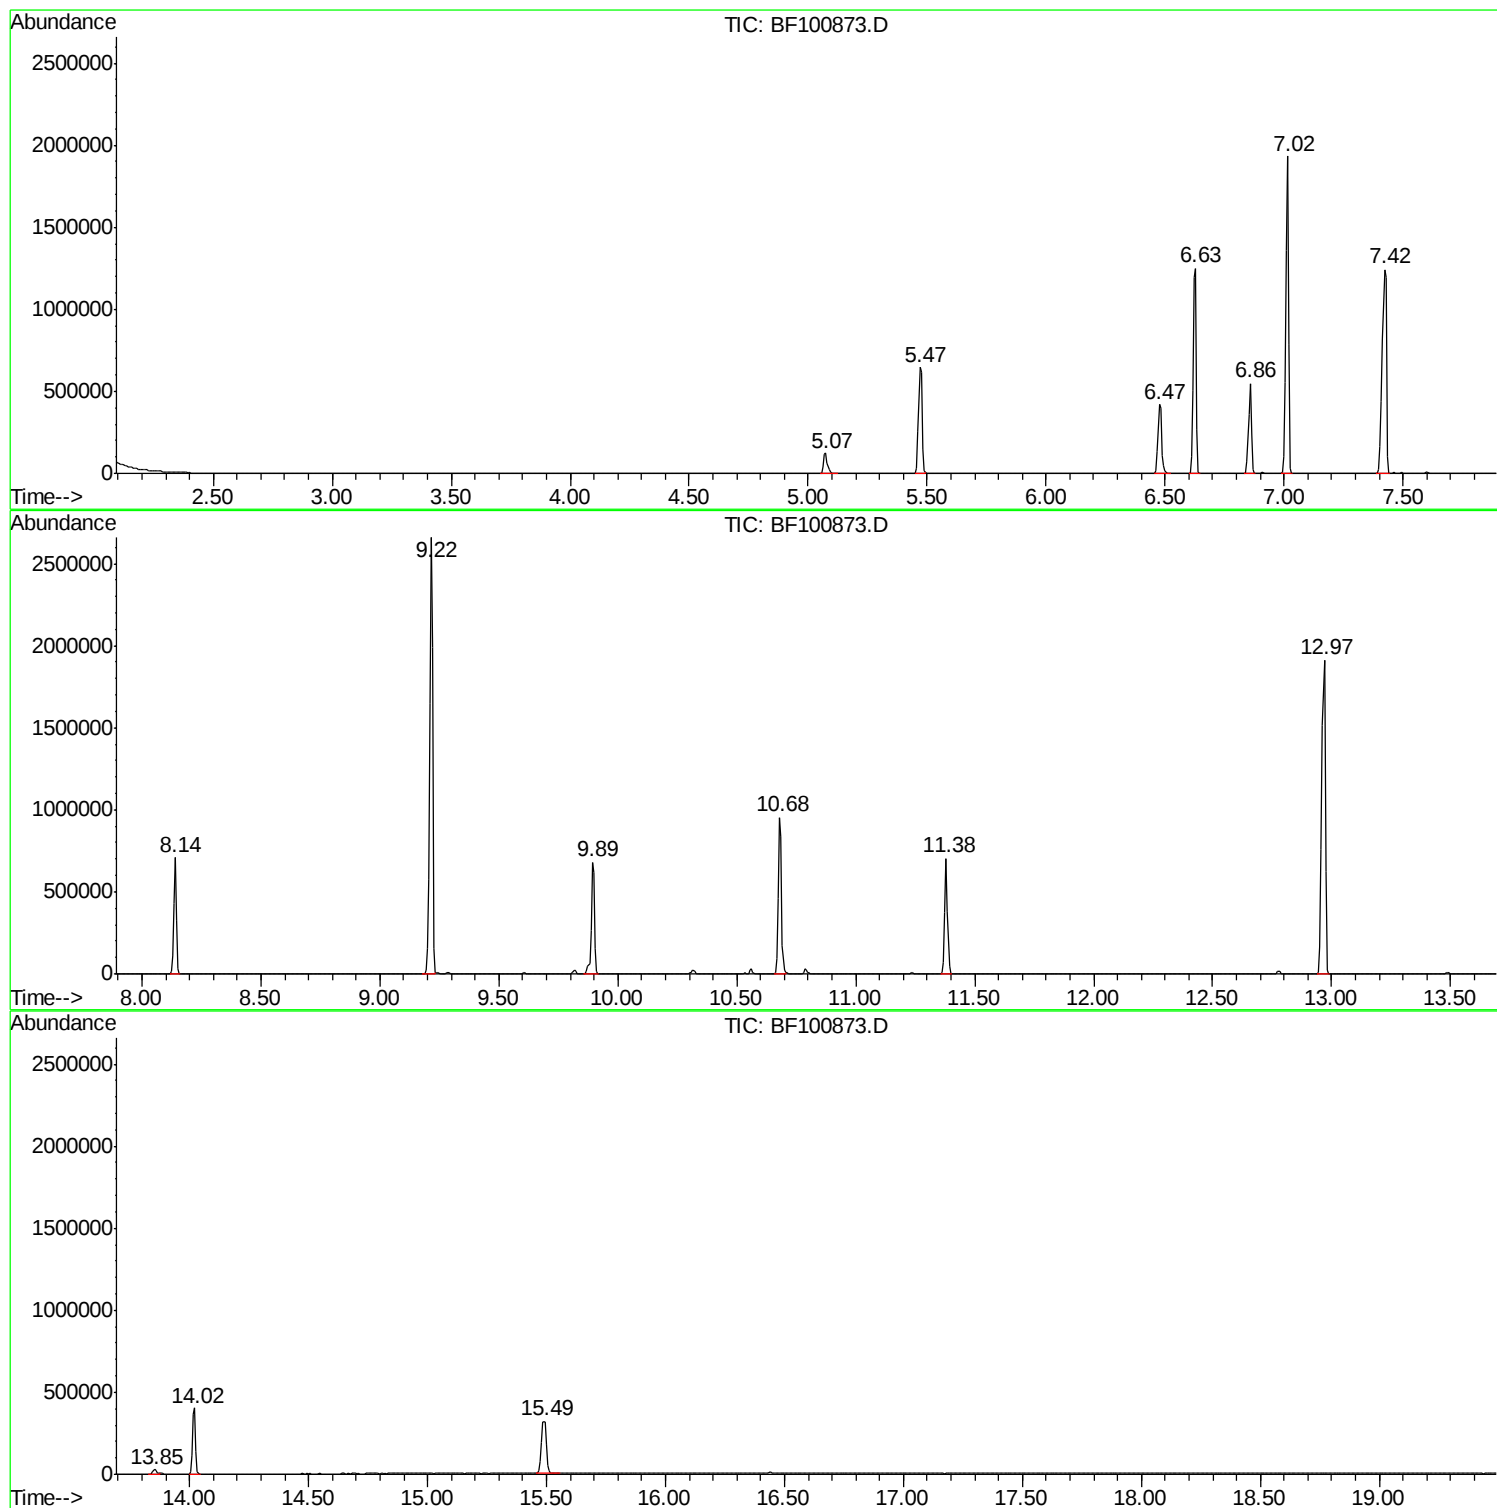

Data Path : Z:\HPCHEM1\BNA F\DATA\BF112217\
Data File : BF100873.D
Acq On : 23 Nov 2017 14:12
Operator : SJ/JU
Sample : I6567-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
112017-JETT-F-D-B










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.07	6.10 ng	133512	1,4-Dichlorobenzene-d4	6.86

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	38
2			Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	38
3			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
4			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
5			Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	9

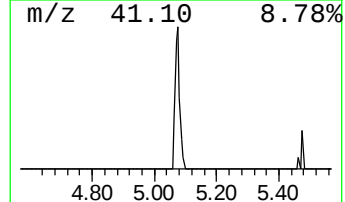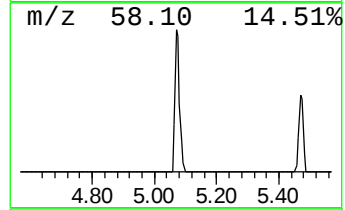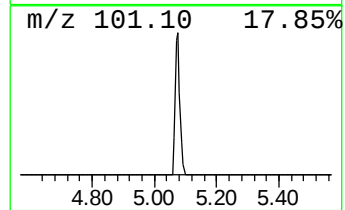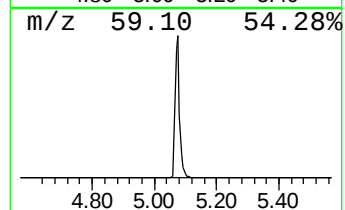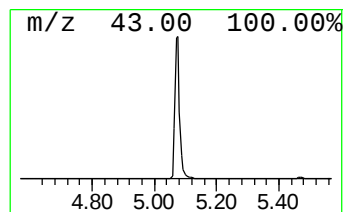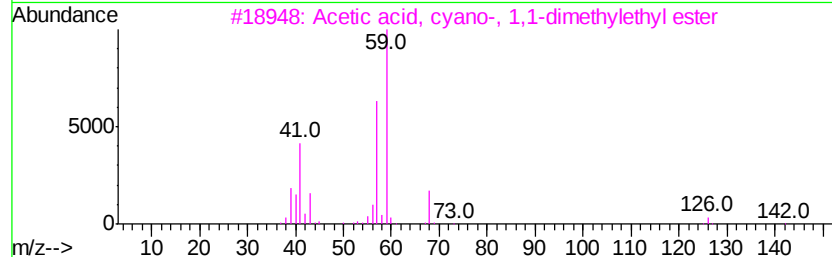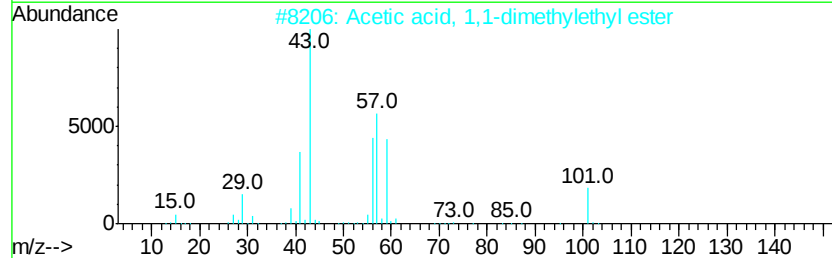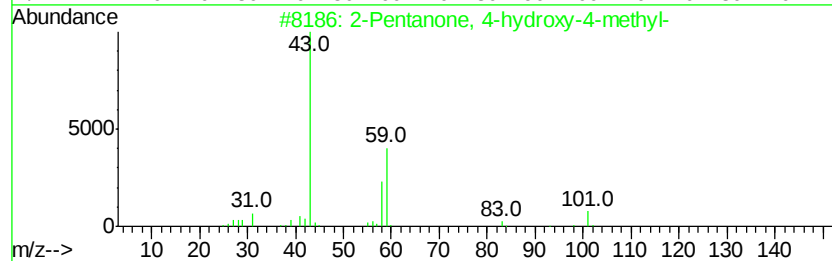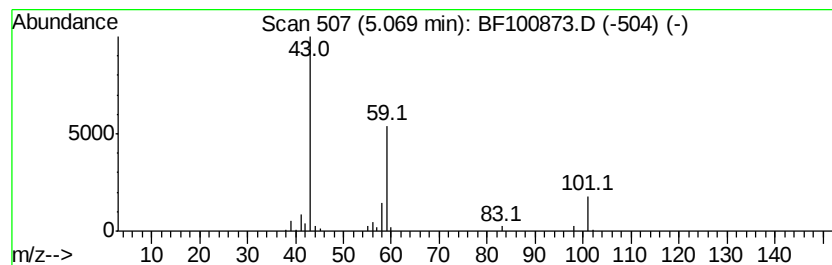

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112217\
Data File : BF100873.D
Acq On : 23 Nov 2017 14:12
Operator : SJ/JU
Sample : I6567-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
112017-JETT-F-D-B










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.63 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.63	53.83 ng	1178550	1,4-Dichlorobenzene-d4	6.86

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		Xenon	132	Xe	007440-63-3	9
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

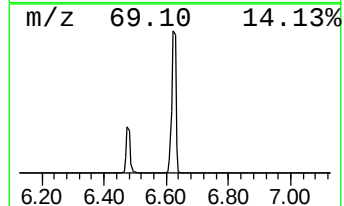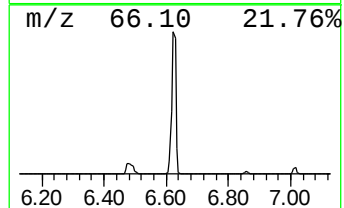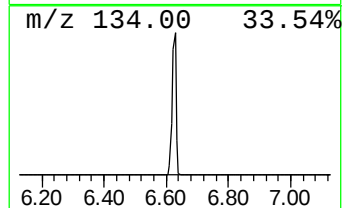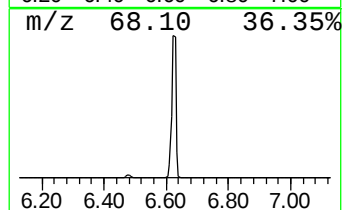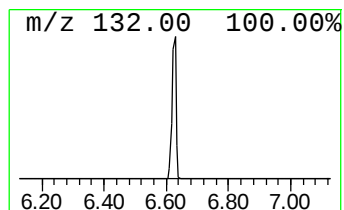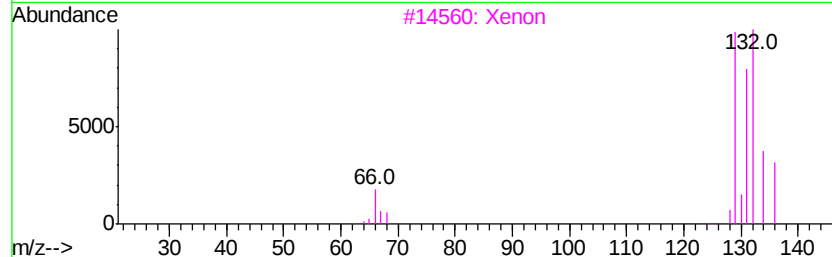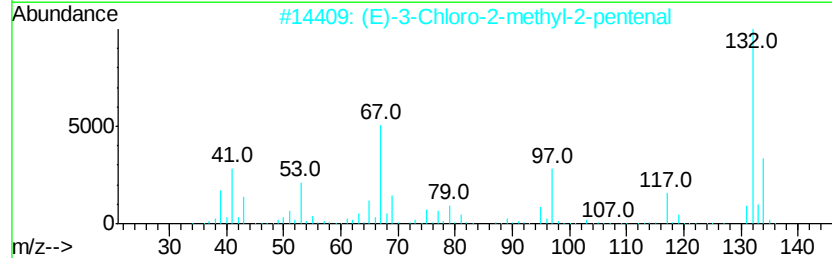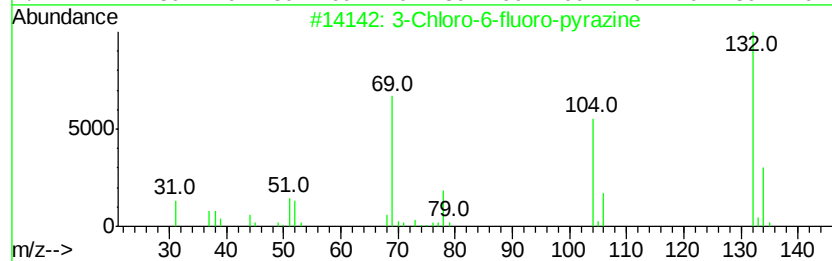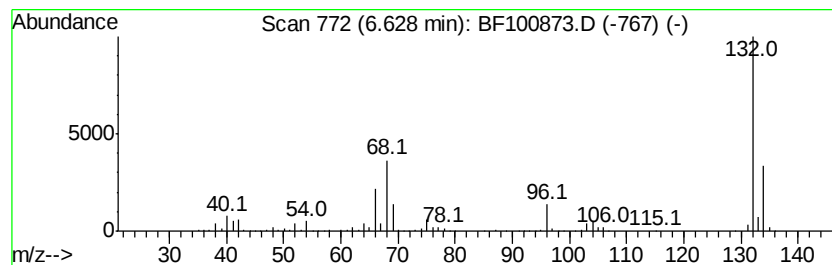

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112217\
Data File : BF100873.D
Acq On : 23 Nov 2017 14:12
Operator : SJ/JU
Sample : I6567-05
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
112017-JETT-F-D-B

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.07	6.1	ng	133512	1	6.86	437876	20.0
unknown6.63	6.63	53.8	ng	1178550	1	6.86	437876	20.0