


Data Path : Z:\HPCHEM1\BNA F\Data\BF112217\
 Data File : BF100828.D
 Acq On : 22 Nov 2017 17:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 17 15:22:08 2017

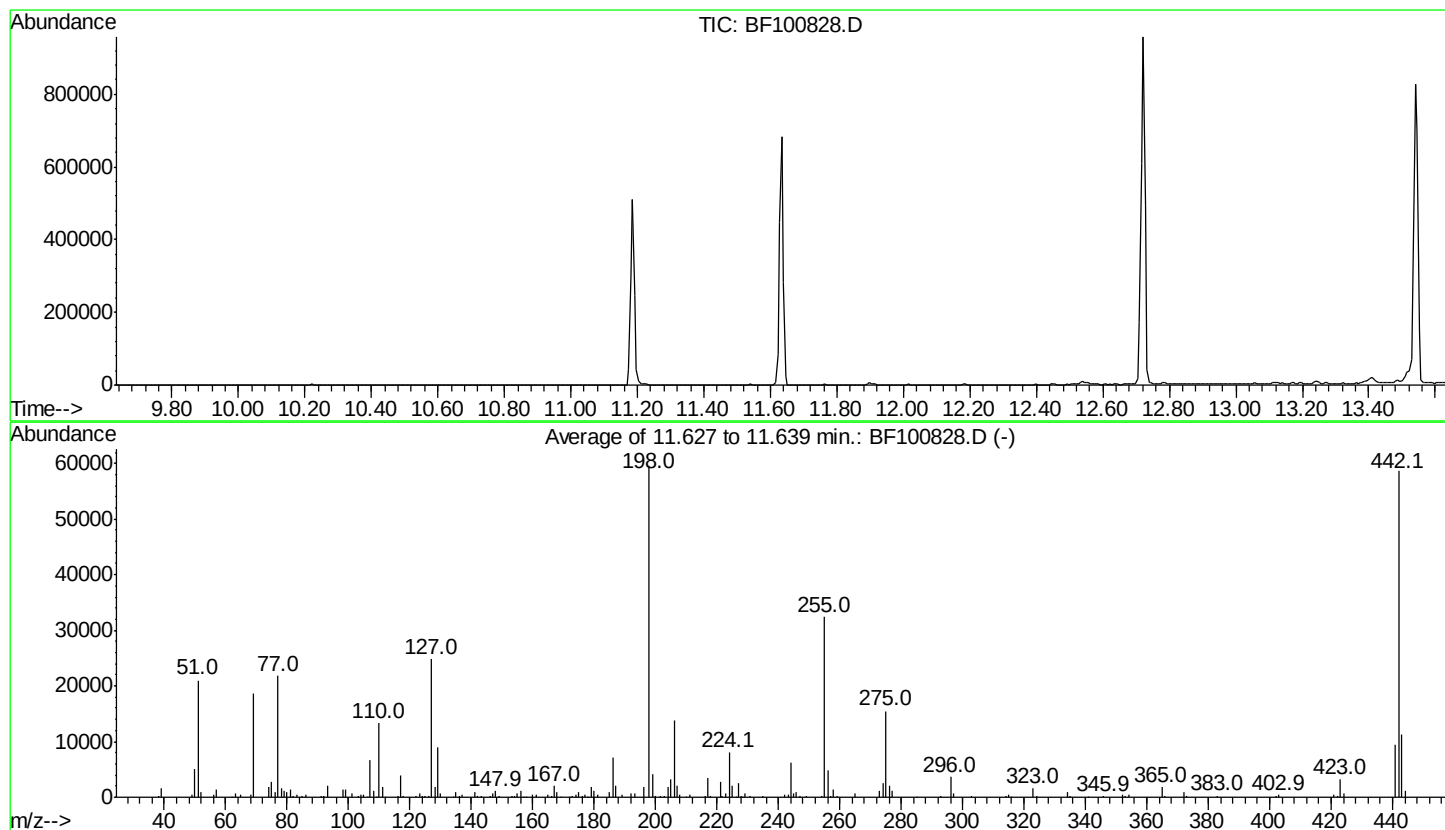

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	21037	PASS
68	69	0.00	2	2.0	365	PASS
69	198	0.00	100	31.4	18684	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.7	24822	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	59592	PASS
199	198	5	9	6.9	4089	PASS
275	198	10	60	26.0	15474	PASS
365	198	1	100	3.0	1777	PASS
441	443	0.01	100	82.8	9415	PASS
442	198	50	100	98.6	58762	PASS
443	442	15	24	19.3	11364	PASS