


Data Path : Z:\HPCHEM1\BNA_F\Data\BF112217\
 Data File : BF100854.D
 Acq On : 23 Nov 2017 5:41
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 17 15:22:08 2017

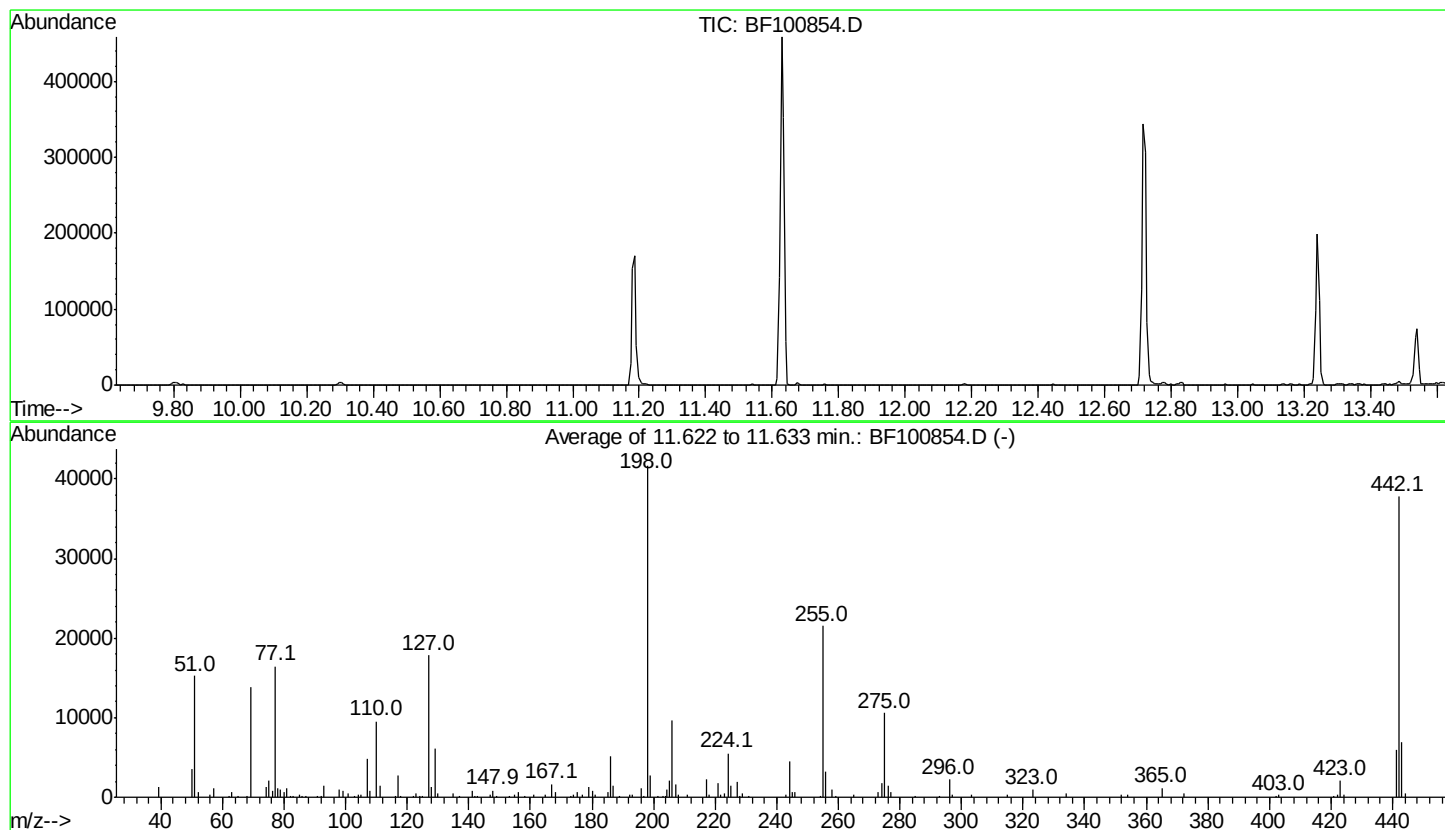

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	15245	PASS
68	69	0.00	2	0.9	130	PASS
69	198	0.00	100	33.4	13915	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.7	17797	PASS
197	198	0.00	2	0.4	149	PASS
198	198	100	100	100.0	41666	PASS
199	198	5	9	6.5	2691	PASS
275	198	10	60	25.5	10614	PASS
365	198	1	100	2.8	1148	PASS
441	443	0.01	100	85.8	5958	PASS
442	198	50	100	90.6	37743	PASS
443	442	15	24	18.4	6947	PASS