


Data Path : Z:\HPCHEM1\BNA F\Data\BF112217\
 Data File : BF100812.D
 Acq On : 22 Nov 2017 8:44
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 17 15:22:08 2017

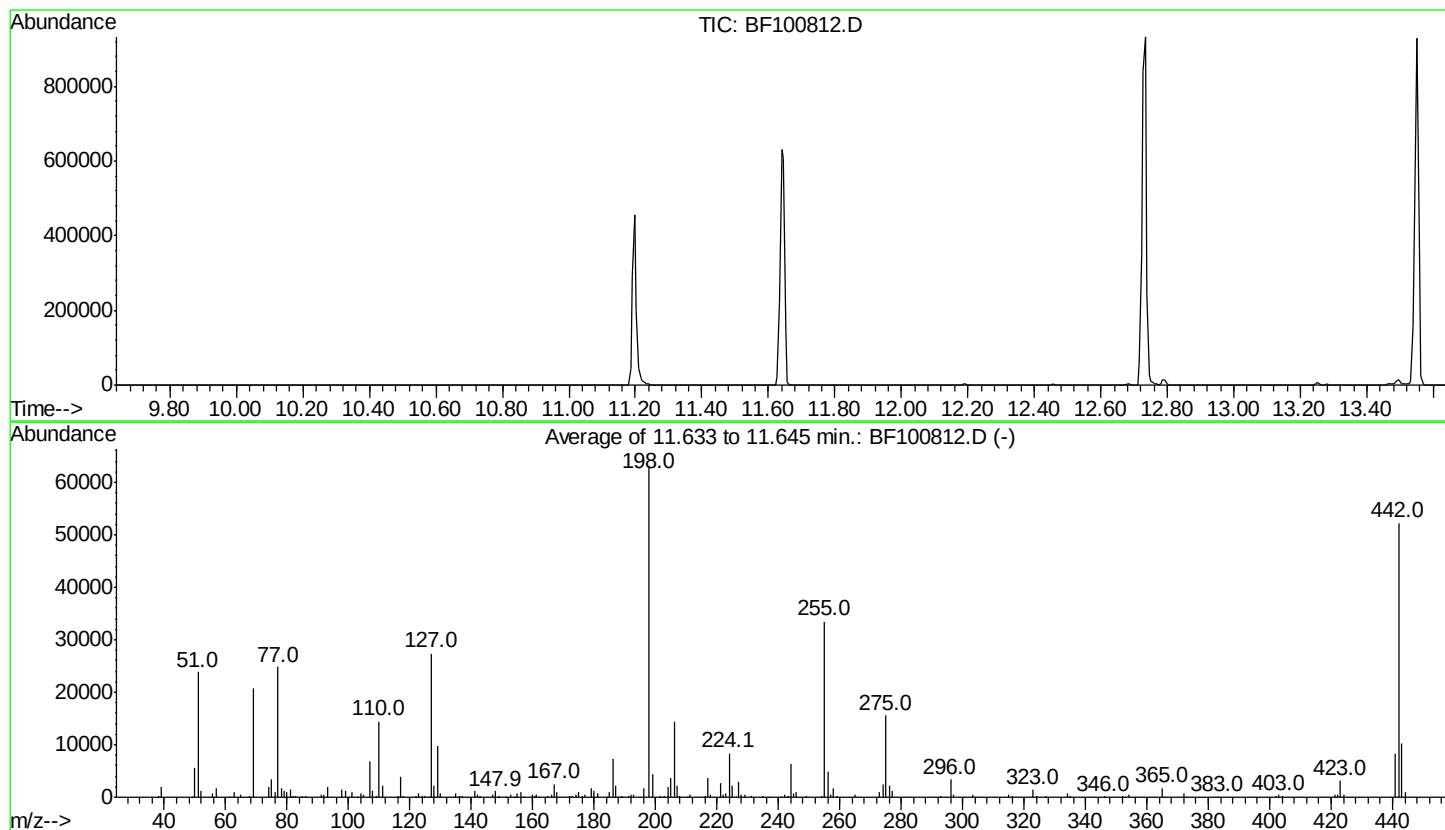

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	23806	PASS
68	69	0.00	2	0.8	172	PASS
69	198	0.00	100	32.8	20702	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.4	27398	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63170	PASS
199	198	5	9	7.0	4434	PASS
275	198	10	60	24.6	15544	PASS
365	198	1	100	2.8	1788	PASS
441	443	0.01	100	81.3	8405	PASS
442	198	50	100	82.8	52298	PASS
443	442	15	24	19.8	10338	PASS