

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112222\
 Data File : BF131339.D
 Acq On : 22 Nov 2022 20:07
 Operator : CG\JU
 Sample : N5642-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RIGHT-SIDE-FLATS-25

Quant Time: Nov 23 04:18:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 22 01:17:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.963	152	101639	20.000	ng	0.00
21) Naphthalene-d8	8.251	136	372625	20.000	ng	0.00
39) Acenaphthene-d10	10.016	164	216891	20.000	ng	-0.01
64) Phenanthrene-d10	11.510	188	380727	20.000	ng	-0.01
76) Chrysene-d12	14.168	240	189790	20.000	ng	-0.01
86) Perylene-d12	15.710	264	200763	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.575	112	500761	93.769	ng	0.00
7) Phenol-d6	6.575	99	676929	99.348	ng	-0.01
23) Nitrobenzene-d5	7.528	82	453363	61.331	ng	-0.01
42) 2,4,6-Tribromophenol	10.804	330	106801	58.530	ng	-0.01
45) 2-Fluorobiphenyl	9.334	172	863891	57.946	ng	0.00
79) Terphenyl-d14	13.110	244	841550	72.509	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112222\
Data File : BF131339.D
Acq On : 22 Nov 2022 20:07
Operator : CG\JU
Sample : N5642-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RIGHT-SIDE-FLATS-25

Quant Time: Nov 23 04:18:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 01:17:52 2022
Response via : Initial Calibration




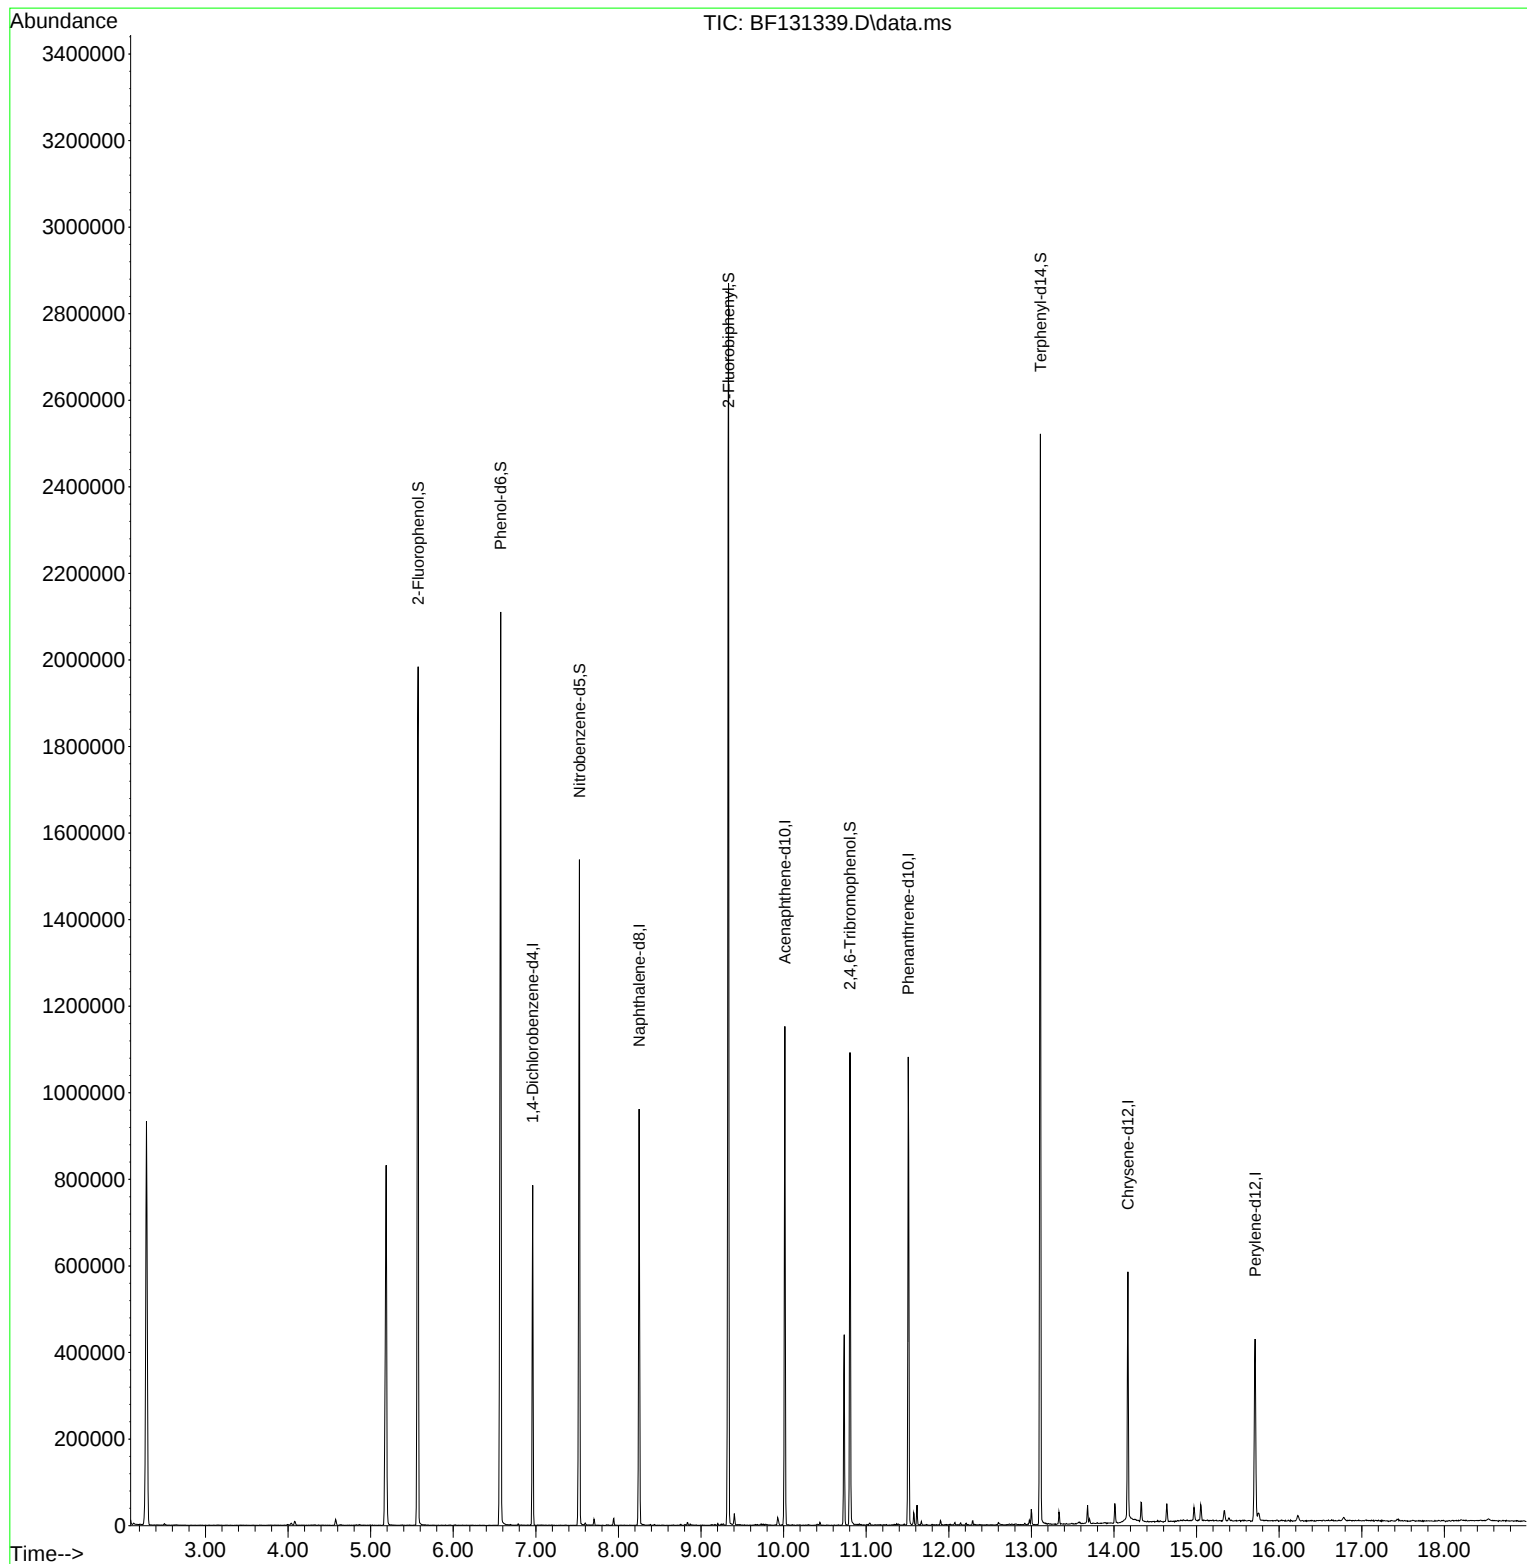


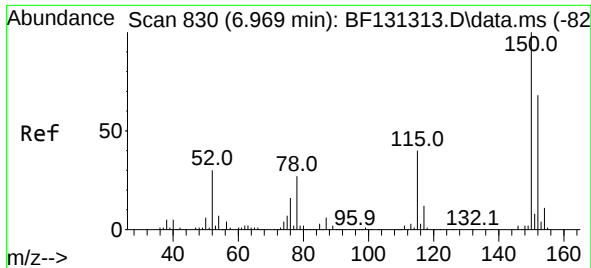

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.963 min Scan# 81
 Delta R.T. -0.006 min
 Lab File: BF131339.D
 Acq: 22 Nov 2022 20:07




Instrument :
 BNA_F
 ClientSampleId :
 RIGHT-SIDE-FLATS-25


Tgt Ion:152 Resp: 101639
 Ion Ratio Lower Upper
 152 100
 150 146.2 117.8 176.8
 115 60.5 47.1 70.7

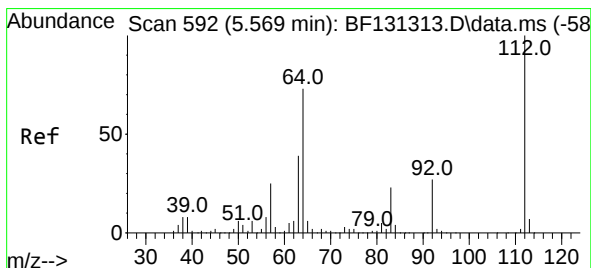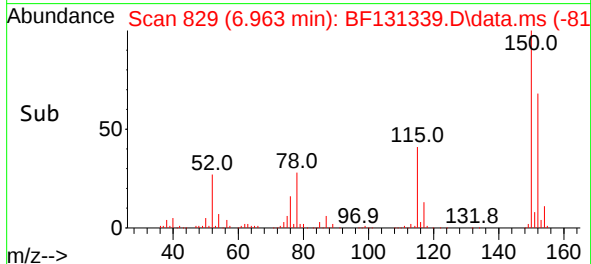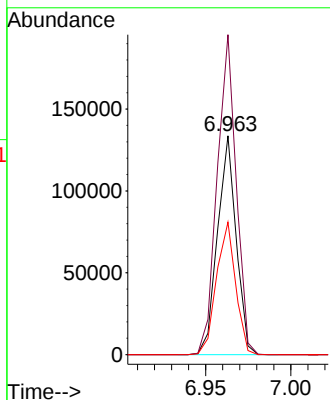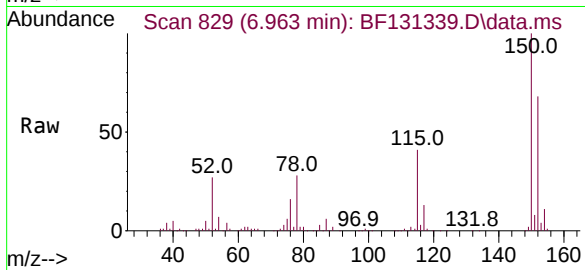

#5
 2-Fluorophenol
 Concen: 93.769 ng
 RT: 5.575 min Scan# 593
 Delta R.T. 0.006 min
 Lab File: BF131339.D
 Acq: 22 Nov 2022 20:07

Tgt Ion:112 Resp: 500761
 Ion Ratio Lower Upper
 112 100
 64 68.6 58.6 88.0
 63 36.7 31.4 47.0

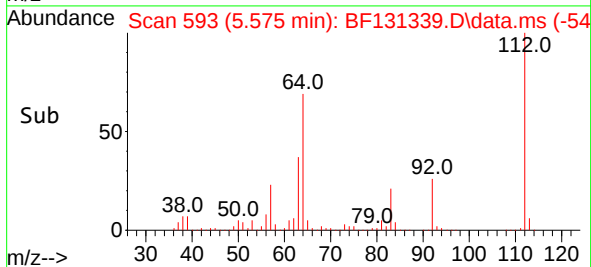
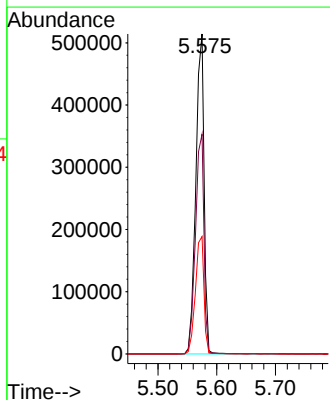
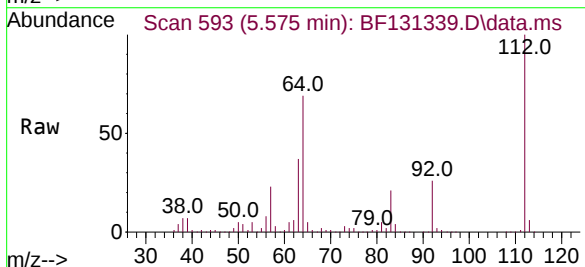


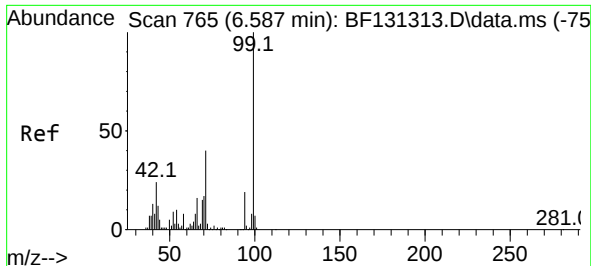

#7
Phenol-d6
Concen: 99.348 ng
RT: 6.575 min Scan# 70
Delta R.T. -0.012 min
Lab File: BF131339.D
Acq: 22 Nov 2022 20:07




Instrument :
BNA_F
ClientSampleId :
RIGHT-SIDE-FLATS-25

Tgt Ion: 99 Resp: 676929
Ion Ratio Lower Upper
99 100
42 23.5 19.4 29.2
71 39.4 32.3 48.5

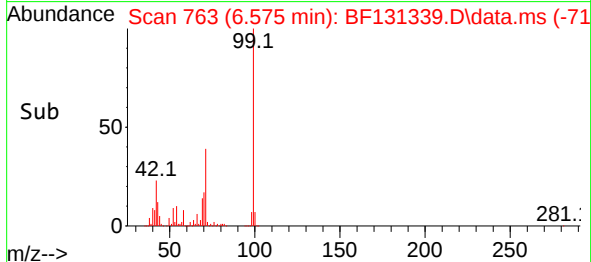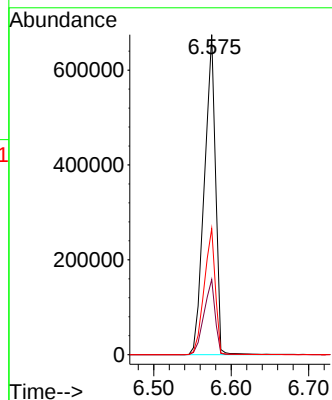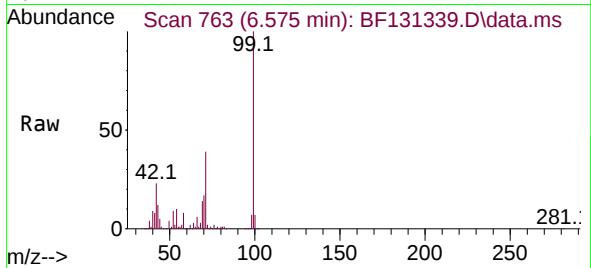

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.251 min Scan# 1048
Delta R.T. -0.006 min
Lab File: BF131339.D
Acq: 22 Nov 2022 20:07

Tgt Ion: 136 Resp: 372625
Ion Ratio Lower Upper
136 100
137 11.0 9.0 13.6
54 10.4 9.4 14.0
68 5.3 4.5 6.7


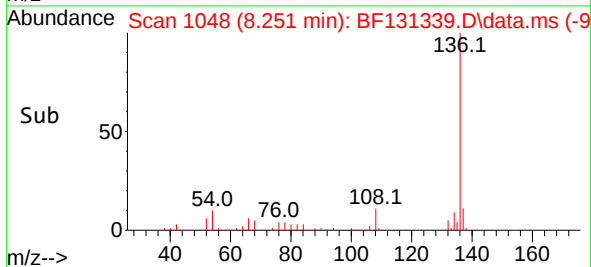
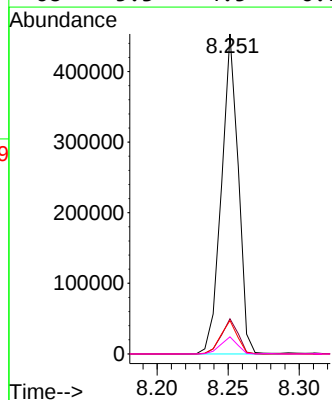
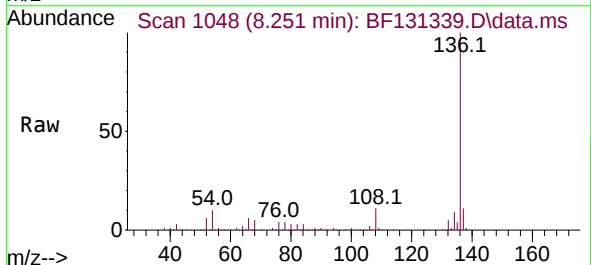




#23
Nitrobenzene-d5
Concen: 61.331 ng
RT: 7.528 min Scan# 91
Delta R.T. -0.012 min
Lab File: BF131339.D
Acq: 22 Nov 2022 20:07




Instrument :
BNA_F
ClientSampleId :
RIGHT-SIDE-FLATS-25

Tgt Ion: 82 Resp: 453363
Ion Ratio Lower Upper
82 100
128 40.9 31.4 47.0
54 61.5 49.8 74.6

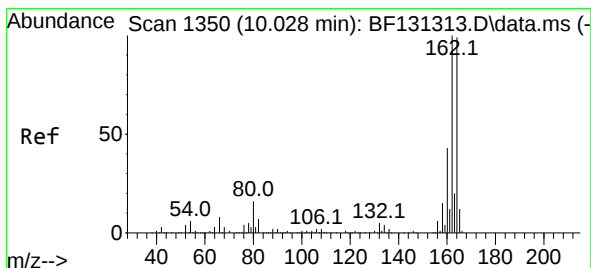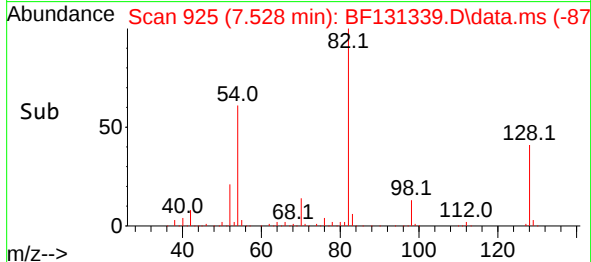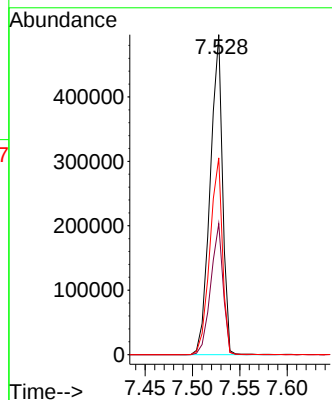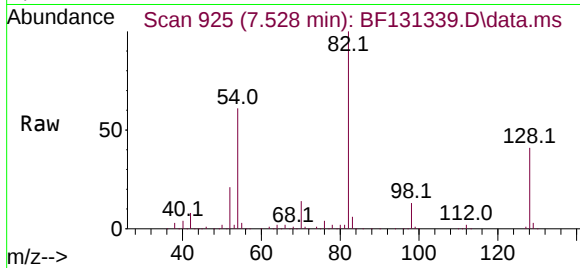

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.016 min Scan# 1348
Delta R.T. -0.012 min
Lab File: BF131339.D
Acq: 22 Nov 2022 20:07

Tgt Ion:164 Resp: 216891
Ion Ratio Lower Upper
164 100
162 100.6 80.6 120.8
160 44.1 34.4 51.6

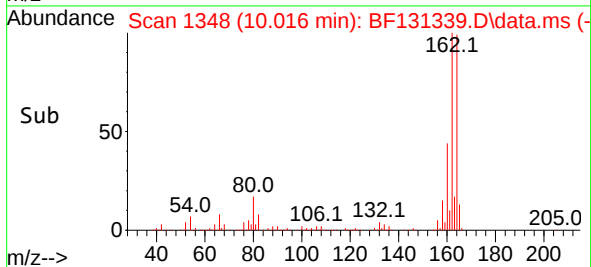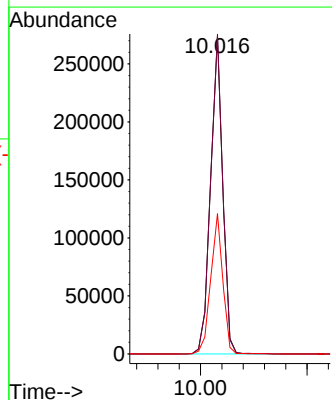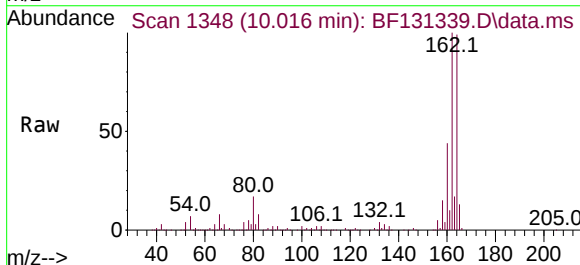



#42

2,4,6-Tribromophenol

Concen: 58.530 ng

RT: 10.804 min Scan# 1482

Delta R.T. -0.012 min

Lab File: BF131339.D


Acq: 22 Nov 2022 20:07

Instrument :

BNA_F

ClientSampleId :

RIGHT-SIDE-FLATS-25

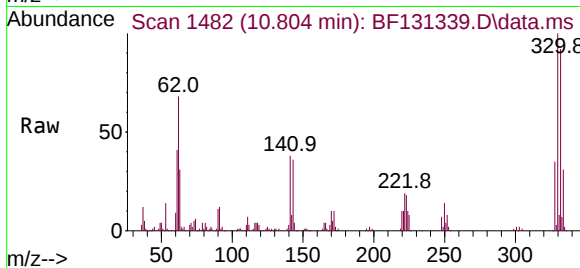




Tgt Ion:330 Resp: 106801

Ion Ratio Lower Upper

330 100

332 95.7 77.5 116.3

141 35.9 29.3 43.9

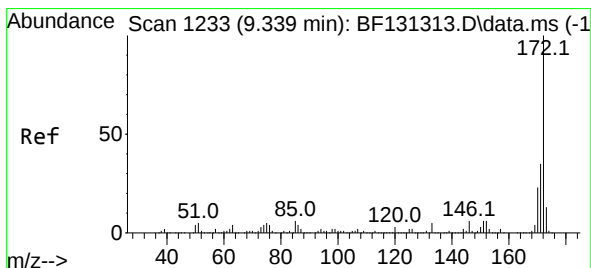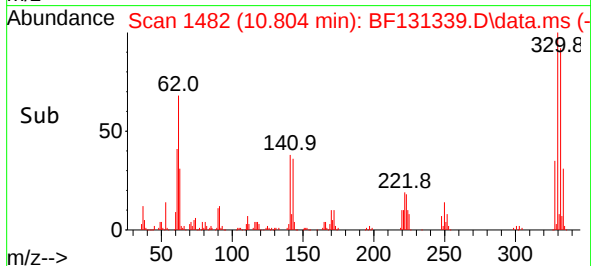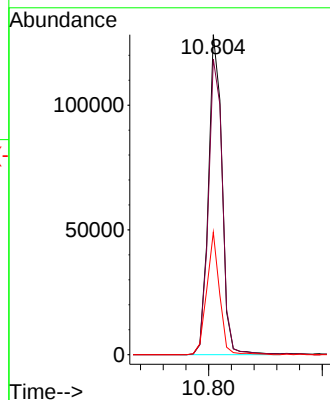

#45

2-Fluorobiphenyl

Concen: 57.946 ng

RT: 9.334 min Scan# 1232

Delta R.T. -0.006 min

Lab File: BF131339.D

Acq: 22 Nov 2022 20:07




Tgt Ion:172 Resp: 863891


Ion Ratio Lower Upper

172 100

171 34.8 28.2 42.2

170 23.7 18.7 28.1

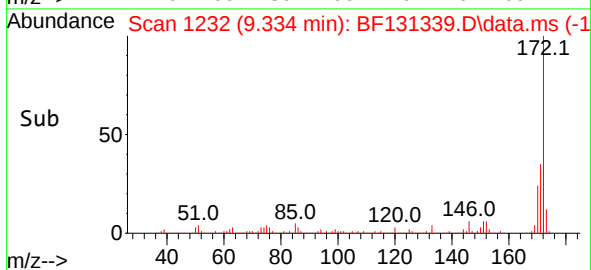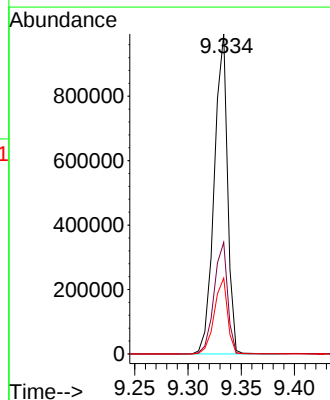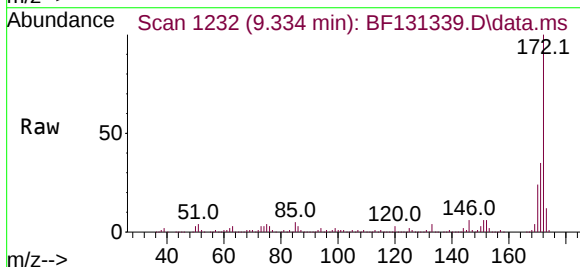

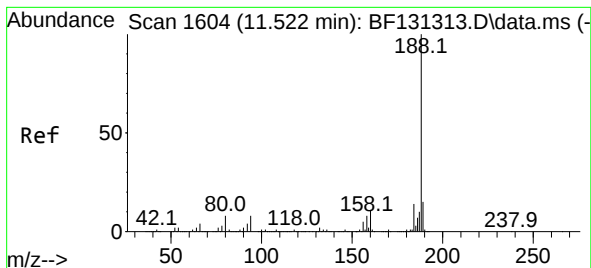

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.510 min Scan# 10

Delta R.T. -0.012 min

Lab File: BF131339.D

Acq: 22 Nov 2022 20:07

Instrument :

BNA_F

ClientSampleId :

RIGHT-SIDE-FLATS-25





Tgt Ion:188 Resp: 380727

Ion Ratio Lower Upper

188 100

94 8.7 6.3 9.5

80 9.4 6.8 10.2

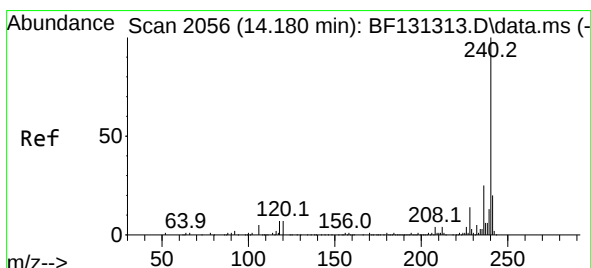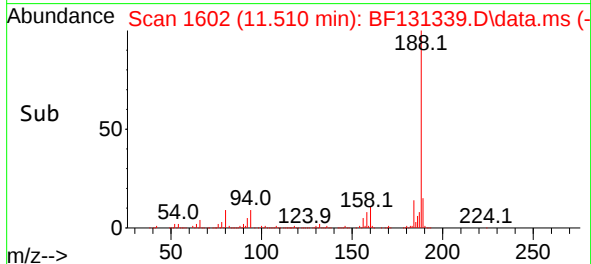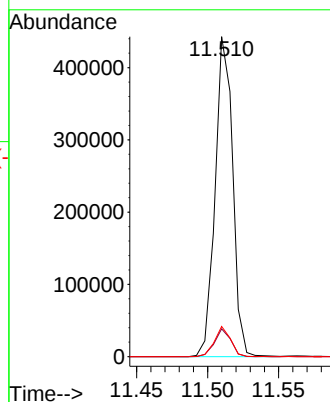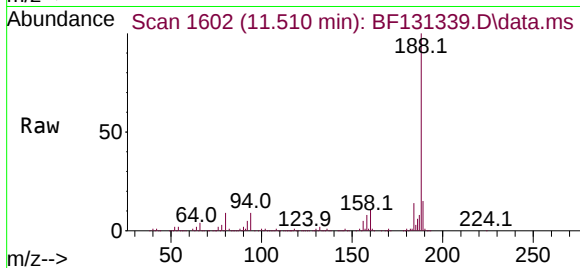

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.168 min Scan# 2054

Delta R.T. -0.012 min

Lab File: BF131339.D

Acq: 22 Nov 2022 20:07




Tgt Ion:240 Resp: 189790

Ion Ratio Lower Upper

240 100

120 8.4 5.8 8.8


236 24.8 20.3 30.5

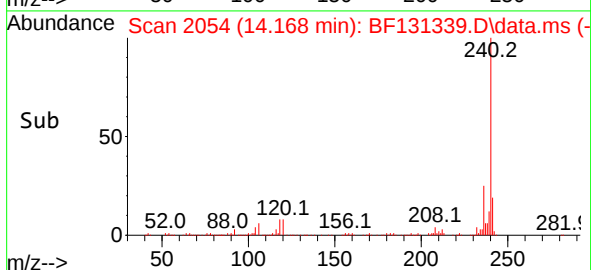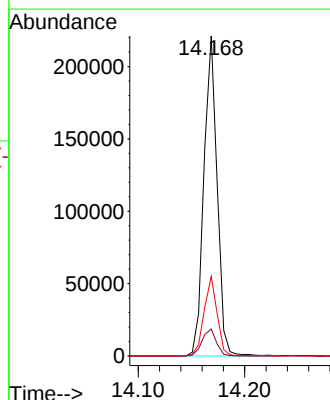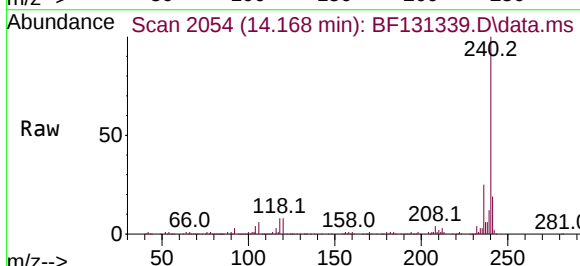






#79
 Terphenyl-d14
 Concen: 72.509 ng
 RT: 13.110 min Scan# 1875
 Delta R.T. -0.006 min
 Lab File: BF131339.D
 Acq: 22 Nov 2022 20:07

Instrument :
 BNA_F
 ClientSampleId :
 RIGHT-SIDE-FLATS-25

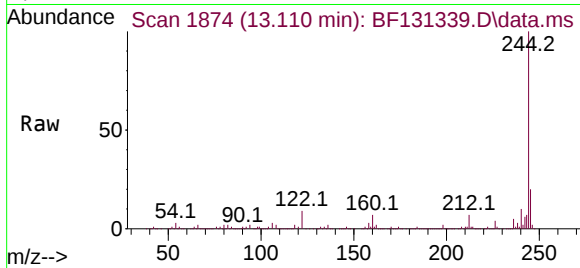

Tgt Ion:244 Resp: 841550
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.9 8.9
 122 8.7 7.5 11.3

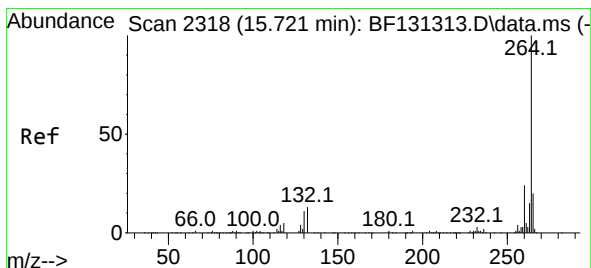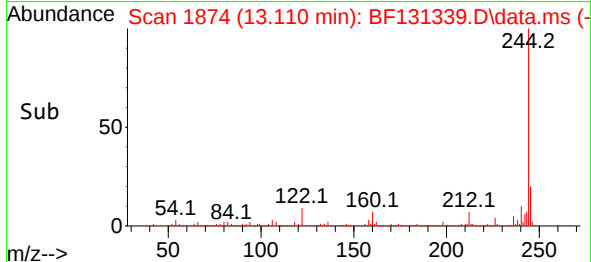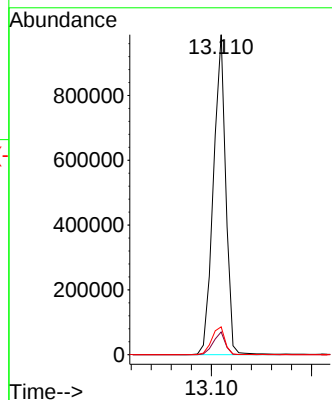

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.710 min Scan# 2316
 Delta R.T. -0.012 min
 Lab File: BF131339.D
 Acq: 22 Nov 2022 20:07

Tgt Ion:264 Resp: 200763
 Ion Ratio Lower Upper
 264 100
 260 23.6 19.0 28.4
 265 21.9 16.4 24.6

