

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112222\
 Data File : BF131328.D
 Acq On : 22 Nov 2022 13:36
 Operator : CG\JU
 Sample : PB149160BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB149160BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF131328.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.340	33	43	54	rVB	117519	169163	3.69%	0.648%
2	5.204	524	530	541	rVB	325262	470014	10.25%	1.800%
3	5.581	588	594	597	rBV	2807456	3301284	71.97%	12.640%
4	6.581	757	764	767	rBV	2770677	3247215	70.79%	12.433%
5	6.963	825	829	832	rBV	887835	687268	14.98%	2.632%
6	7.528	919	925	928	rBV	1848095	2166575	47.23%	8.296%
7	8.251	1043	1048	1052	rBV	1005958	904920	19.73%	3.465%
8	9.334	1226	1232	1235	rBV	4045388	4019166	87.62%	15.389%
9	10.016	1343	1348	1352	rBV	1293633	1106446	24.12%	4.237%
10	10.810	1476	1483	1487	rBV	2585103	2646400	57.70%	10.133%
11	11.516	1599	1603	1606	rBV	1395994	1206109	26.29%	4.618%
12	13.116	1870	1875	1878	rBV	4459732	4586853	100.00%	17.563%
13	14.169	2050	2054	2058	rBV	1086169	930650	20.29%	3.563%
14	15.710	2310	2316	2322	rBV	516351	674746	14.71%	2.584%




Sum of corrected areas: 26116809

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112222\
Data File : BF131328.D
Acq On : 22 Nov 2022 13:36
Operator : CG\JU
Sample : PB149160BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB149160BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

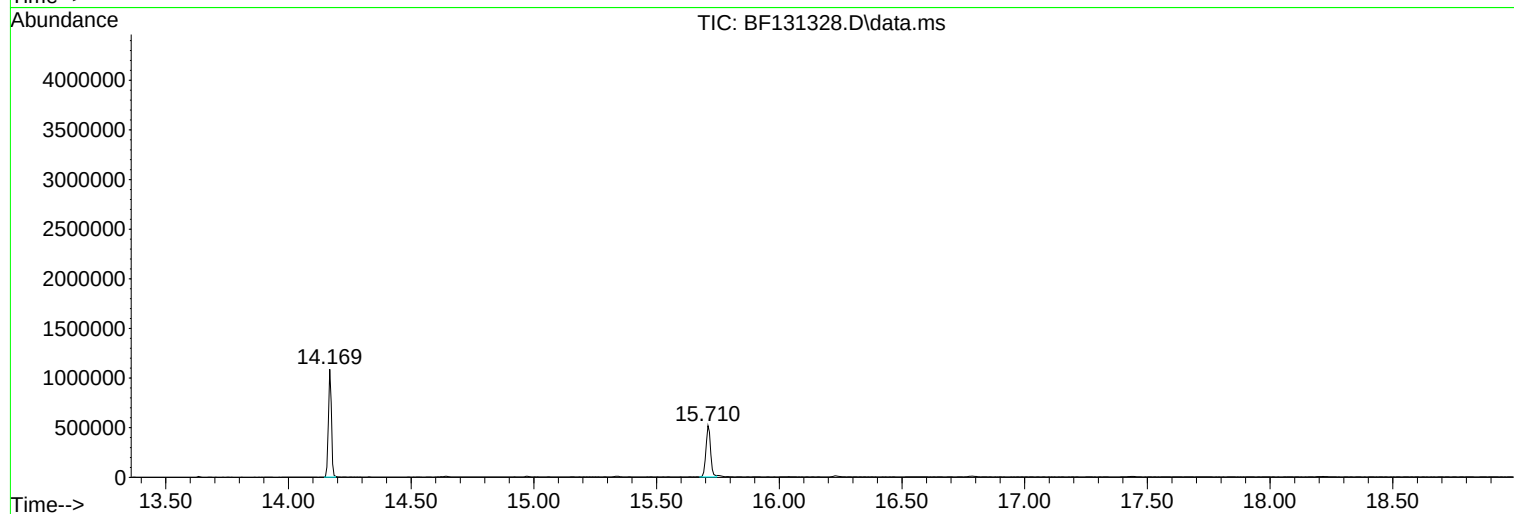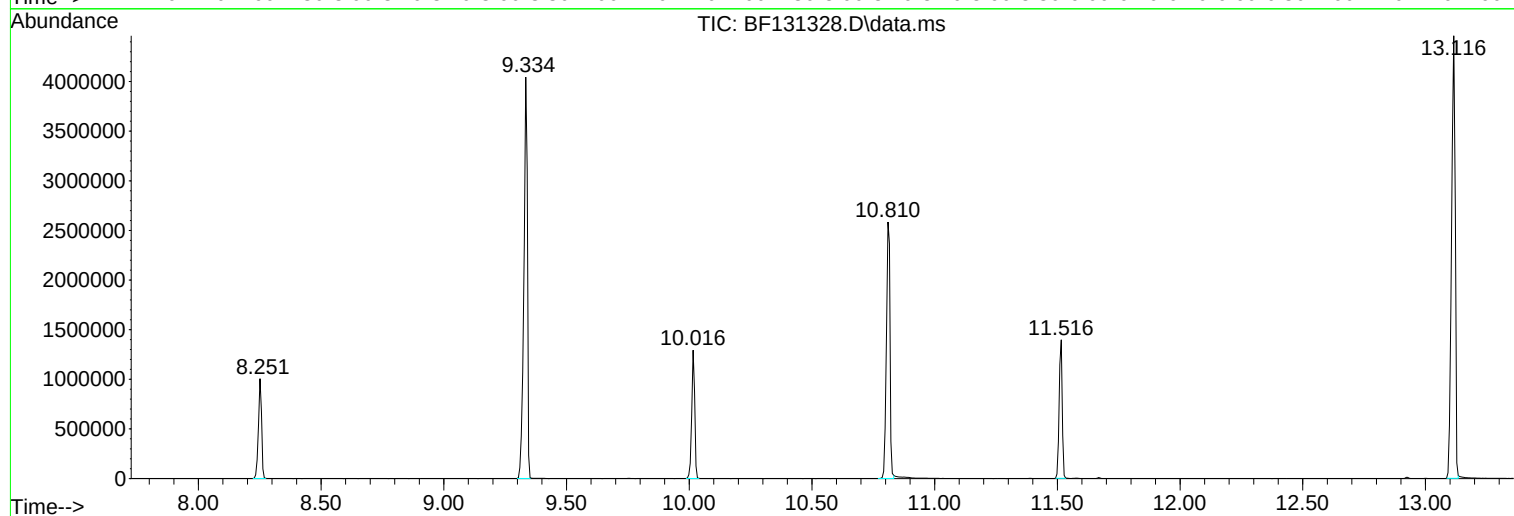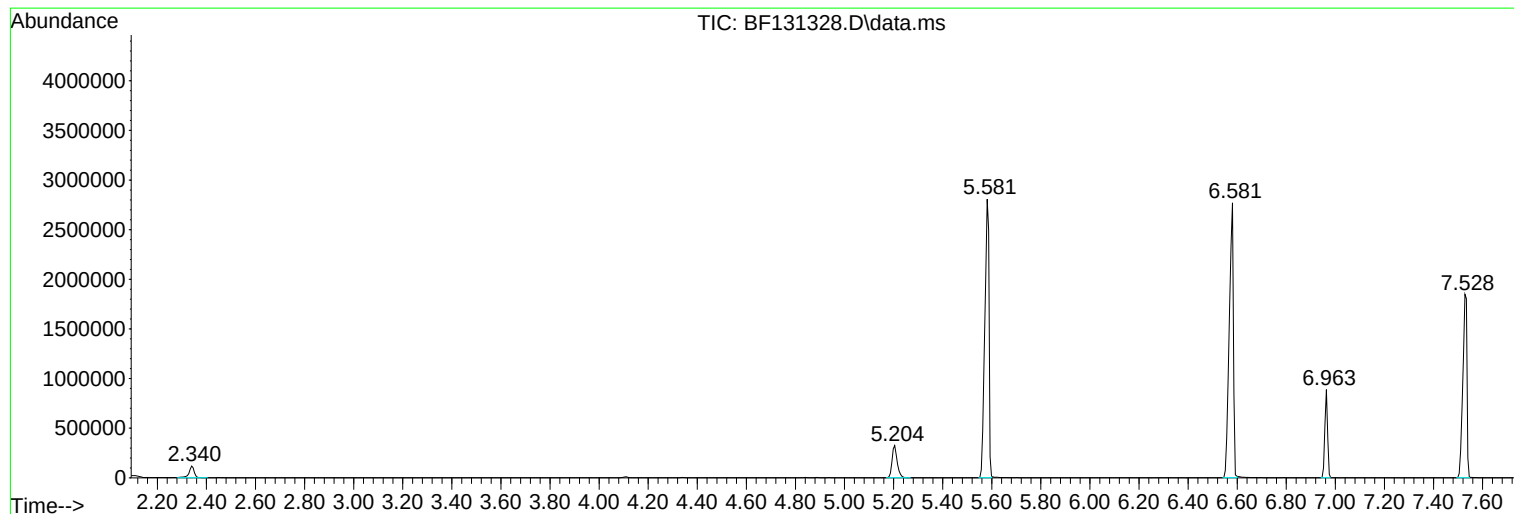

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112222\
Data File : BF131328.D
Acq On : 22 Nov 2022 13:36
Operator : CG\JU
Sample : PB149160BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB149160BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.340	4.92 ng	169163	1,4-Dichlorobenzene-d4	6.963

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	28
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	12
5			Boronic acid, ethyl-, dimethyl e...	102	C4H11BO2	007318-82-3	12

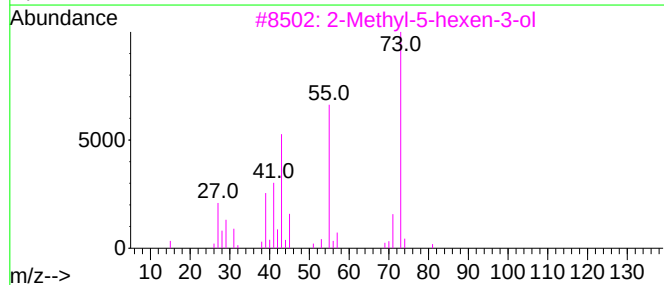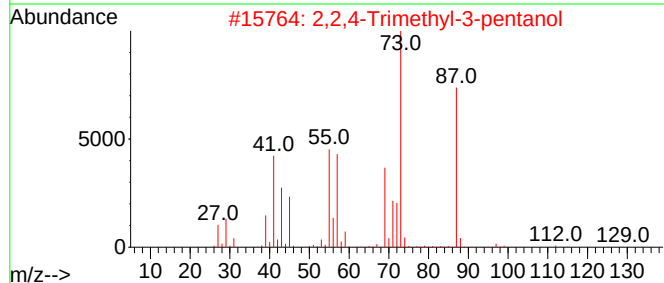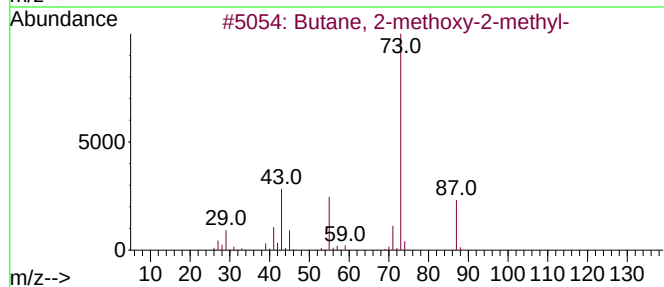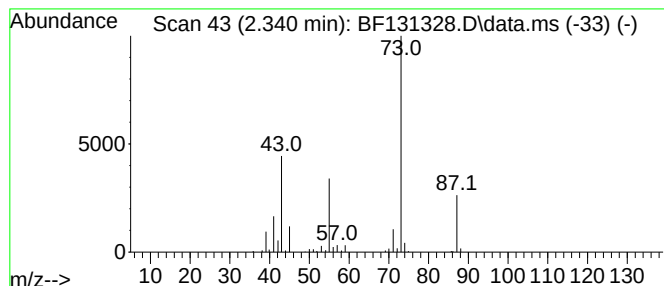

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112222\
Data File : BF131328.D
Acq On : 22 Nov 2022 13:36
Operator : CG\JU
Sample : PB149160BL
Misc :
ALS Vial : 9 Sample Multiplier: 1









Instrument :
BNA_F
ClientSampleId :
PB149160BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
5.204	13.68 ng	470014	1,4-Dichlorobenzene-d4	6.963	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	78
2	Acetone	58	C3H6O	000067-64-1	14
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12
4	5-Aminovaleric acid	117	C5H11NO2	000660-88-8	9
5	5-Oxohexanenitrile	111	C6H9NO	010412-98-3	9

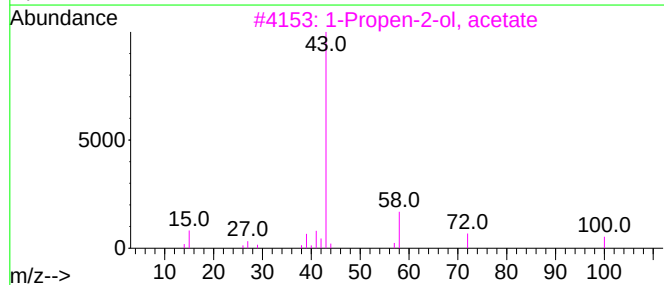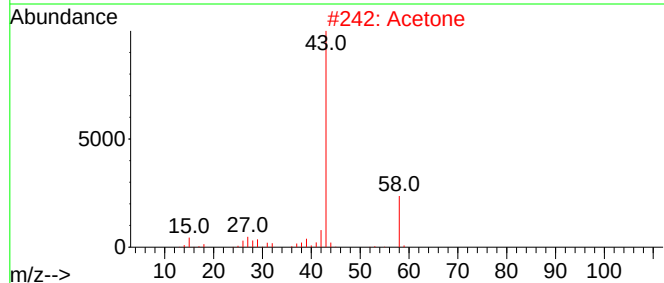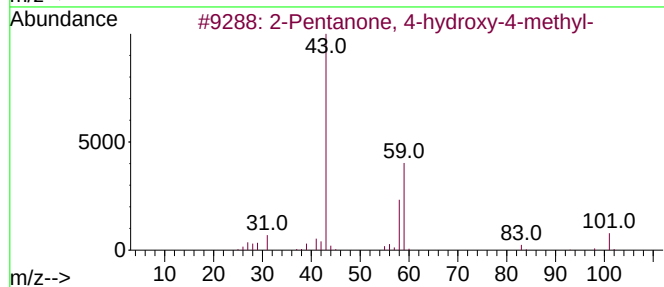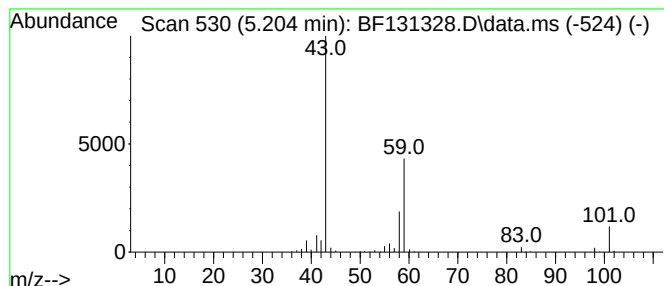

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112222\
Data File : BF131328.D
Acq On : 22 Nov 2022 13:36
Operator : CG\JU
Sample : PB149160BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB149160BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.340	4.9	ng	169163	1	6.963	687268	20.0
2-Pentanone, 4-...	5.204	13.7	ng	470014	1	6.963	687268	20.0