


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112222\
Data File : BF131320.D
Acq On : 22 Nov 2022 08:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 22 01:17:52 2022

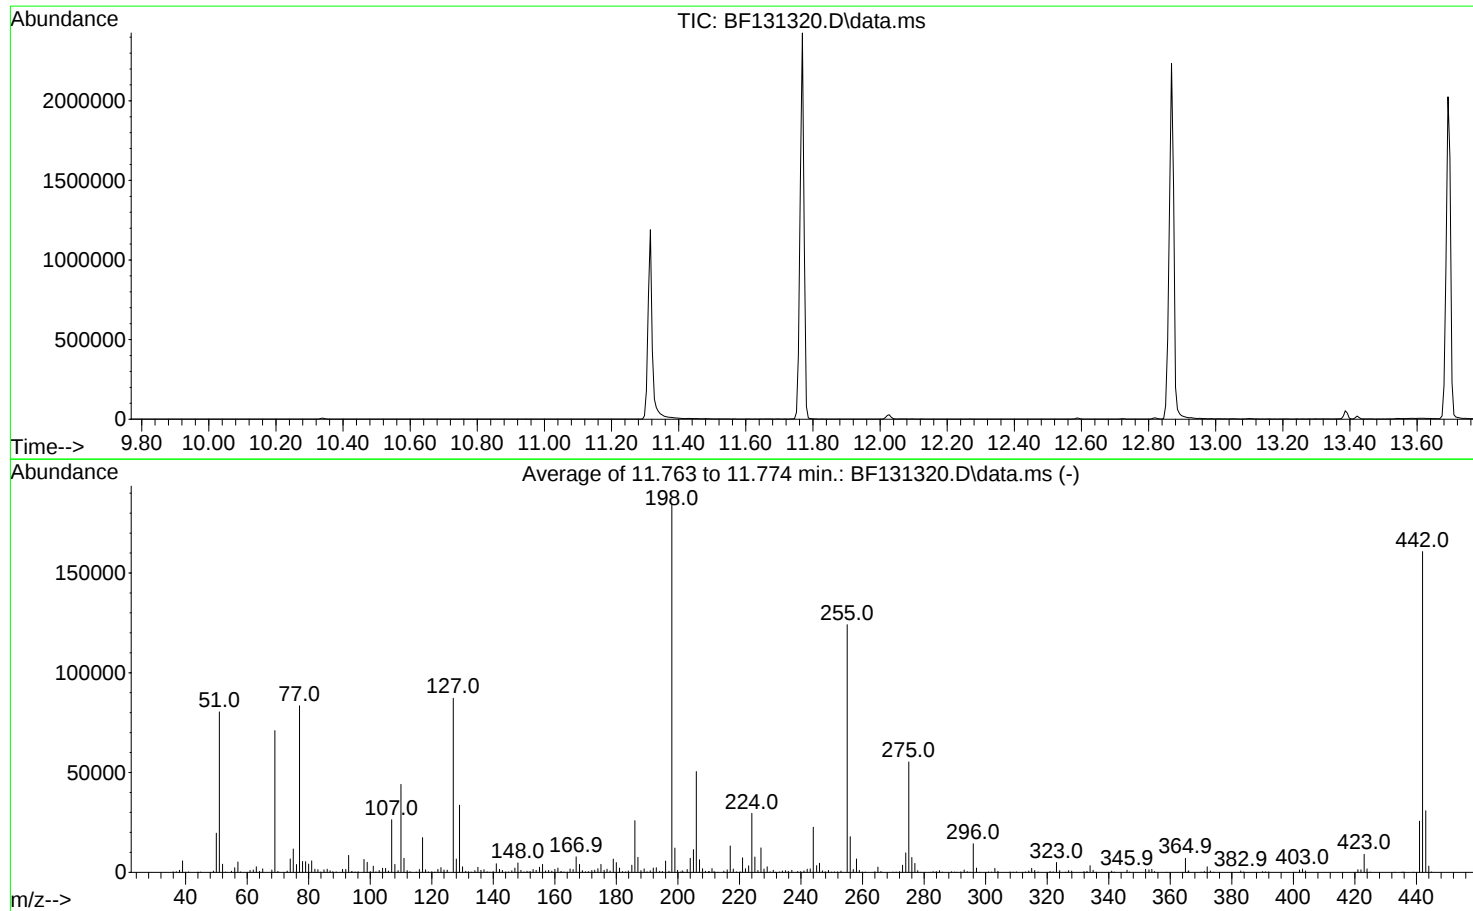




AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.6	80397	PASS
68	69	0.00	2	1.7	1182	PASS
69	198	0.00	100	38.5	71027	PASS
70	69	0.00	2	0.6	427	PASS
127	198	10	80	47.3	87176	PASS
197	198	0.00	2	0.3	534	PASS
198	198	100	100	100.0	184368	PASS
199	198	5	9	6.6	12158	PASS
275	198	10	60	30.0	55272	PASS
365	198	1	100	3.8	7058	PASS
441	198	0.01	100	13.9	25649	PASS
442	442	50	100	100.0	160741	PASS
443	442	15	24	19.2	30859	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112222\
Data File : BF131320.D
Acq On : 22 Nov 2022 08:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 23 07:32:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 01:17:52 2022
Response via : Initial Calibration

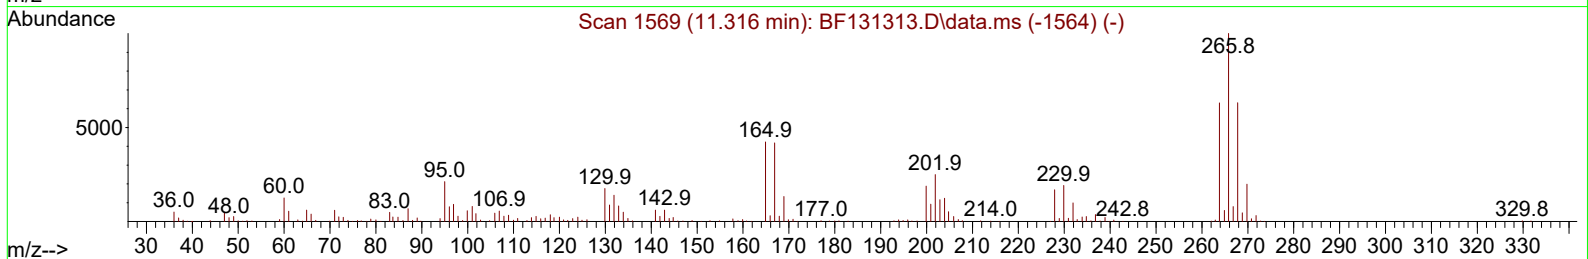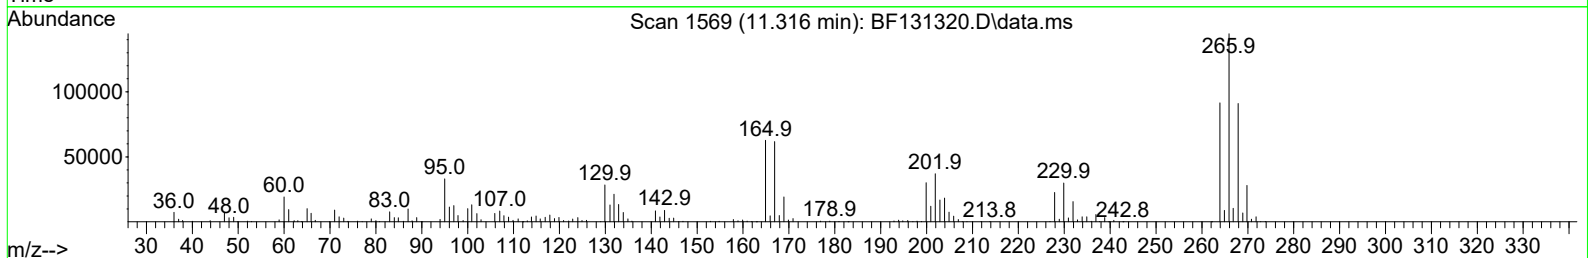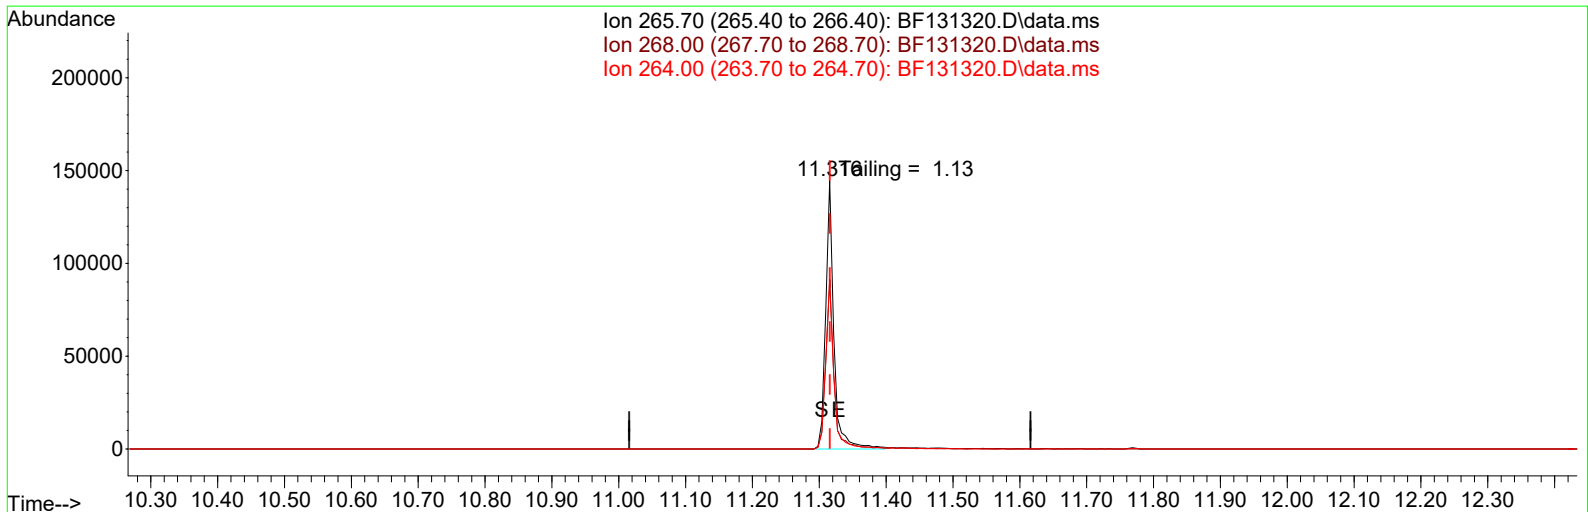

TIC: BF131320.D\data.ms

(70) Pentachlorophenol (C)

11.316min (-0.000) 132876.84 ng




response 125136

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	62.94
264.00	63.00	63.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112222\
Data File : BF131320.D
Acq On : 22 Nov 2022 08:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 23 07:32:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 01:17:52 2022
Response via : Initial Calibration

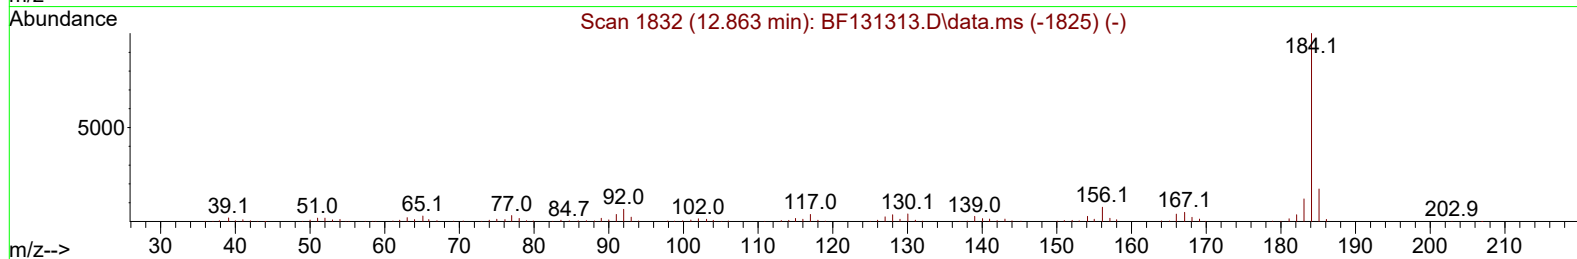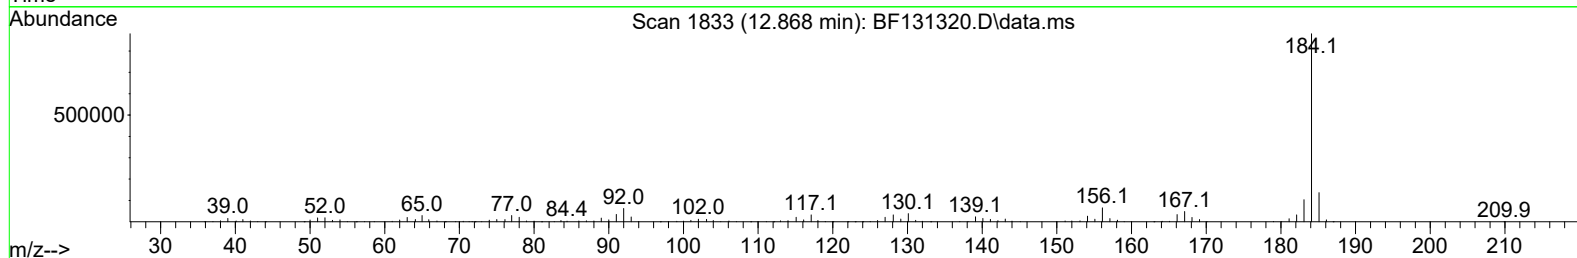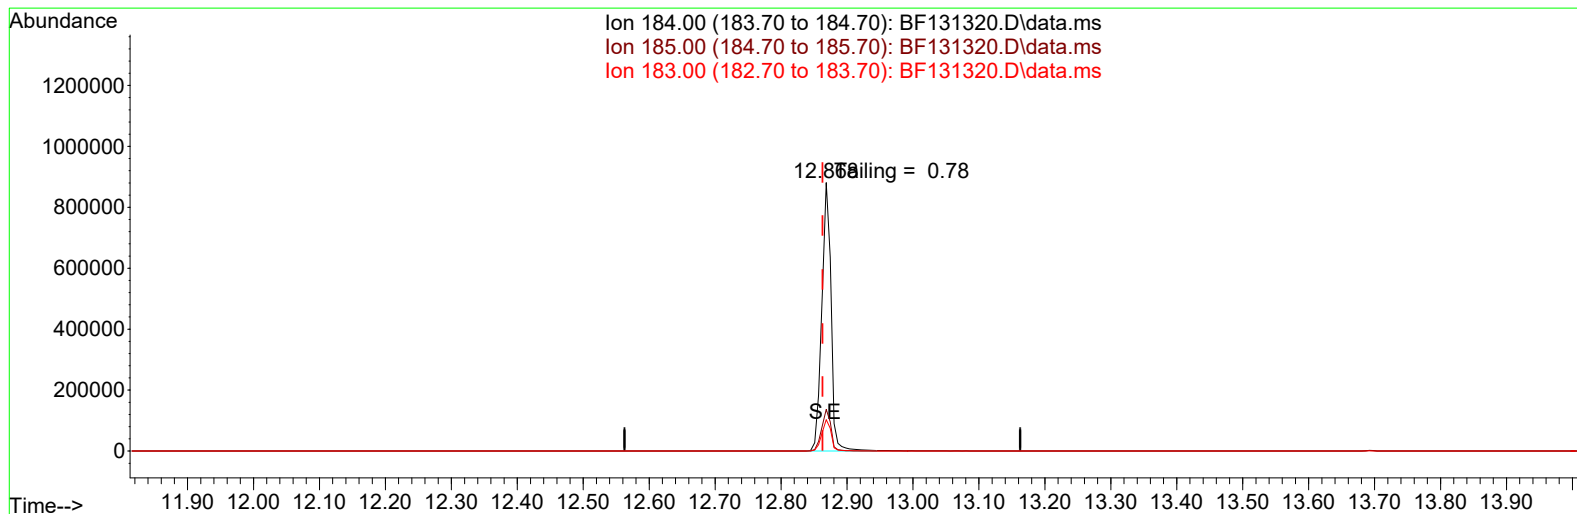

TIC: BF131320.D\data.ms

(77) Benzidine

12.868min (+ 0.006) 0.00 ng

response 861302

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	15.50
183.00	12.00	11.73
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/22/2022	BNA_F	<u>BF131320.D</u>
Compound Name	Response	Retention Time
DDT	303929	13.692
DDD	10456	13.386
DDE	337	13.051
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10793	314722	3.43

Instrument :
BNA_F
ClientSampleId :
DFTPP