


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112222\
 Data File : BF131331.D
 Acq On : 22 Nov 2022 15:36
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 22 01:17:52 2022

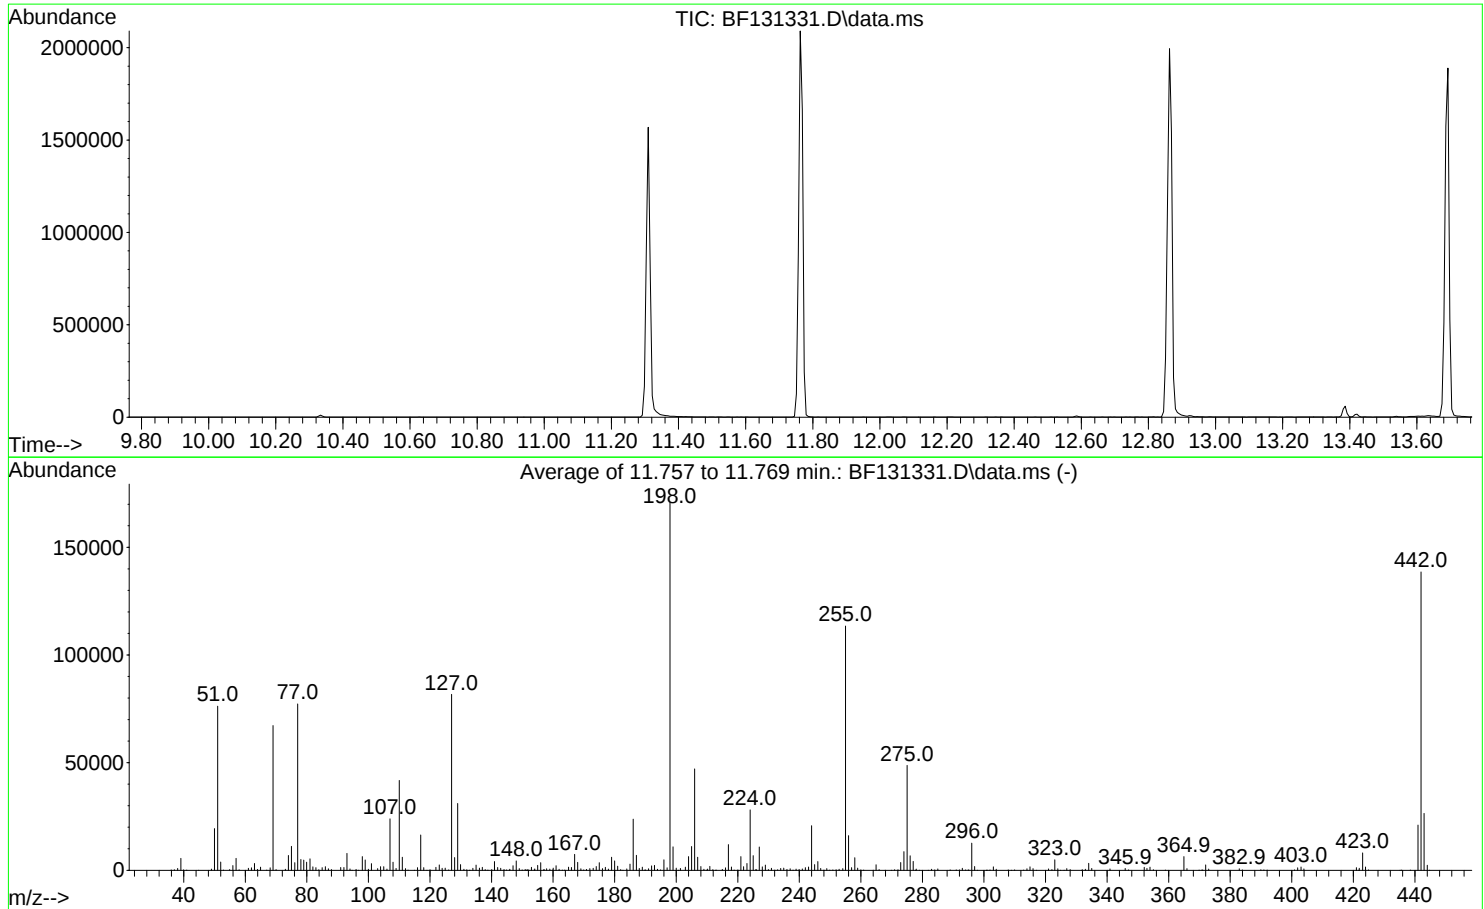




AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1639

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.6	76181	PASS
68	69	0.00	2	1.7	1160	PASS
69	198	0.00	100	39.4	67232	PASS
70	69	0.00	2	0.5	359	PASS
127	198	10	80	47.8	81704	PASS
197	198	0.00	2	0.7	1160	PASS
198	198	100	100	100.0	170845	PASS
199	198	5	9	6.4	10902	PASS
275	198	10	60	28.5	48680	PASS
365	198	1	100	3.7	6364	PASS
441	198	0.01	100	12.3	21027	PASS
442	442	50	100	100.0	138523	PASS
443	442	15	24	19.1	26441	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112222\
Data File : BF131331.D
Acq On : 22 Nov 2022 15:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 23 07:34:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 01:17:52 2022
Response via : Initial Calibration

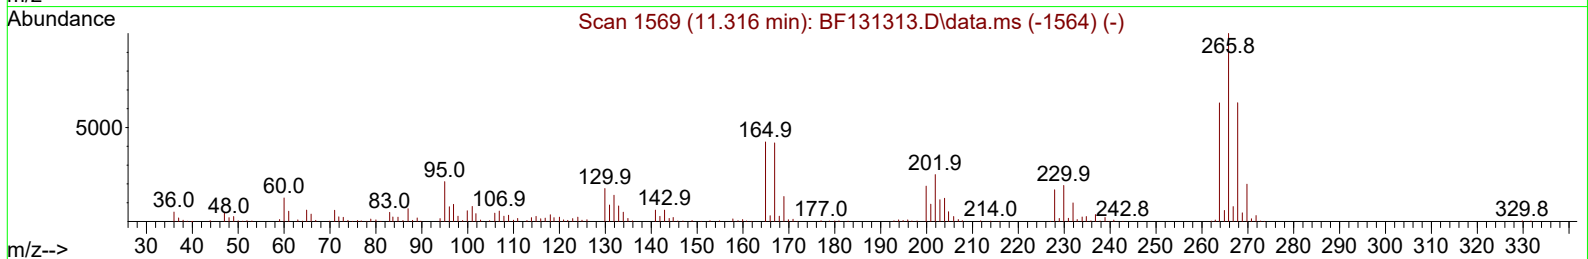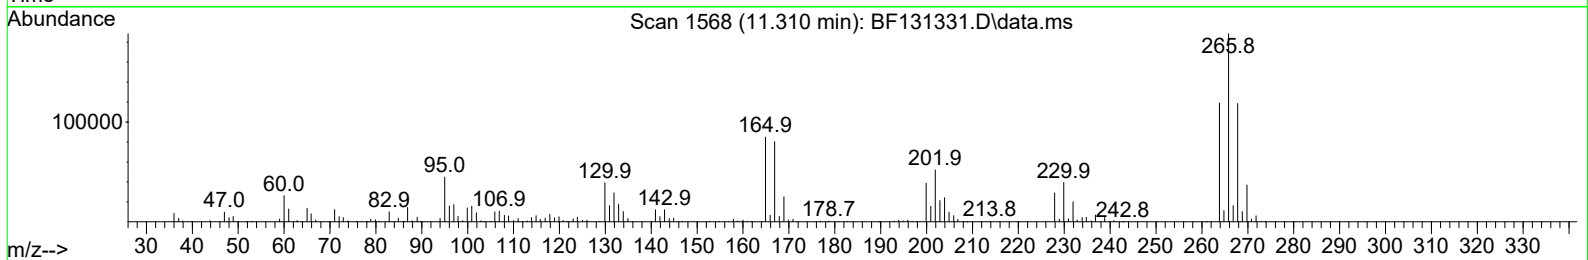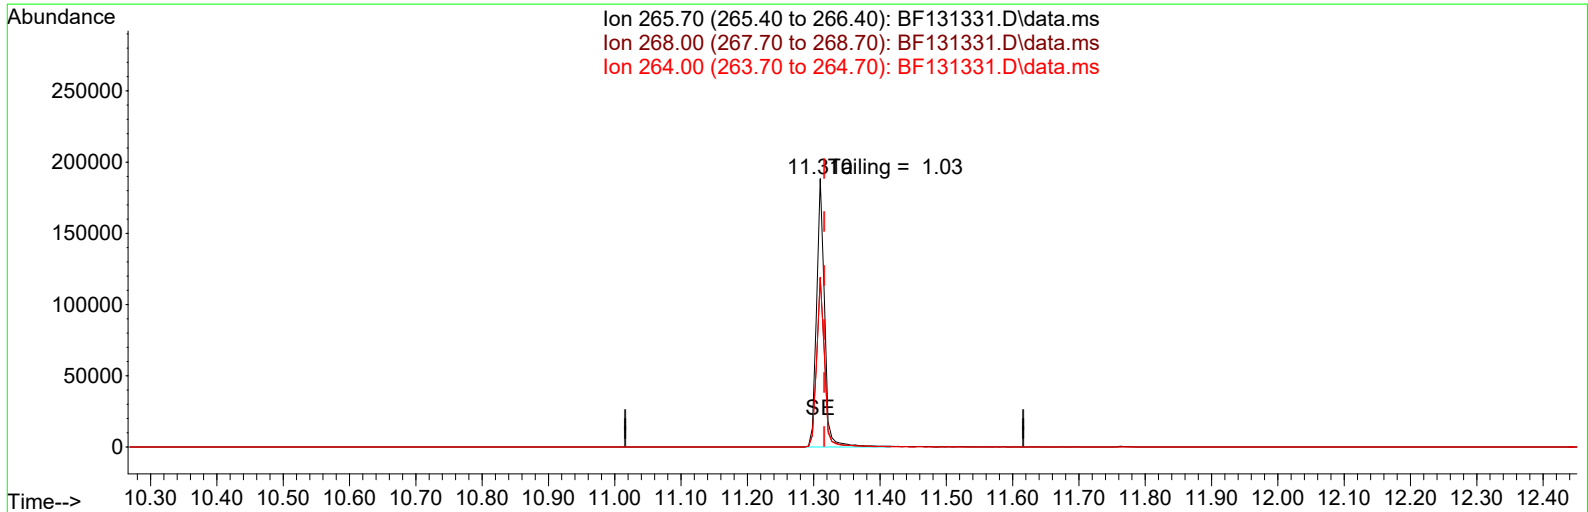

TIC: BF131331.D\data.ms

(70) Pentachlorophenol (C)

11.310min (-0.006) 22169.58 ng




response 158787

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	62.96
264.00	63.00	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112222\
Data File : BF131331.D
Acq On : 22 Nov 2022 15:36
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 23 07:34:28 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 22 01:17:52 2022
Response via : Initial Calibration

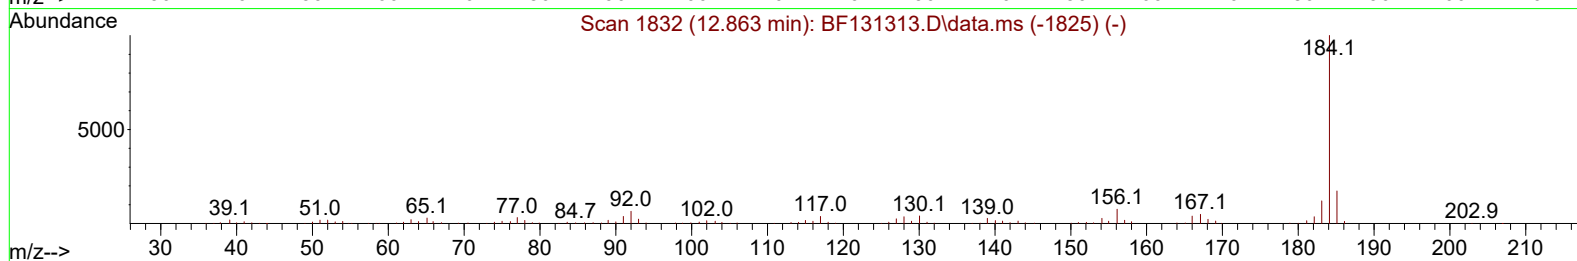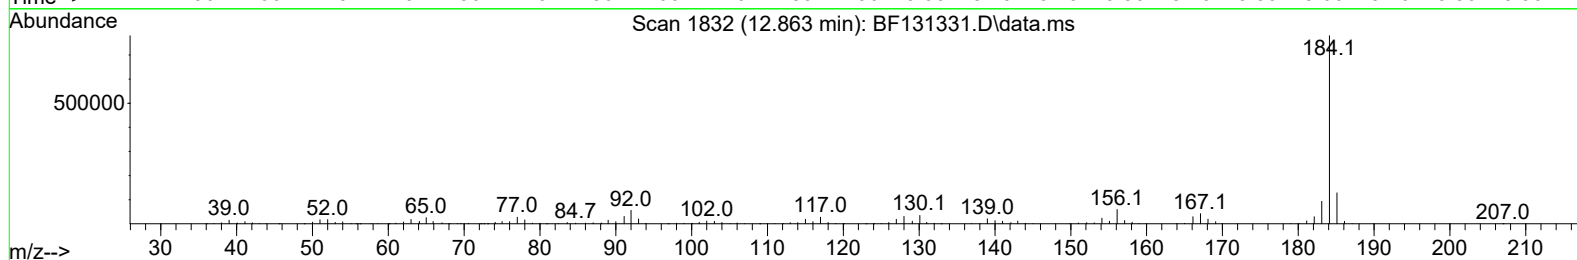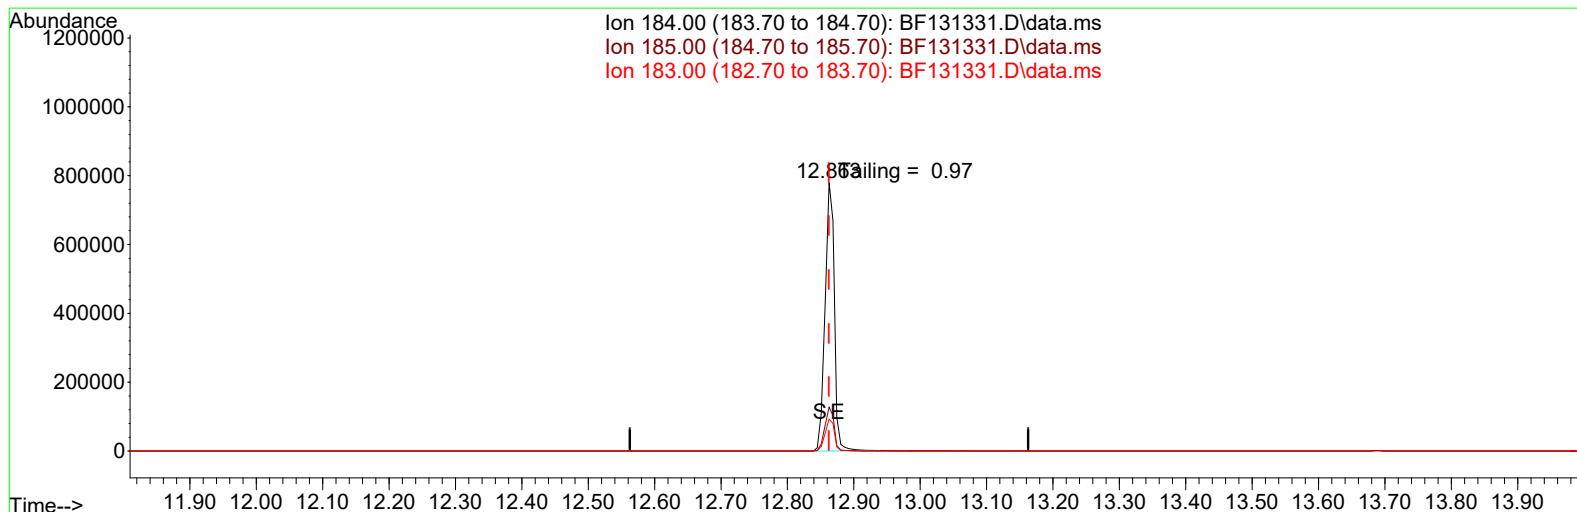

TIC: BF131331.D\data.ms

(77) Benzidine

12.863min (+ 0.000) 0.00 ng

response 761477

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	16.43
183.00	12.00	11.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/22/2022	BNA_F	<u>BF131331.D</u>
Compound Name	Response	Retention Time
DDT	307944	13.692
DDD	12257	13.386
DDE	267	13.045
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12524	320468	3.91

Instrument :
BNA_F
ClientSampleId :
DFTPP