

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112224\
 Data File : BF140568.D
 Acq On : 22 Nov 2024 11:10
 Operator : RC/JU
 Sample : P4910-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MH-COTTAGE

Quant Time: Nov 22 11:38:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 21 15:23:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.869	152	90391	20.000	ng	0.00
21) Naphthalene-d8	8.151	136	340003	20.000	ng	0.00
39) Acenaphthene-d10	9.904	164	188041	20.000	ng	-0.01
64) Phenanthrene-d10	11.398	188	346986	20.000	ng	0.00
76) Chrysene-d12	14.045	240	224754	20.000	ng	0.00
86) Perylene-d12	15.539	264	204242	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.510	112	731166	138.014	ng	0.01
7) Phenol-d6	6.510	99	929222	132.675	ng	0.00
23) Nitrobenzene-d5	7.434	82	635351	95.583	ng	0.00
42) 2,4,6-Tribromophenol	10.704	330	293011	145.696	ng	0.00
45) 2-Fluorobiphenyl	9.228	172	1169491	92.665	ng	0.00
79) Terphenyl-d14	12.986	244	1361281	94.312	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112224\
Data File : BF140568.D
Acq On : 22 Nov 2024 11:10
Operator : RC/JU
Sample : P4910-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-COTTAGE

Quant Time: Nov 22 11:38:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration




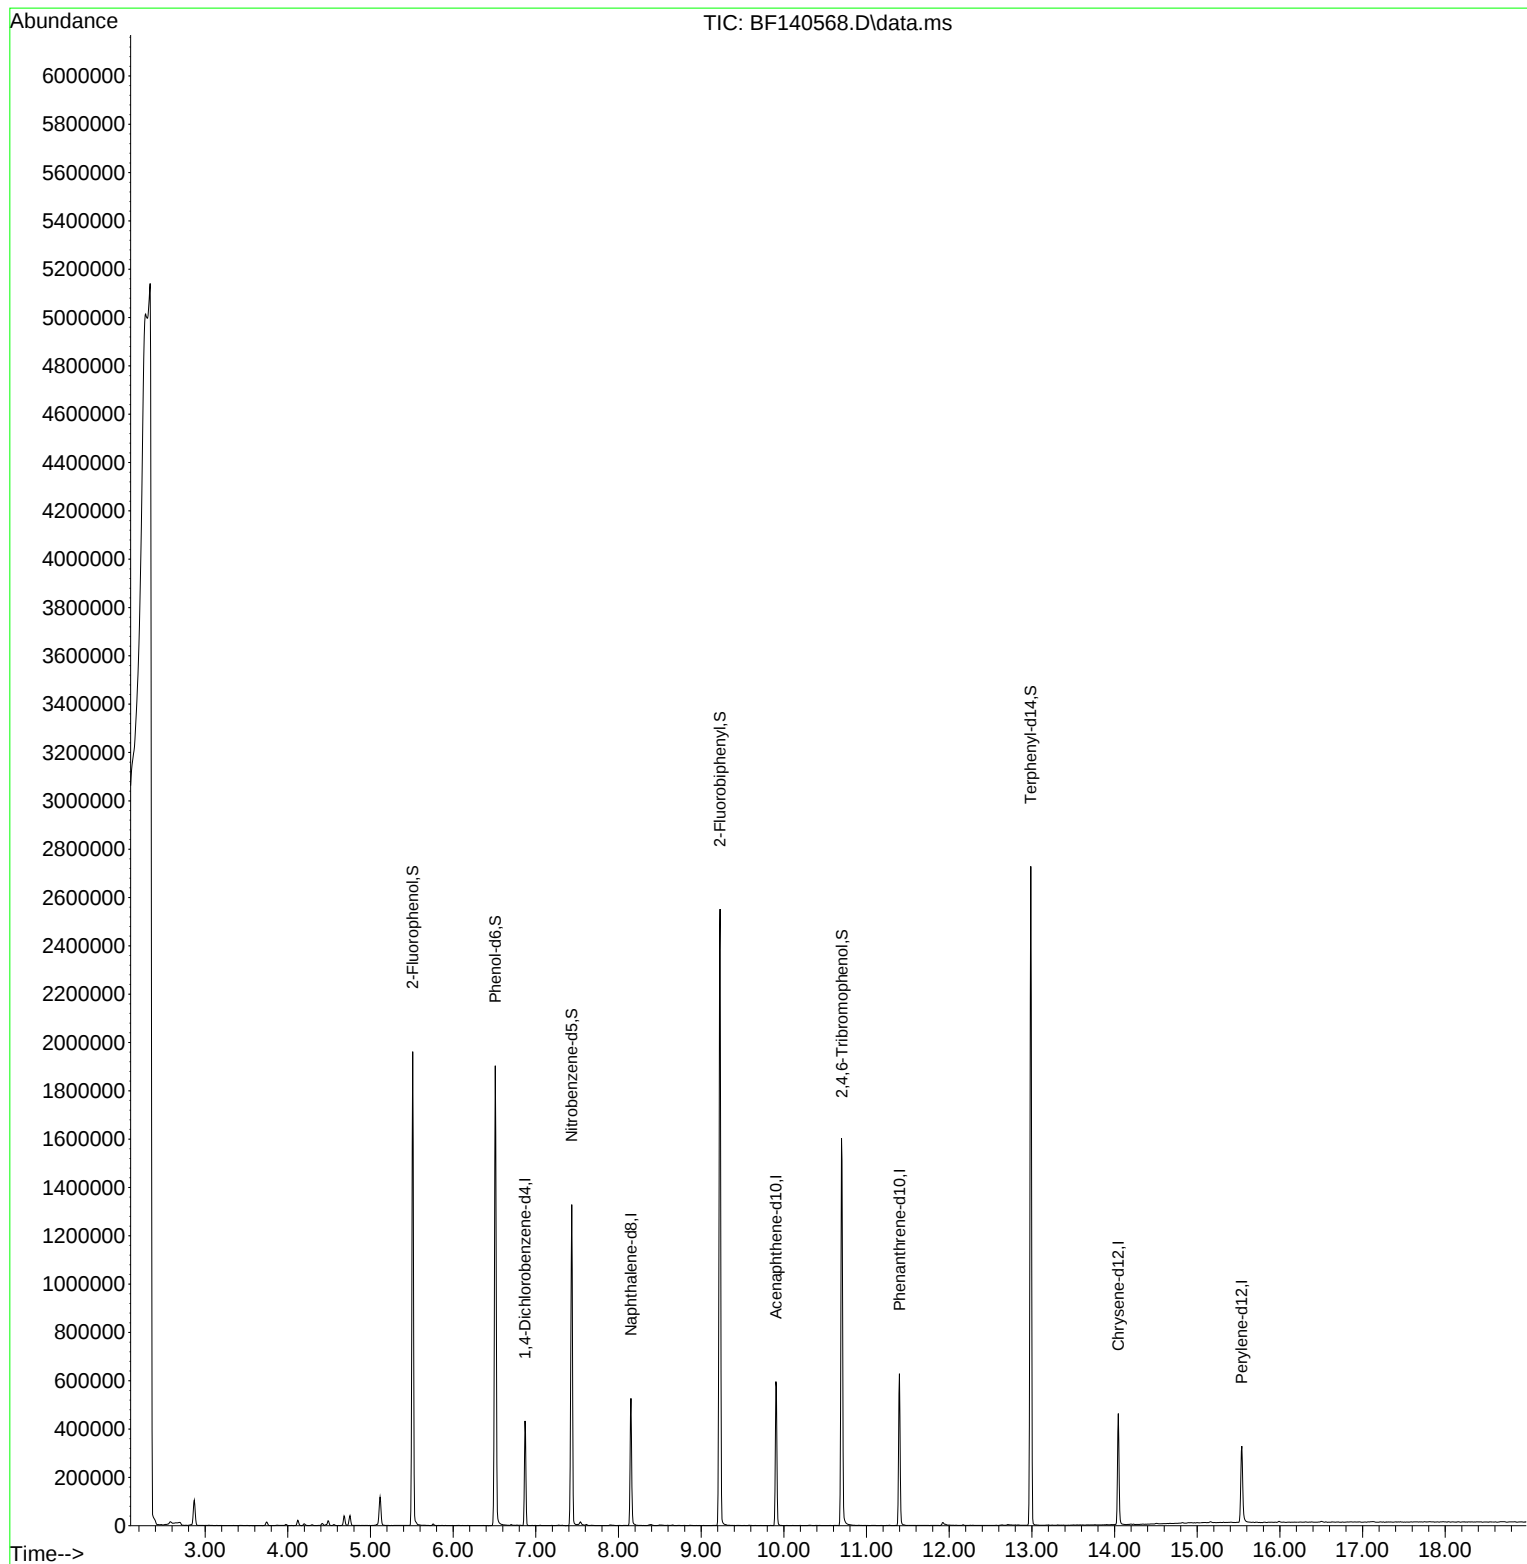


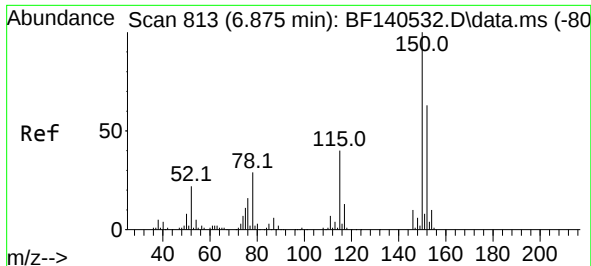

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.869 min Scan# 813
Delta R.T. -0.006 min
Lab File: BF140568.D
Acq: 22 Nov 2024 11:10




Instrument :
BNA_F
ClientSampleId :
MH-COTTAGE


Tgt Ion:152 Resp: 90391
Ion Ratio Lower Upper
152 100
150 156.8 128.5 192.7
115 61.7 50.2 75.4

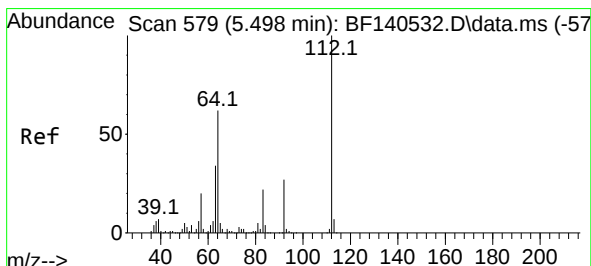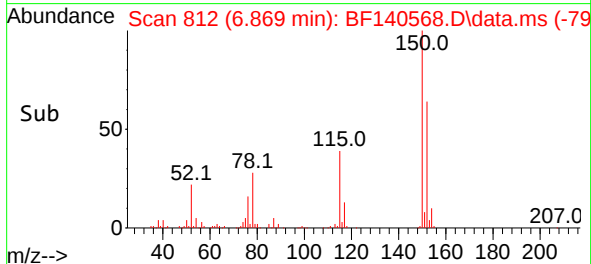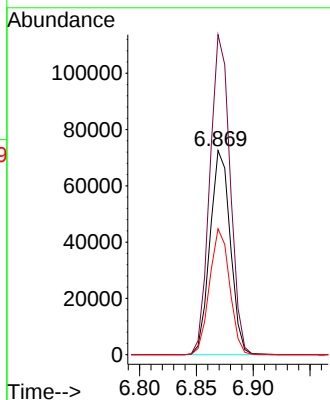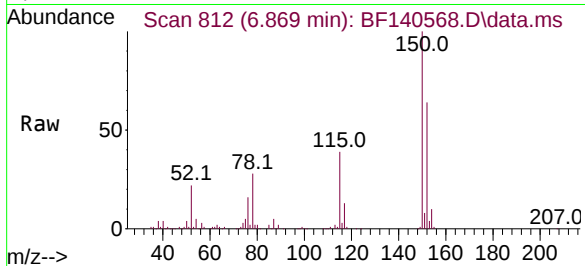

#5
2-Fluorophenol
Concen: 138.014 ng
RT: 5.510 min Scan# 581
Delta R.T. 0.012 min
Lab File: BF140568.D
Acq: 22 Nov 2024 11:10

Tgt Ion:112 Resp: 731166
Ion Ratio Lower Upper
112 100
64 59.8 49.2 73.8
63 32.0 27.0 40.4


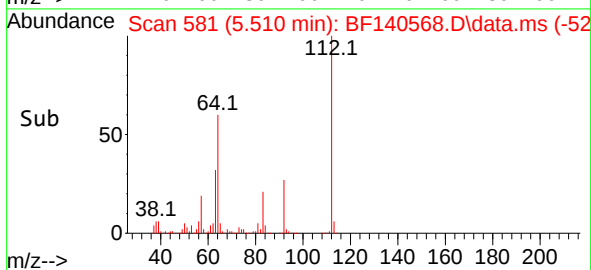
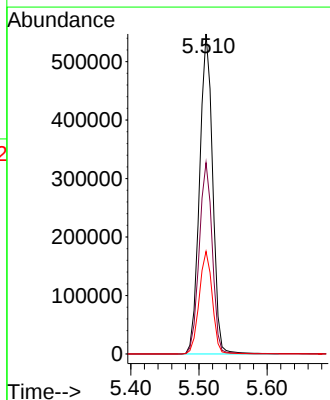
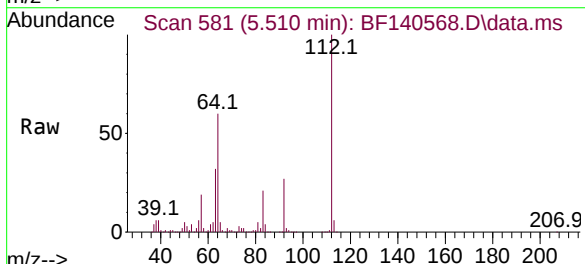


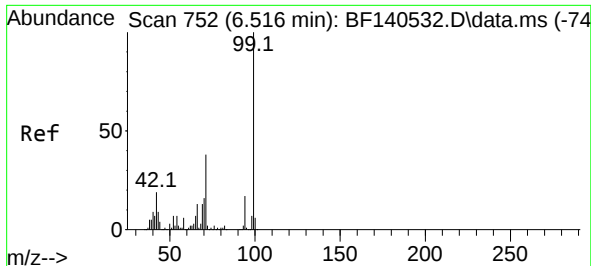

#7
Phenol-d6
Concen: 132.675 ng
RT: 6.510 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF140568.D
Acq: 22 Nov 2024 11:10




Instrument :
BNA_F
ClientSampleId :
MH-COTTAGE


Tgt Ion: 99 Resp: 929222
Ion Ratio Lower Upper
99 100
42 18.6 15.4 23.0
71 37.4 30.6 46.0

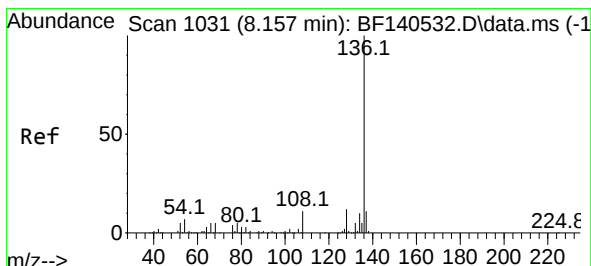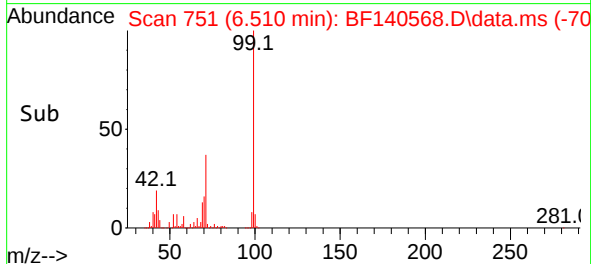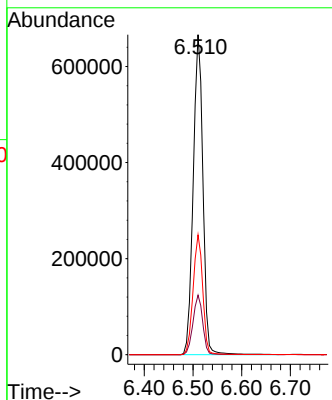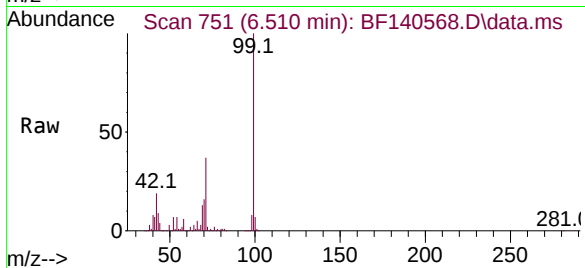

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.151 min Scan# 1030
Delta R.T. -0.006 min
Lab File: BF140568.D
Acq: 22 Nov 2024 11:10

Tgt Ion: 136 Resp: 340003
Ion Ratio Lower Upper
136 100
137 10.8 8.6 13.0
54 6.8 5.8 8.8
68 5.0 4.1 6.1


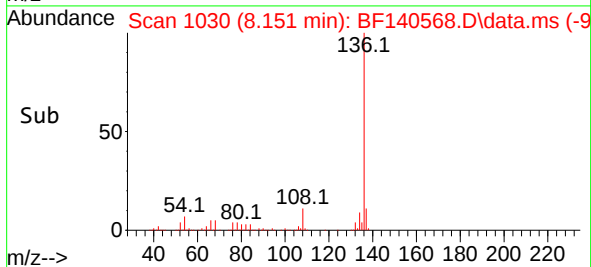
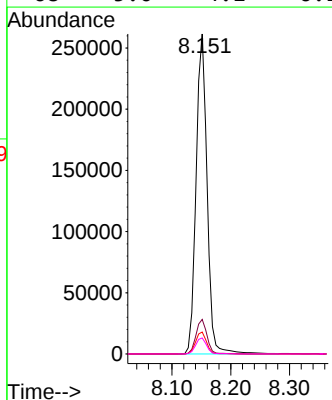
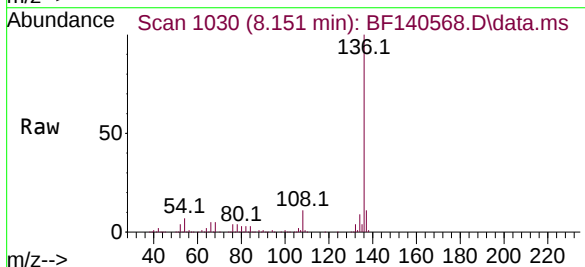


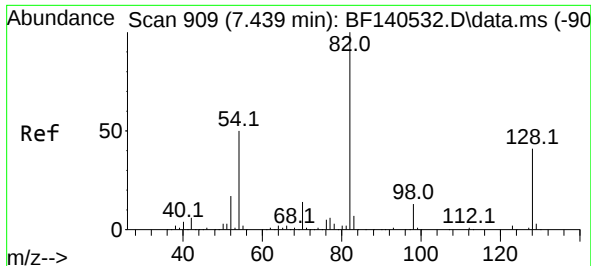

#23
 Nitrobenzene-d5
 Concen: 95.583 ng
 RT: 7.434 min Scan# 909
 Delta R.T. -0.006 min
 Lab File: BF140568.D
 Acq: 22 Nov 2024 11:10




Instrument :
 BNA_F
 ClientSampleId :
 MH-COTTAGE


Tgt Ion: 82 Resp: 635351
 Ion Ratio Lower Upper
 82 100
 128 42.0 33.0 49.4
 54 48.6 39.5 59.3

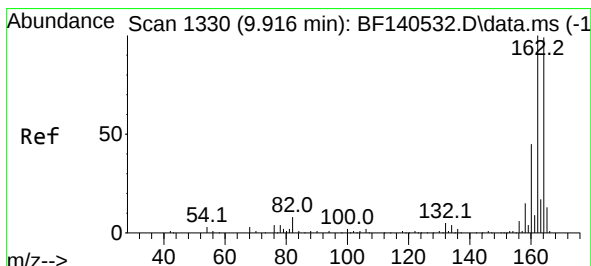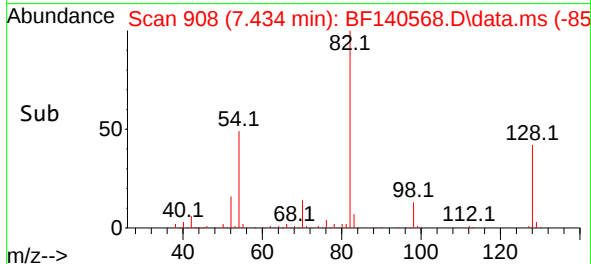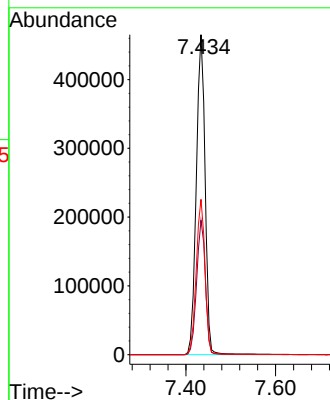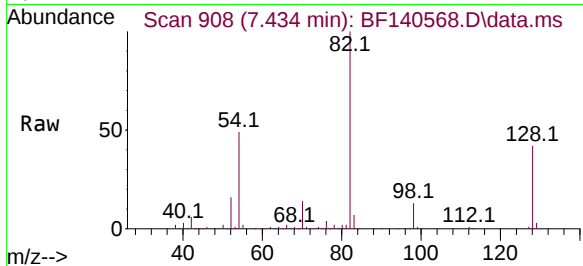

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.904 min Scan# 1328
 Delta R.T. -0.012 min
 Lab File: BF140568.D
 Acq: 22 Nov 2024 11:10


Tgt Ion:164 Resp: 188041
 Ion Ratio Lower Upper
 164 100
 162 100.2 80.6 120.8
 160 44.7 36.2 54.4

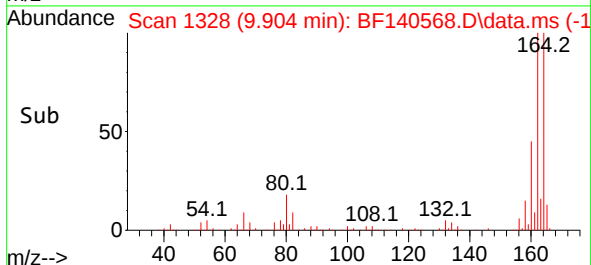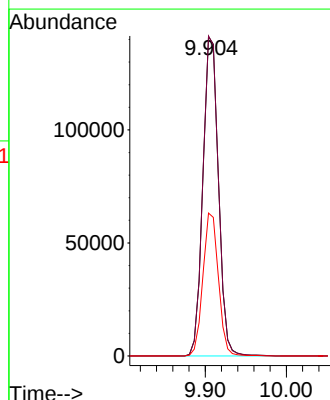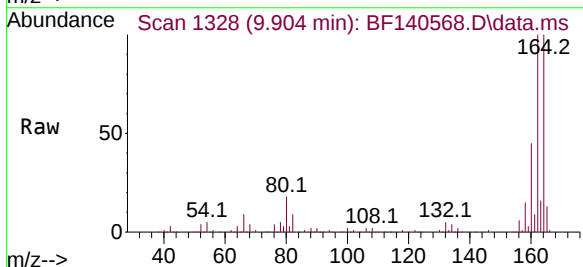



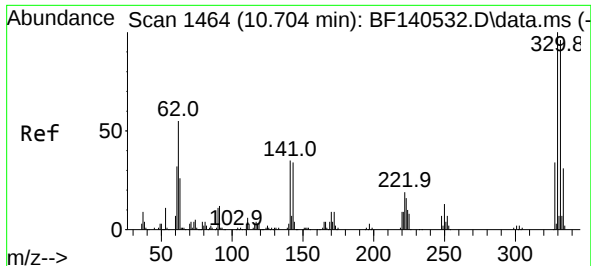


#42
2,4,6-Tribromophenol
Concen: 145.696 ng
RT: 10.704 min Scan# 1464
Delta R.T. 0.000 min
Lab File: BF140568.D
Acq: 22 Nov 2024 11:10

Instrument :
BNA_F
ClientSampleId :
MH-COTTAGE



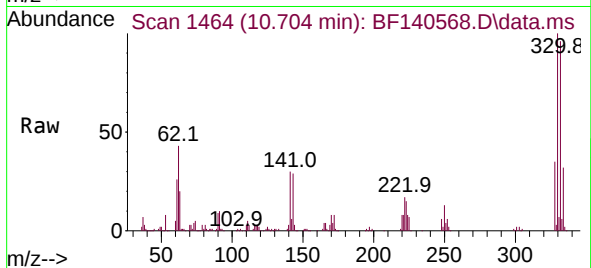



Tgt Ion:330 Resp: 293011
Ion Ratio Lower Upper
330 100
332 95.0 76.9 115.3
141 33.1 26.7 40.1

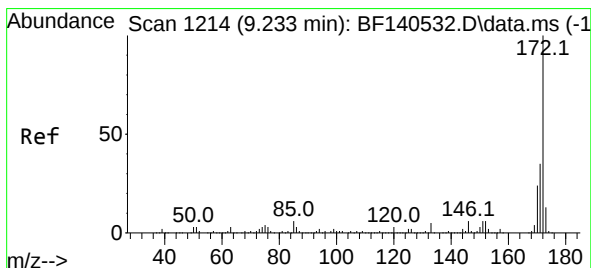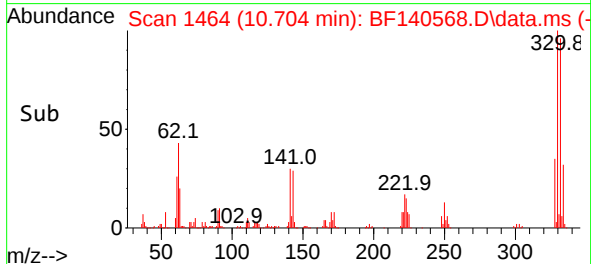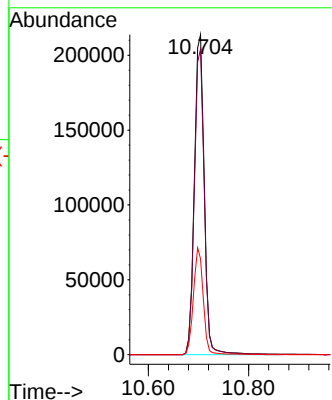

#45
2-Fluorobiphenyl
Concen: 92.665 ng
RT: 9.228 min Scan# 1213
Delta R.T. -0.006 min
Lab File: BF140568.D
Acq: 22 Nov 2024 11:10

Tgt Ion:172 Resp: 1169491
Ion Ratio Lower Upper
172 100
171 35.7 28.4 42.6
170 23.5 19.0 28.6


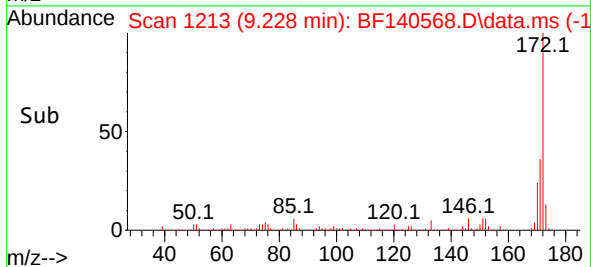
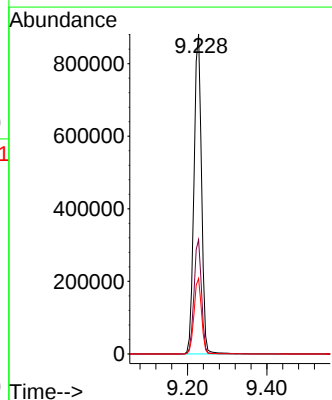
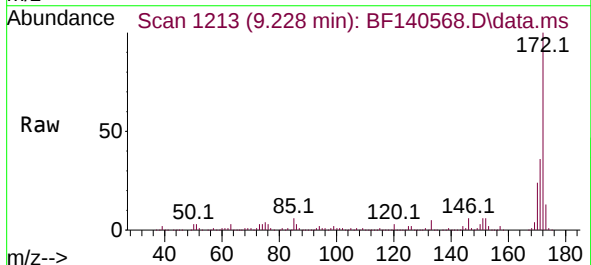


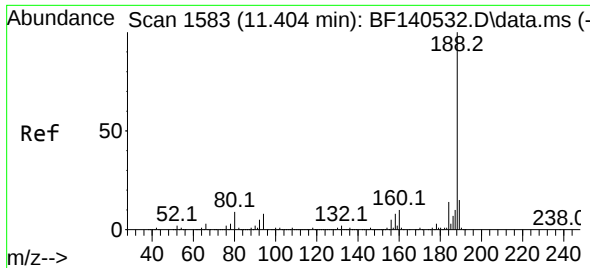

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.398 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF140568.D
Acq: 22 Nov 2024 11:10




Instrument :
BNA_F
ClientSampleId :
MH-COTTAGE


Tgt Ion:188 Resp: 346986
Ion Ratio Lower Upper
188 100
94 8.2 6.4 9.6
80 8.8 6.9 10.3

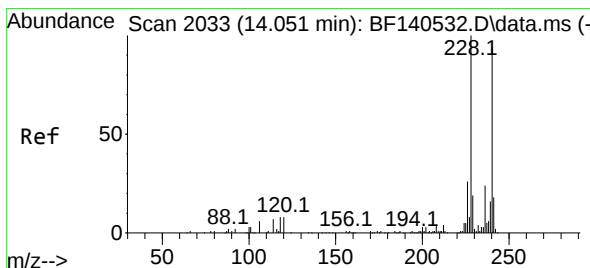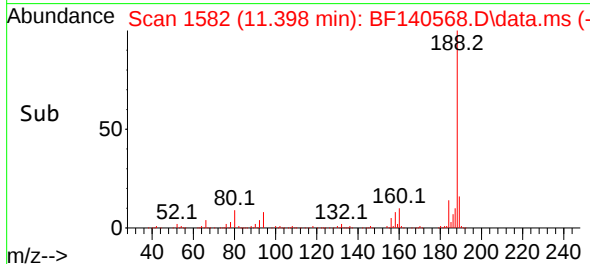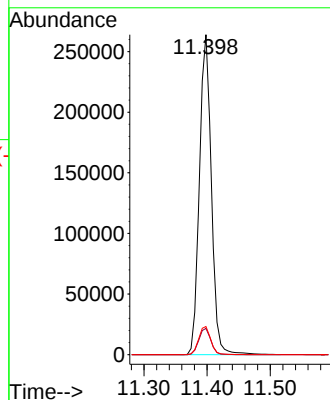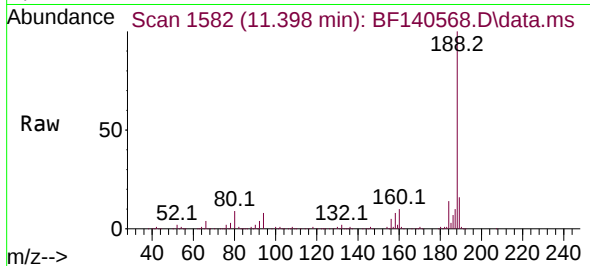

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.045 min Scan# 2032
Delta R.T. -0.006 min
Lab File: BF140568.D
Acq: 22 Nov 2024 11:10


Tgt Ion:240 Resp: 224754
Ion Ratio Lower Upper
240 100
120 9.6 7.3 10.9
236 26.1 20.6 31.0

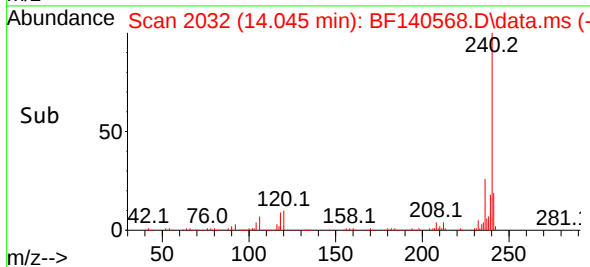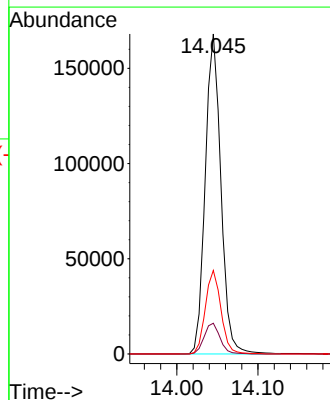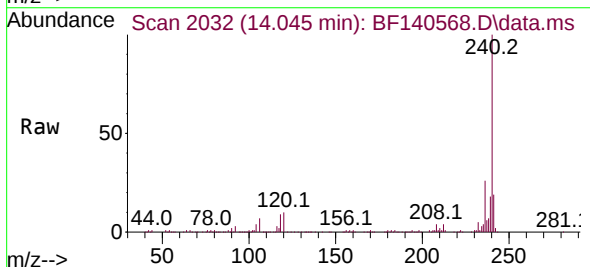



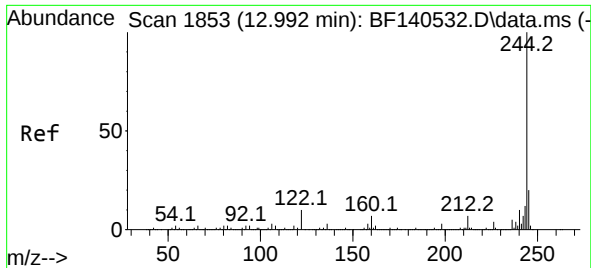


#79
Terphenyl-d14
Concen: 94.312 ng
RT: 12.986 min Scan# 1852
Delta R.T. -0.006 min
Lab File: BF140568.D
Acq: 22 Nov 2024 11:10

Instrument :
BNA_F
ClientSampleId :
MH-COTTAGE

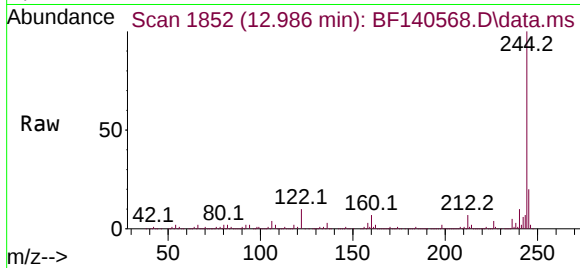

Tgt Ion:244 Resp: 1361281
Ion Ratio Lower Upper
244 100
212 7.2 5.8 8.8
122 10.2 8.0 12.0

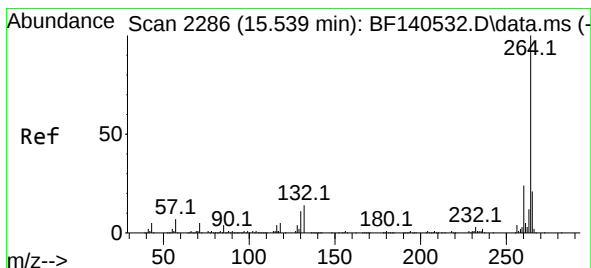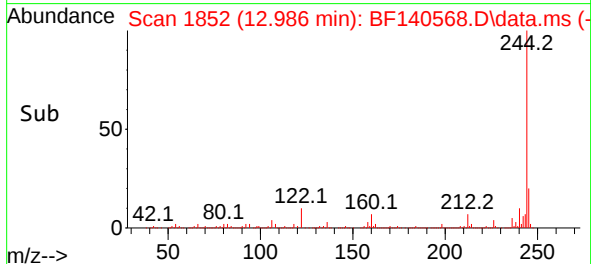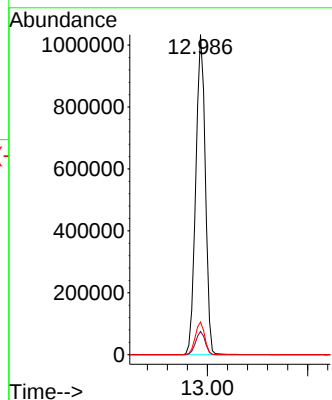

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.539 min Scan# 2286
Delta R.T. 0.000 min
Lab File: BF140568.D
Acq: 22 Nov 2024 11:10

Tgt Ion:264 Resp: 204242
Ion Ratio Lower Upper
264 100
260 23.7 19.0 28.6
265 20.6 16.6 25.0

