

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112224\
Data File : BF140565.D
Acq On : 22 Nov 2024 09:46
Operator : RC/JU
Sample : PB165129BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165129BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140565.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.252	13	27	37	rVB	41084	72598	1.64%	0.302%
2	5.510	575	581	603	rBV	2204595	3045958	68.83%	12.654%
3	6.510	744	751	756	rBV	2120697	3127675	70.68%	12.994%
4	6.869	807	812	817	rBV	485417	591822	13.37%	2.459%
5	7.434	901	908	913	rBV	1434318	2082882	47.07%	8.653%
6	8.151	1023	1030	1041	rBV	564720	768137	17.36%	3.191%
7	9.228	1205	1213	1218	rBV	2924824	4118198	93.06%	17.109%
8	9.904	1322	1328	1342	rBV	680069	925126	20.91%	3.843%
9	10.704	1457	1464	1489	rBV	1837003	2599398	58.74%	10.799%
10	11.398	1576	1582	1604	rVB	787406	1013626	22.91%	4.211%
11	12.992	1846	1853	1858	rBV	3170633	4425249	100.00%	18.384%
12	14.045	2027	2032	2044	rVB	573925	755250	17.07%	3.138%
13	15.545	2280	2287	2302	rVB	324250	544669	12.31%	2.263%




Sum of corrected areas: 24070588

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112224\
Data File : BF140565.D
Acq On : 22 Nov 2024 09:46
Operator : RC/JU
Sample : PB165129BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165129BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

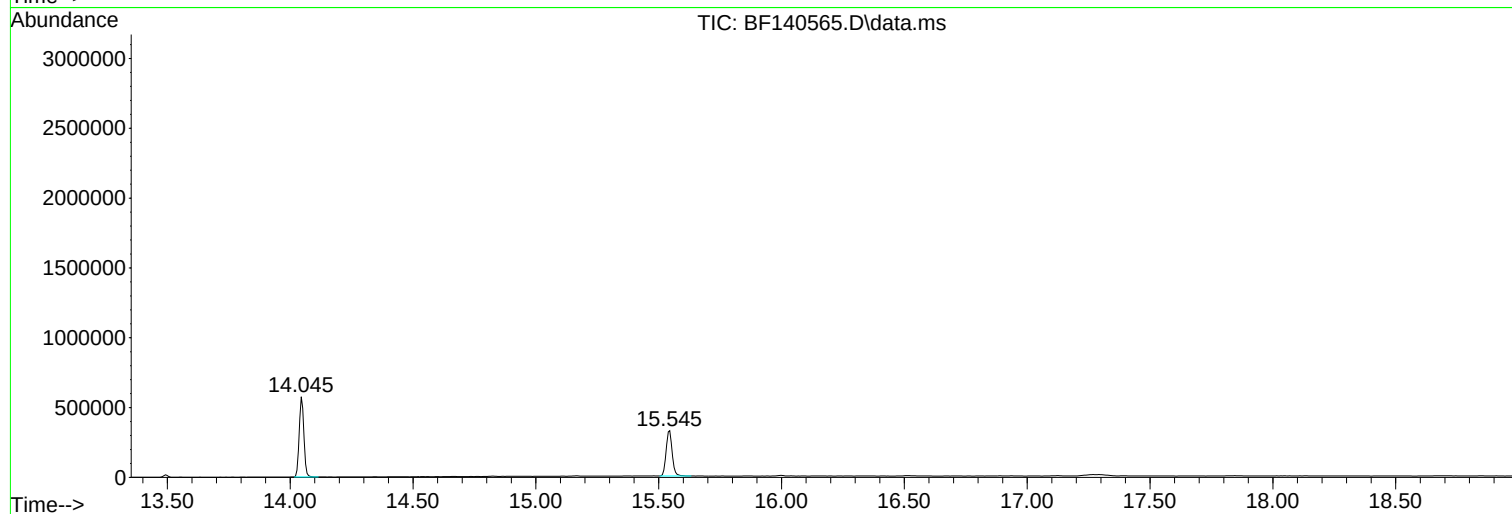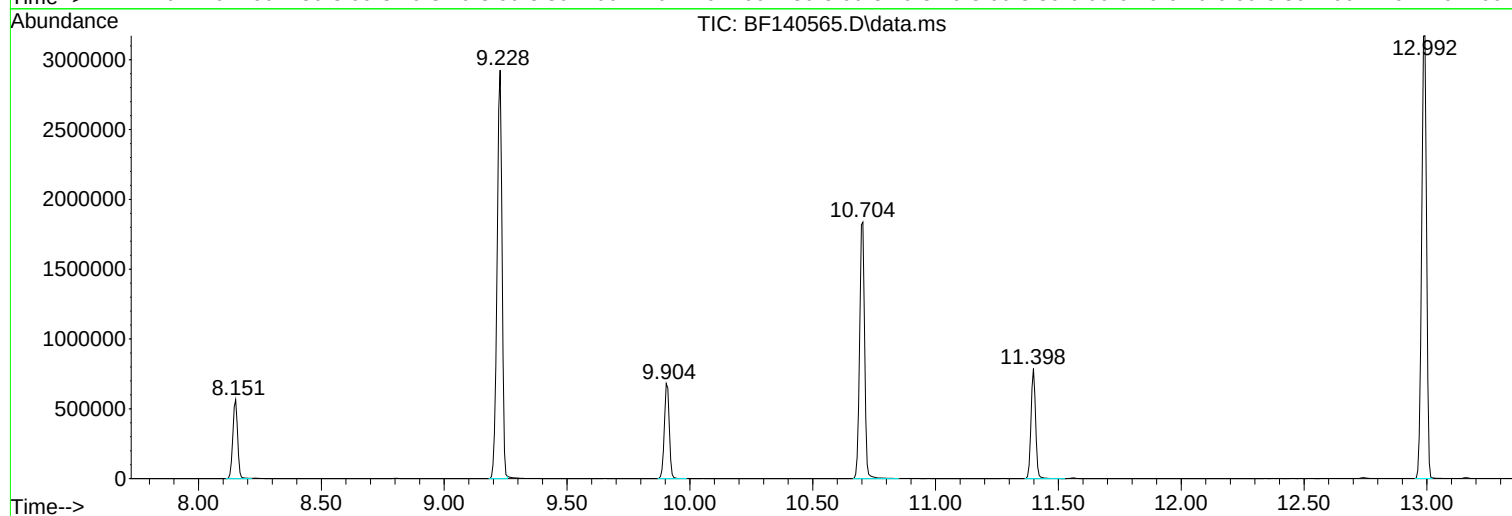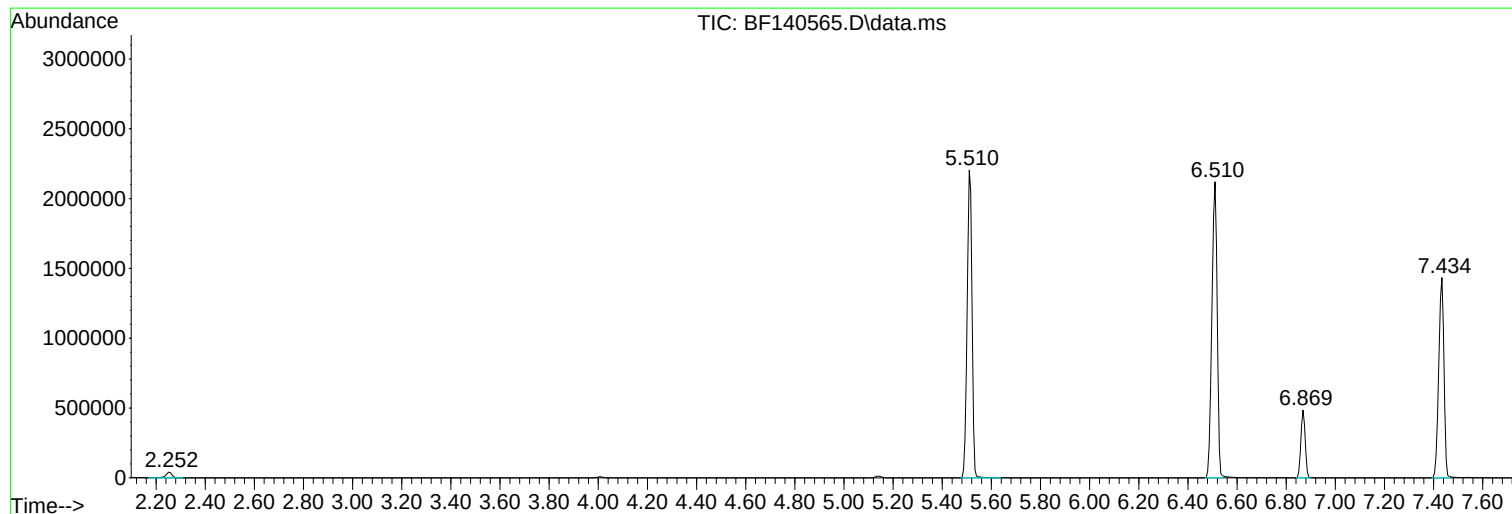

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112224\
Data File : BF140565.D
Acq On : 22 Nov 2024 09:46
Operator : RC/JU
Sample : PB165129BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165129BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.252	2.45 ng	72598	1,4-Dichlorobenzene-d4	6.869

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
3			3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	16
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	12
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	12

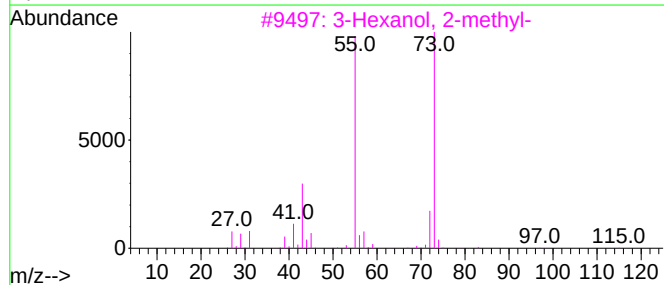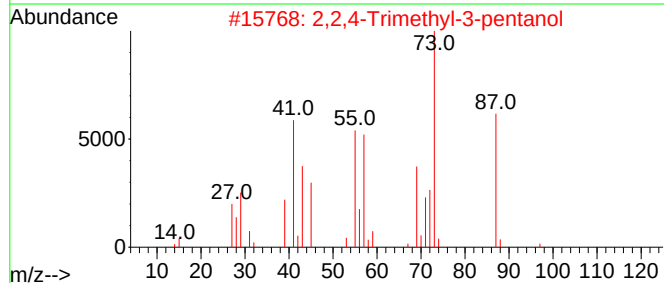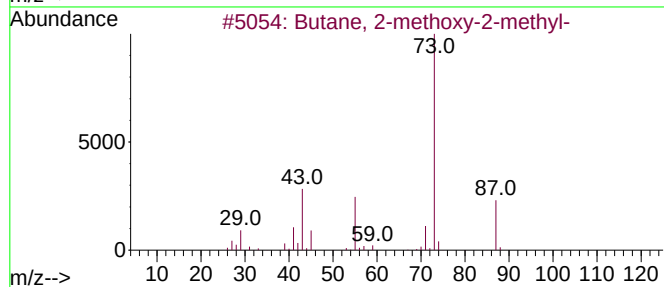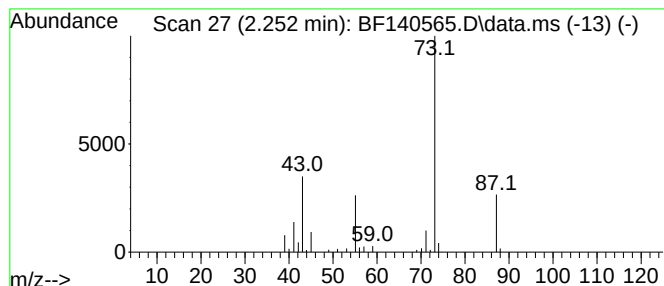

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112224\
Data File : BF140565.D
Acq On : 22 Nov 2024 09:46
Operator : RC/JU
Sample : PB165129BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165129BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.252	2.5	ng	72598	1	6.869	591822	20.0