


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112224\
Data File : BF140563.D
Acq On : 22 Nov 2024 08:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 21 15:23:48 2024

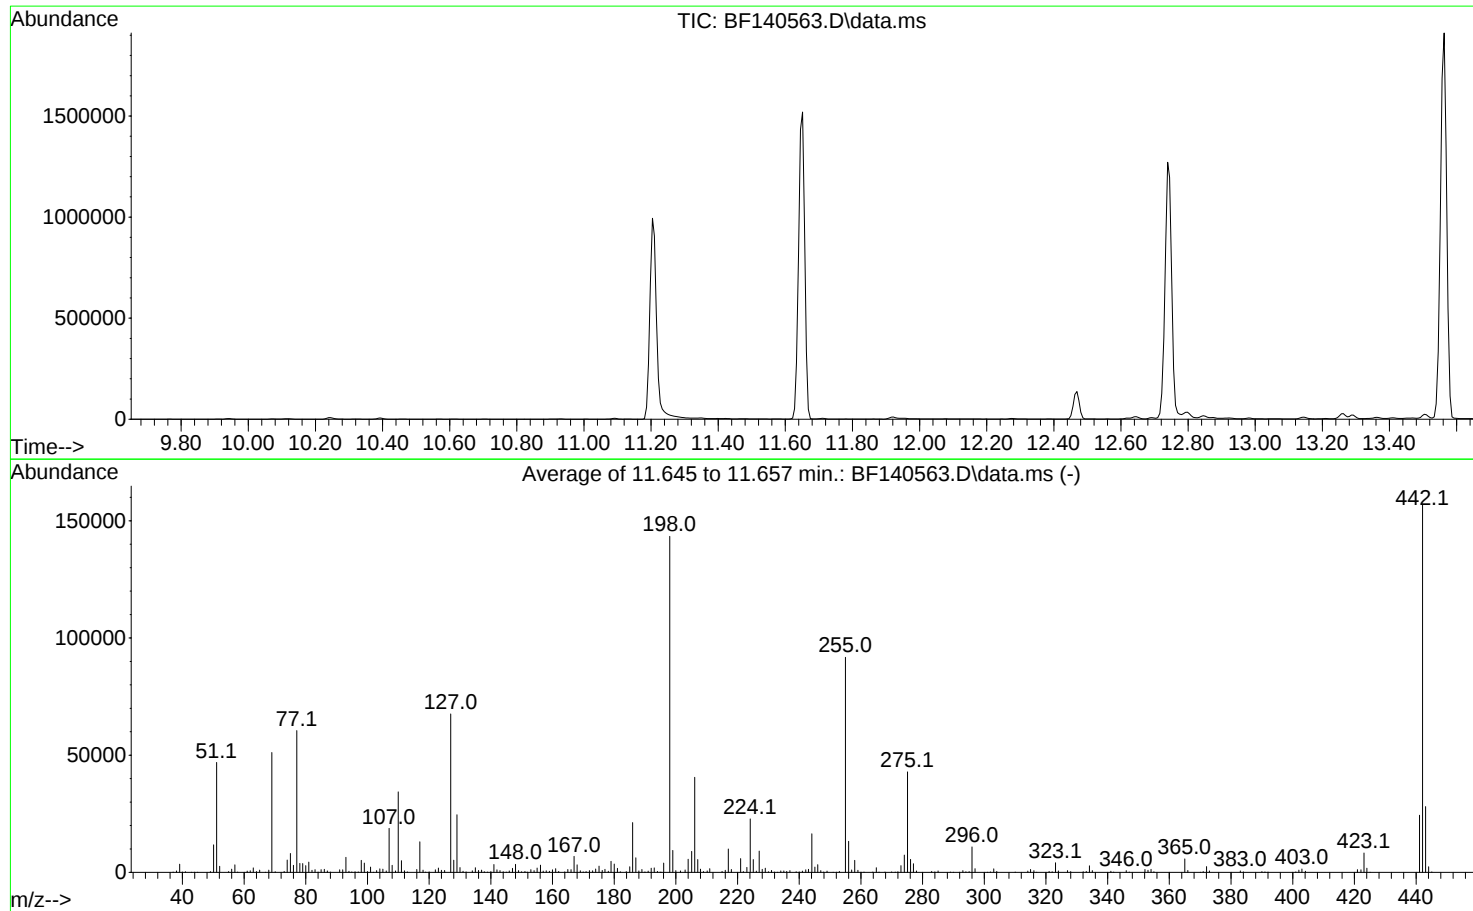

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	46893	PASS
68	69	0.00	2	1.9	946	PASS
69	198	0.00	100	35.6	51112	PASS
70	69	0.00	2	0.6	290	PASS
127	198	10	80	47.1	67563	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	143381	PASS
199	198	5	9	6.5	9364	PASS
275	198	10	60	29.9	42845	PASS
365	198	1	100	4.0	5775	PASS
441	198	0.01	100	17.0	24371	PASS
442	442	50	100	100.0	156949	PASS
443	442	15	24	17.9	28040	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/22/2024	BNA_F	<u>BF140563.D</u>
Compound Name	Response	Retention Time
DDT	483691	13.563
DDD	13127	13.263
DDE	1061	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14188	497879	2.85

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112224\
Data File : BF140563.D
Acq On : 22 Nov 2024 08:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 22 10:51:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

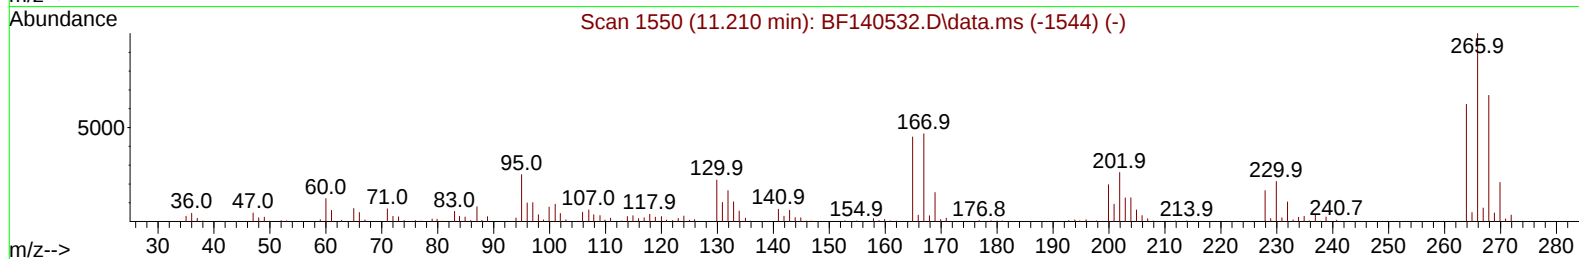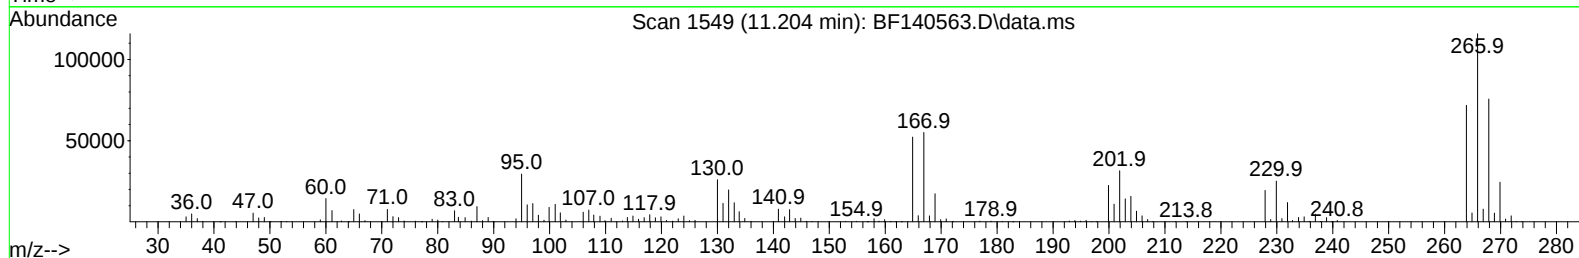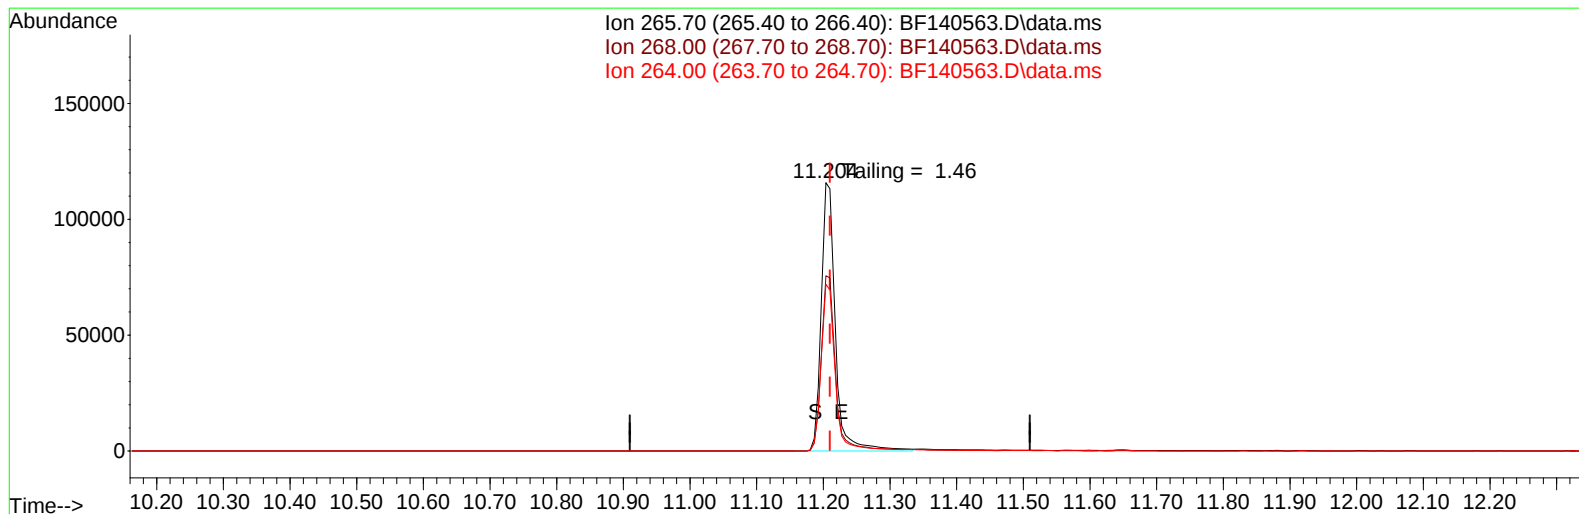

TIC: BF140563.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 42216.94 ng




response 170607

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	65.31
264.00	62.30	62.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112224\
Data File : BF140563.D
Acq On : 22 Nov 2024 08:54
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 22 10:51:57 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112124.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

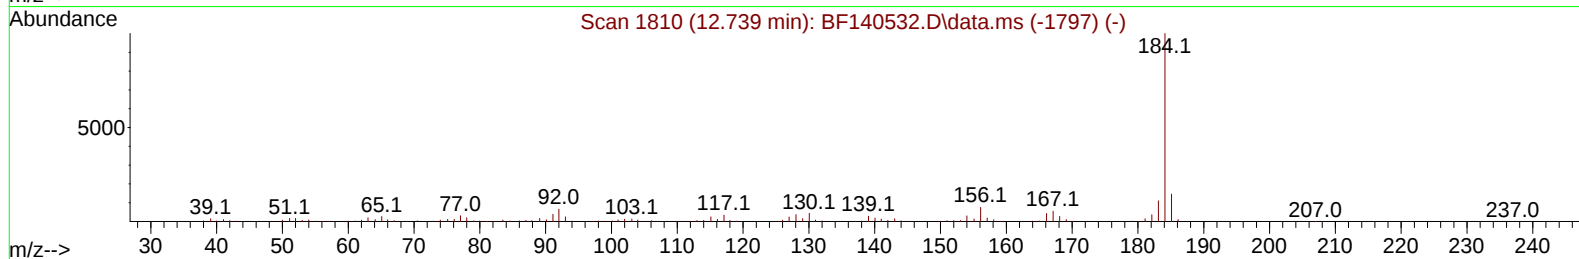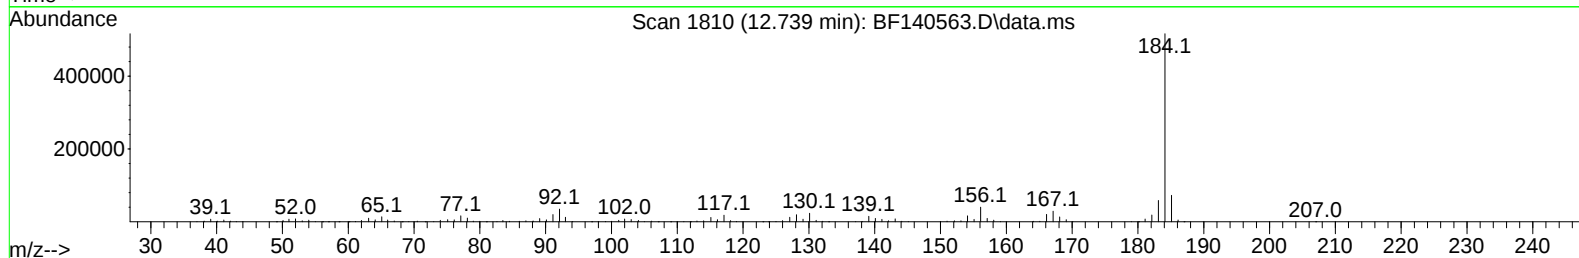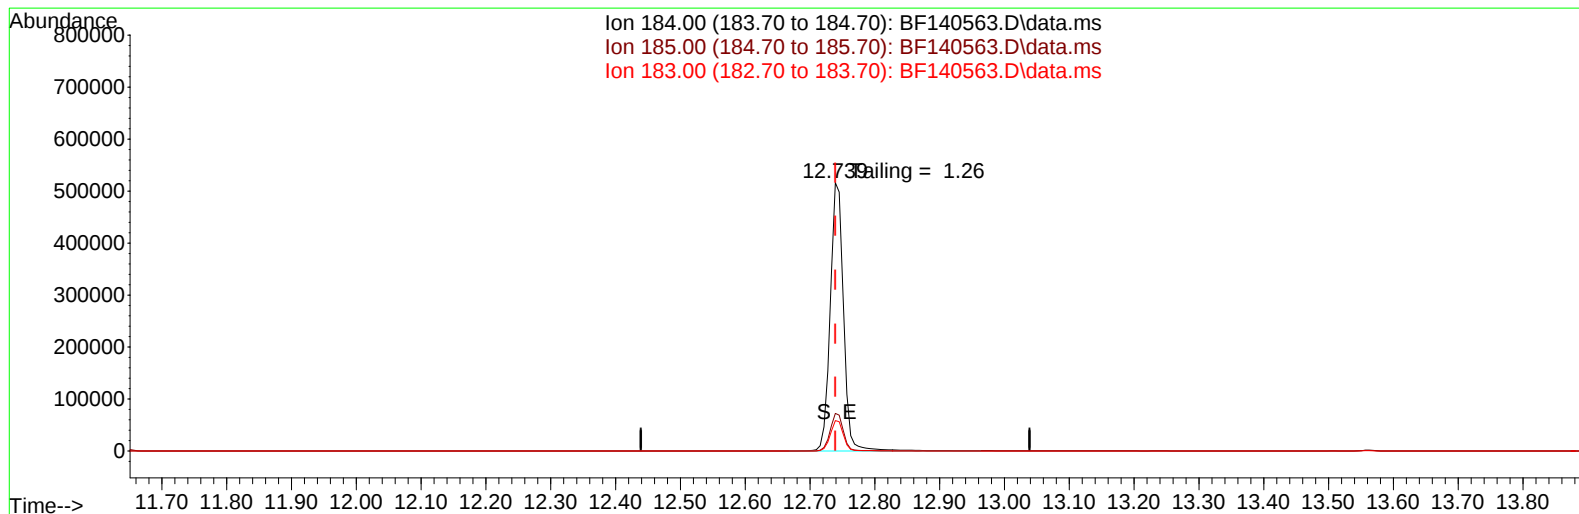

TIC: BF140563.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 28353.32 ng

response 736975

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.05
183.00	11.00	11.34
0.00	0.00	0.00