

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112315\
 Data File : BF083214.D
 Acq On : 23 Nov 2015 20:10
 Operator : UM/IZ
 Sample : G4443-04DL 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 20151110MGP206BRV40DL2

Quant Time: Nov 24 04:35:30 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 22 09:22:46 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.64	152	198261	20.00	ng	-0.02
21) Naphthalene-d8	7.93	136	751578	20.00	ng	-0.02
38) Acenaphthene-d10	9.68	164	376257	20.00	ng	-0.02
63) Phenanthrene-d10	11.15	188	690068	20.00	ng	-0.02
75) Chrysene-d12	13.77	240	543121	20.00	ng	-0.03
86) Perylene-d12	15.13	264	429632	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.27	112	8942	0.68	ng	-0.01
7) Phenol-d6	6.33	99	8510	0.50	ng	-0.01
23) Nitrobenzene-d5	7.21	82	28121	1.71	ng	-0.02
41) 2,4,6-Tribromophenol	10.47	330	4508	1.17	ng	-0.02
44) 2-Fluorobiphenyl	9.00	172	55564	2.06	ng	-0.02
78) Terphenyl-d14	12.73	244	35667	1.55	ng	-0.03
Target Compounds						
9) Benzaldehyde	6.16	77	9646	Below Cal		Qvalue
31) Naphthalene	7.95	128	3034018	74.80	ng	# 1
33) 4-Chloroaniline	7.95	127	433102	27.52	ng	# 95
37) 2-Methylnaphthalene	8.64	142	277521	10.54	ng	# 28
48) Acenaphthylene	9.53	152	144866	3.72	ng	# 97
50) 2,6-Dinitrotoluene	9.68	165	49864	7.67	ng	# 97
56) 2,4-Dinitrotoluene	9.68	165	49864	6.05	ng	# 13
						# 10

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112315\
Data File : BF083214.D
Acq On : 23 Nov 2015 20:10
Operator : UM/IZ
Sample : G4443-04DL 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
20151110MGP206BRV40DL2

Quant Time: Nov 24 04:35:30 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 09:22:46 2015
Response via : Initial Calibration

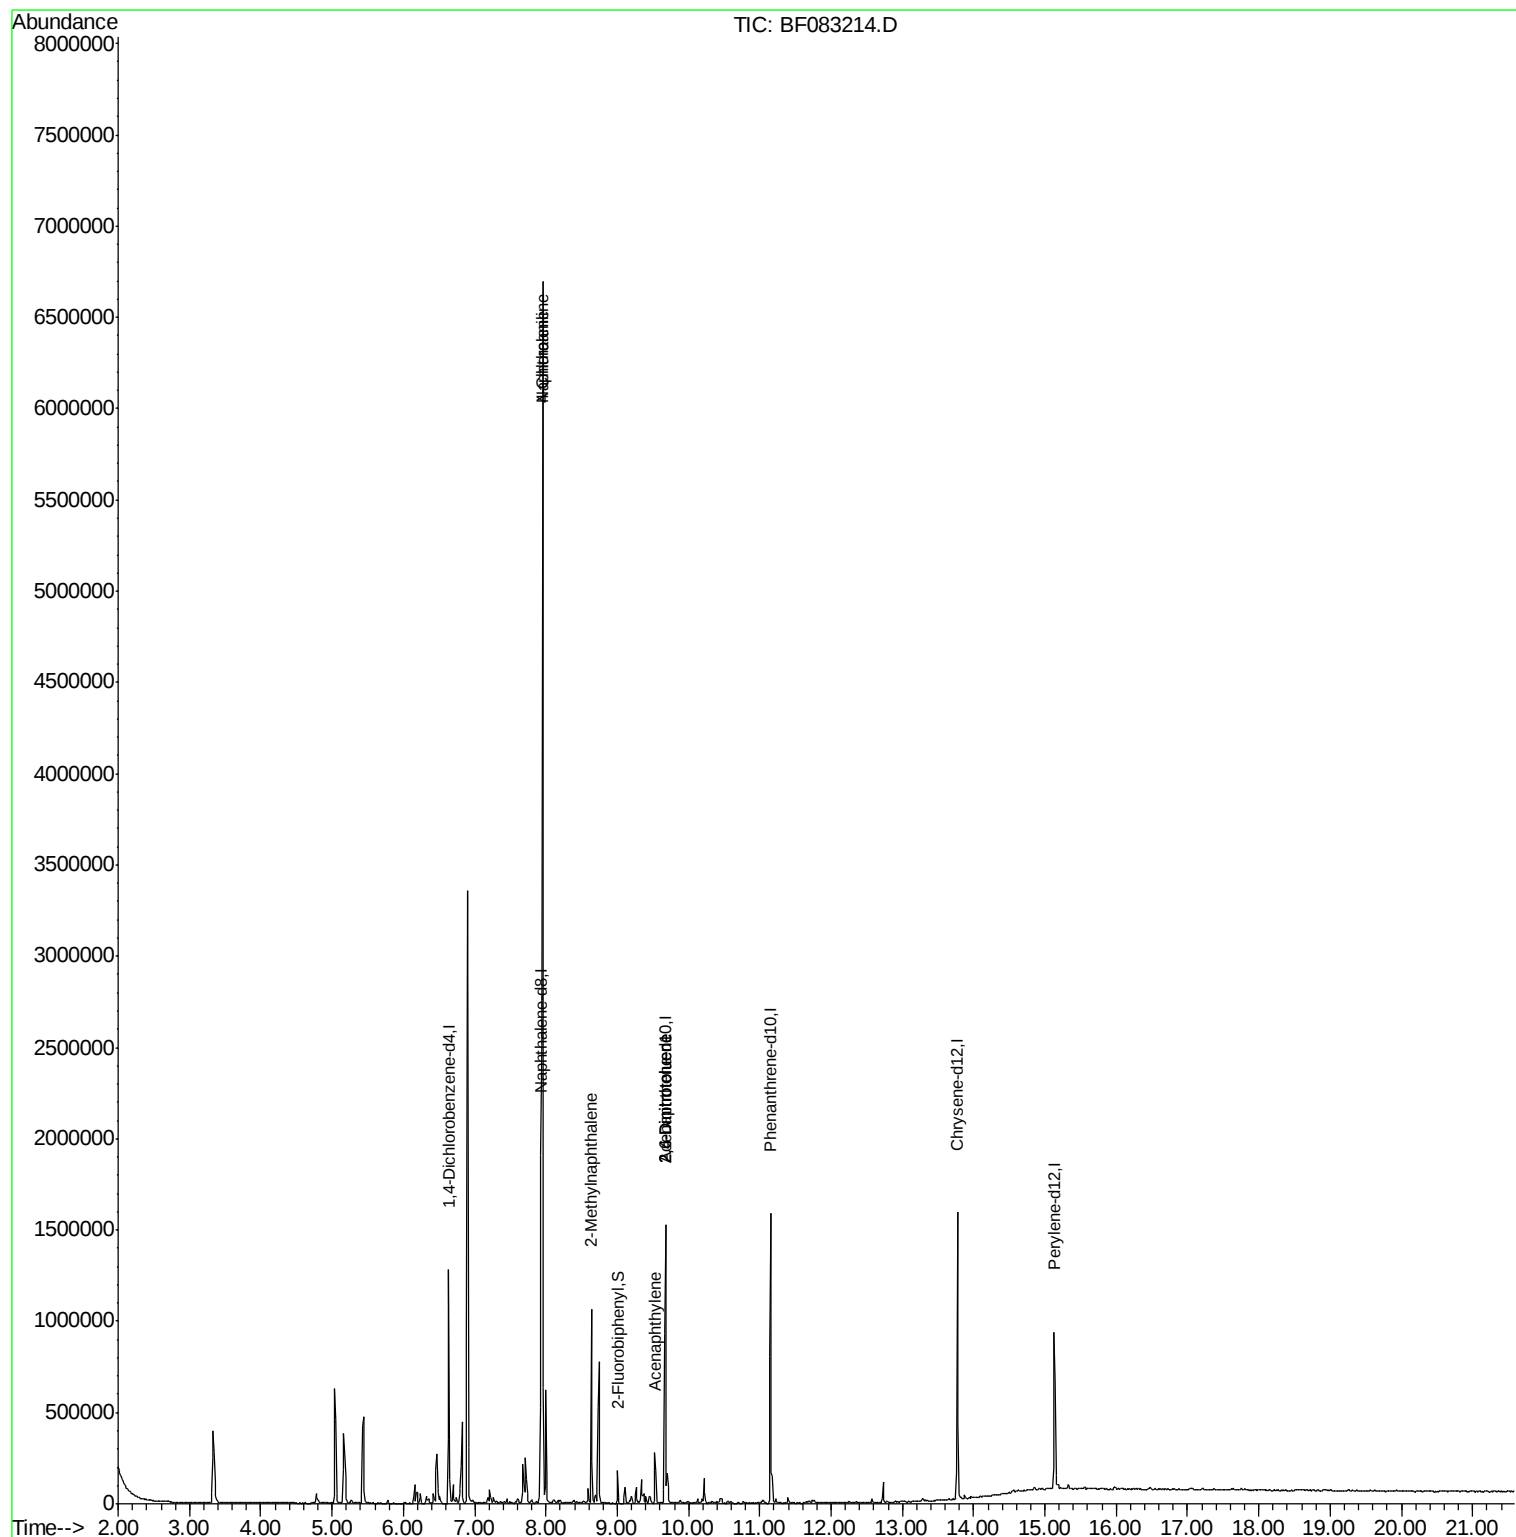



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.64 min Scan# 407

Delta R.T. -0.02 min

Lab File: BF083214.D

Acq: 23 Nov 2015 20:10

Instrument :

BNA_F

ClientSampleId :

20151110MGP206BRV40DL2


Tgt Ion:152 Resp: 198261

Ion Ratio Lower Upper

152 100

150 156.2 125.8 188.8




115 60.6 46.9 70.3

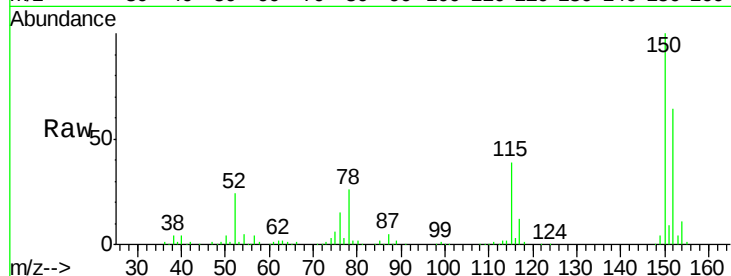

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

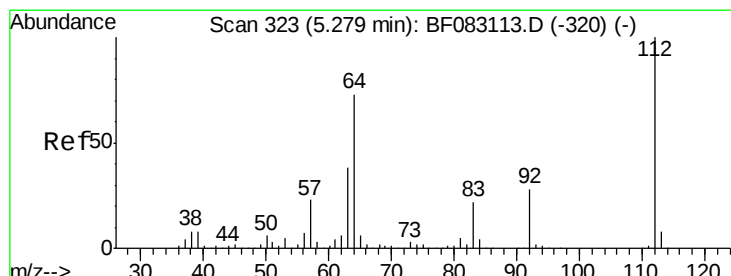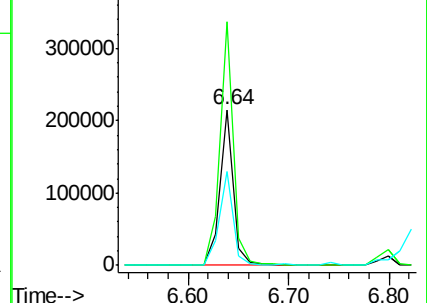

#5

2-Fluorophenol

Concen: 0.68 ng

RT: 5.27 min Scan# 287

Delta R.T. -0.01 min

Lab File: BF083214.D

Acq: 23 Nov 2015 20:10


Tgt Ion:112 Resp: 8942

Ion Ratio Lower Upper

112 100

64 42.9 58.4 87.6#



63 26.0 30.0 45.0#

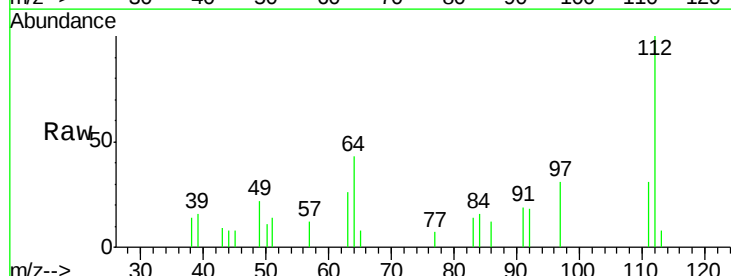


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

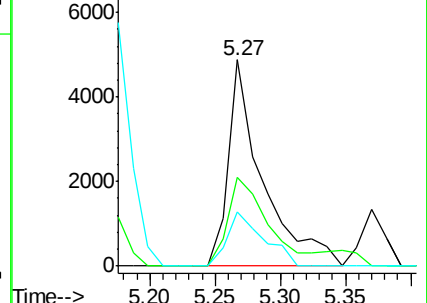



#7

Phenol-d6

Concen: 0.50 ng

RT: 6.33 min Scan# 380

Delta R.T. -0.01 min

Lab File: BF083214.D

Acq: 23 Nov 2015 20:10

Instrument :

BNA_F

ClientSampleId :

20151110MGP206BRV40DL2


Tgt Ion: 99 Resp: 8510

Ion Ratio Lower Upper

99 100

42 20.2 17.7 26.5




71 33.3 30.2 45.4

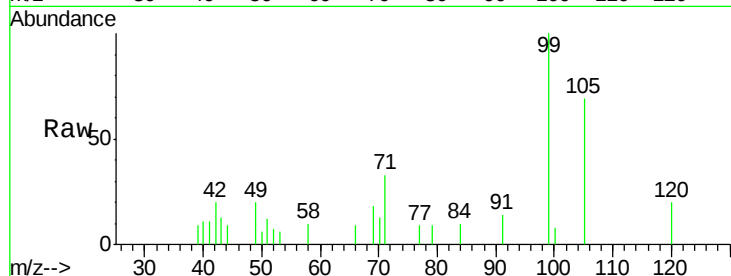

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

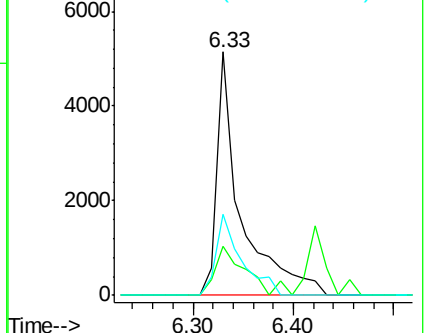

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.93 min Scan# 520

Delta R.T. -0.02 min

Lab File: BF083214.D

Acq: 23 Nov 2015 20:10

Tgt Ion: 136 Resp: 751578


Ion Ratio Lower Upper

136 100

137 11.2 8.7 13.1

54 9.9 5.8 8.6#

68 7.2 3.8 5.8#





Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

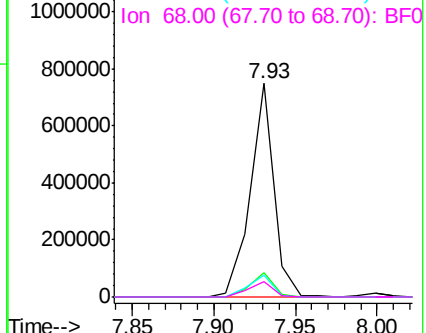



#23

Nitrobenzene-d5

Concen: 1.71 ng

RT: 7.21 min Scan# 457

Delta R.T. -0.02 min

Lab File: BF083214.D

Acq: 23 Nov 2015 20:10

Instrument :

BNA_F

ClientSampleId :

20151110MGP206BRV40DL2


Tgt Ion: 82 Resp: 28121

Ion Ratio Lower Upper

82 100

128 35.5 28.5 42.7




54 52.2 44.6 67.0

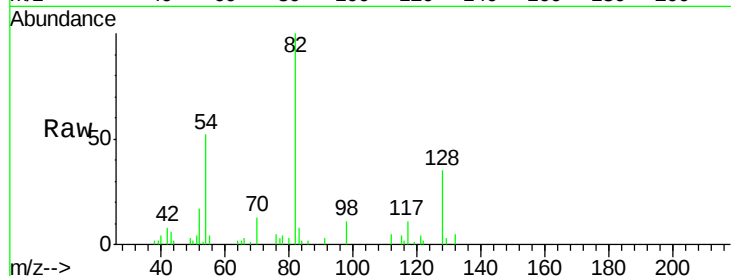

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

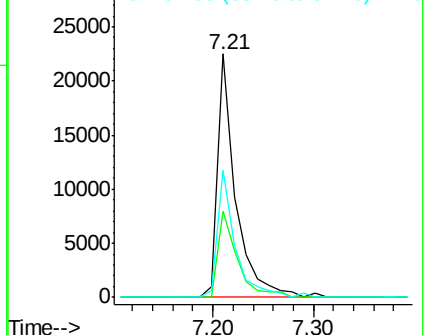

#31

Naphthalene

Concen: 74.80 ng

RT: 7.95 min Scan# 522

Delta R.T. -0.02 min

Lab File: BF083214.D

Acq: 23 Nov 2015 20:10


Tgt Ion: 128 Resp: 3034018

Ion Ratio Lower Upper

128 100

129 12.9 9.0 13.4



127 15.1 10.6 15.8




Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E



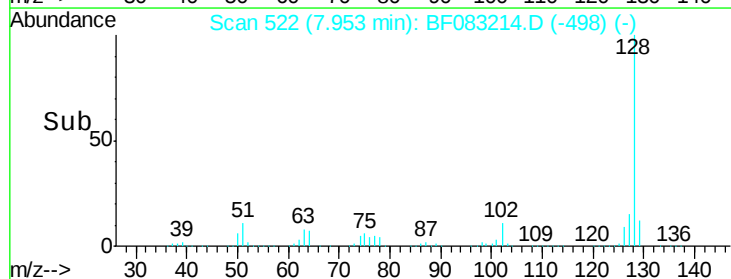
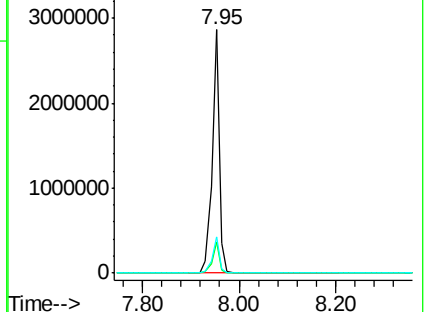




#33
 4-Chloroaniline
 Concen: 27.52 ng
 RT: 7.95 min Scan# 522
 Delta R.T. -0.08 min
 Lab File: BF083214.D
 Acq: 23 Nov 2015 20:10




Instrument :
 BNA_F
 ClientSampleId :
 20151110MGP206BRV40DL2


Tgt Ion:	127	Resp:	433102
Ion	Ratio	Lower	Upper
127	100		
129	85.4	25.7	38.5#
65	0.0	35.5	53.3#
92	0.0	19.4	29.2#

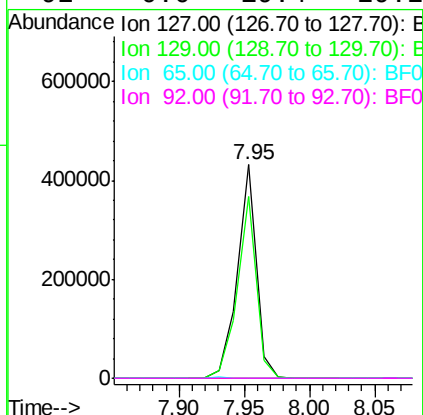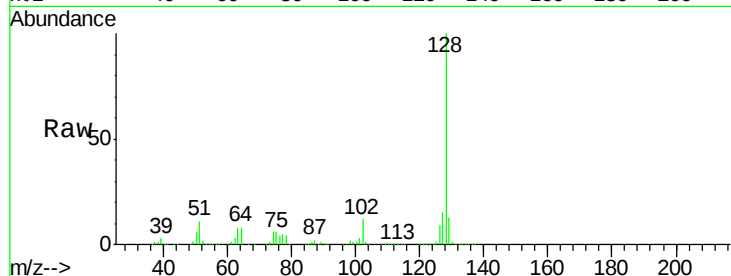

#37
 2-Methylnaphthalene
 Concen: 10.54 ng
 RT: 8.64 min Scan# 582
 Delta R.T. -0.02 min
 Lab File: BF083214.D
 Acq: 23 Nov 2015 20:10

Tgt Ion:	142	Resp:	277521
Ion	Ratio	Lower	Upper
142	100		
141	89.2	70.3	105.5
115	37.6	33.4	50.2

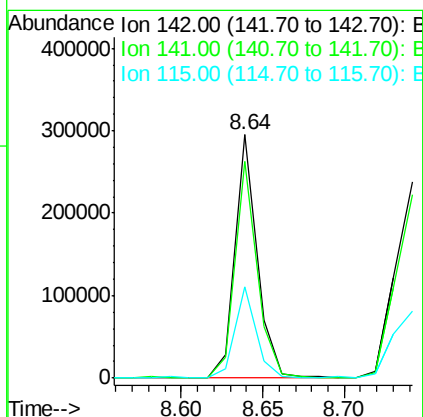


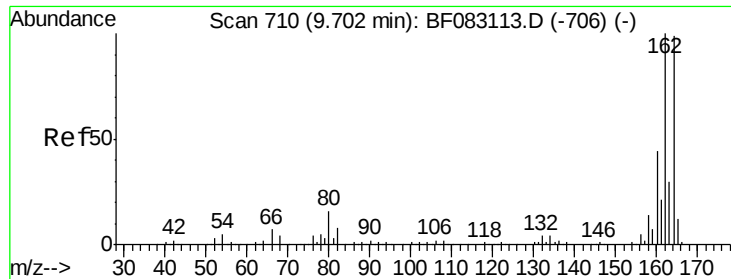




#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.68 min Scan# 673
 Delta R.T. -0.02 min
 Lab File: BF083214.D
 Acq: 23 Nov 2015 20:10

Instrument :
 BNA_F
 ClientSampleId :
 20151110MGP206BRV40DL2

Tgt Ion:164 Resp: 376257
 Ion Ratio Lower Upper
 164 100
 162 105.4 81.2 121.8
 160 47.0 35.6 53.4




Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

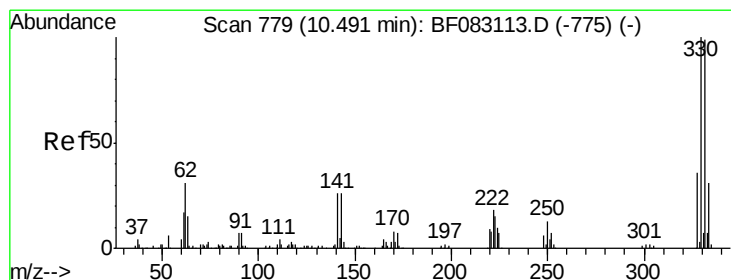
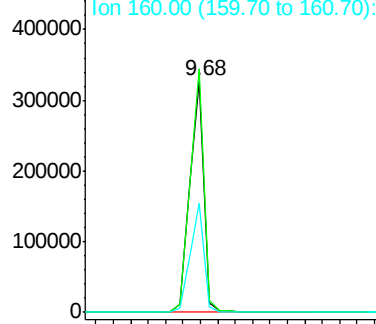



#41
 2,4,6-Tribromophenol
 Concen: 1.17 ng
 RT: 10.47 min Scan# 742
 Delta R.T. -0.02 min
 Lab File: BF083214.D
 Acq: 23 Nov 2015 20:10

Tgt Ion:330 Resp: 4508
 Ion Ratio Lower Upper
 330 100
 332 92.3 77.7 116.5
 141 36.4 29.7 44.5



Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

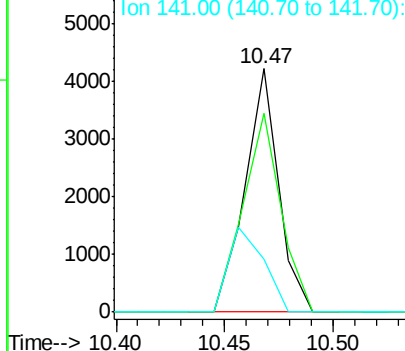


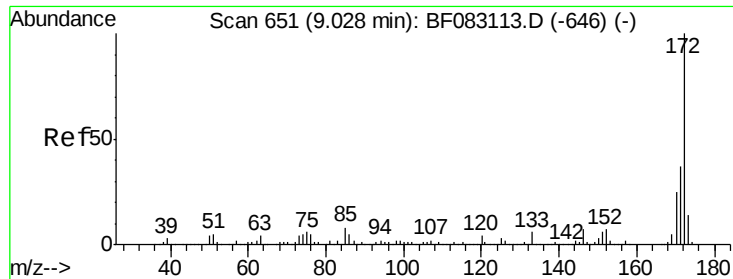




#44
2-Fluorobiphenyl
Concen: 2.06 ng
RT: 9.00 min Scan# 614
Delta R.T. -0.02 min
Lab File: BF083214.D
Acq: 23 Nov 2015 20:10

Instrument :
BNA_F
ClientSampleId :
20151110MGP206BRV40DL2

Tgt Ion:172 Resp: 55564
Ion Ratio Lower Upper
172 100
171 34.7 29.5 44.3
170 21.1 19.9 29.9

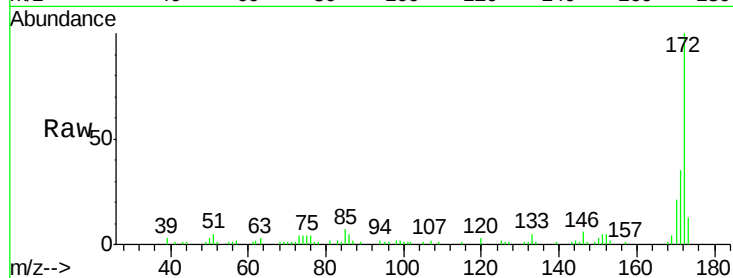


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

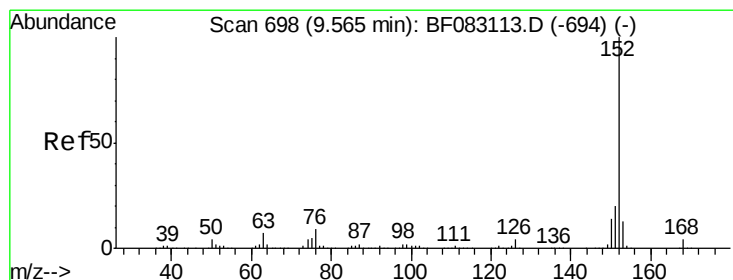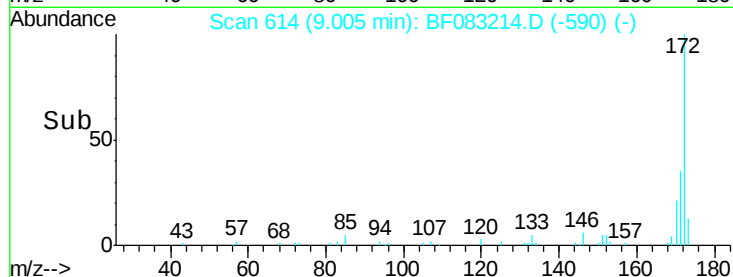
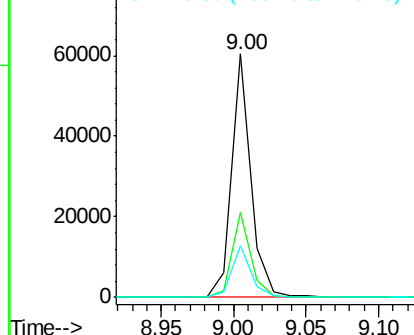



#48
Acenaphthylene
Concen: 3.72 ng
RT: 9.53 min Scan# 660
Delta R.T. -0.03 min
Lab File: BF083214.D
Acq: 23 Nov 2015 20:10

Tgt Ion:152 Resp: 144866
Ion Ratio Lower Upper
152 100
151 18.6 16.3 24.5
153 13.8 10.8 16.2

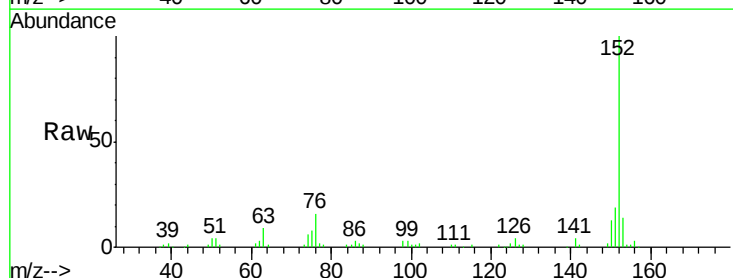

Abundance Ion 152.00 (151.70 to 152.70): E
Ion 151.00 (150.70 to 151.70): E
Ion 153.00 (152.70 to 153.70): E



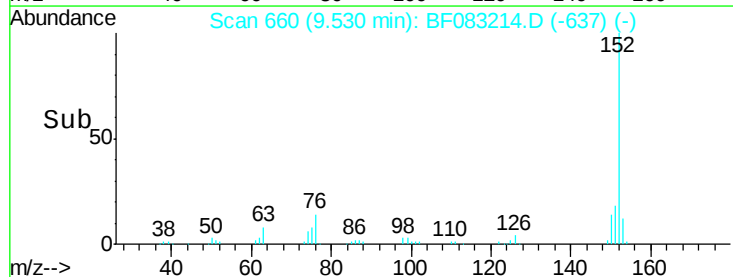
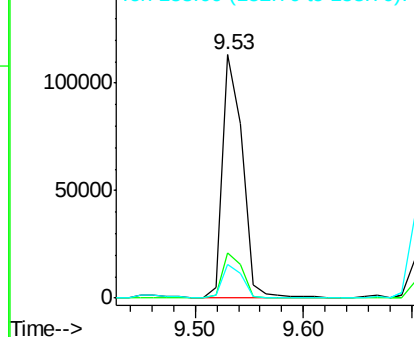


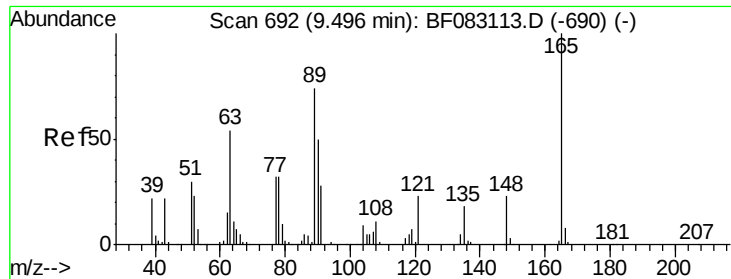

#50
 2,6-Dinitrotoluene
 Concen: 7.67 ng
 RT: 9.68 min Scan# 673
 Delta R.T. 0.18 min
 Lab File: BF083214.D
 Acq: 23 Nov 2015 20:10




Instrument :
 BNA_F
 ClientSampleId :
 20151110MGP206BRV40DL2


Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.4	62.5	93.7#
89	1.6	59.1	88.7#

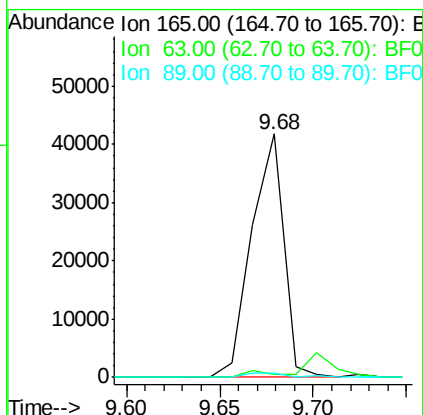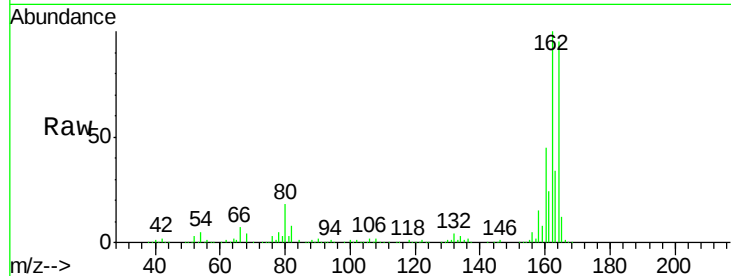

#56
 2,4-Dinitrotoluene
 Concen: 6.05 ng
 RT: 9.68 min Scan# 673
 Delta R.T. -0.22 min
 Lab File: BF083214.D
 Acq: 23 Nov 2015 20:10

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.4	54.5	81.7#
89	1.6	77.3	115.9#
182	0.0	1.8	2.6#


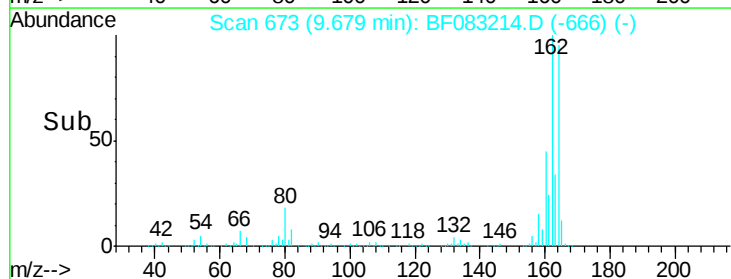
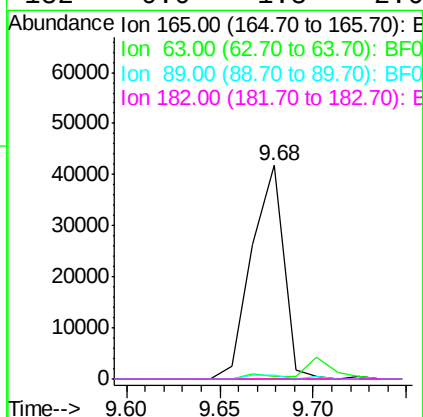





#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.15 min Scan# 802
Delta R.T. -0.02 min
Lab File: BF083214.D
Acq: 23 Nov 2015 20:10




Instrument :
BNA_F
ClientSampleId :
20151110MGP206BRV40DL2


Tgt Ion:188 Resp: 690068
Ion Ratio Lower Upper
188 100
94 8.2 6.0 9.0
80 9.2 6.7 10.1

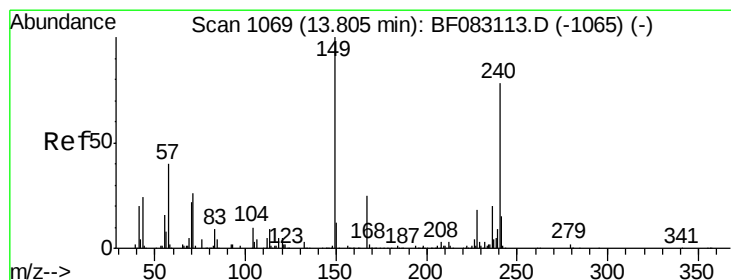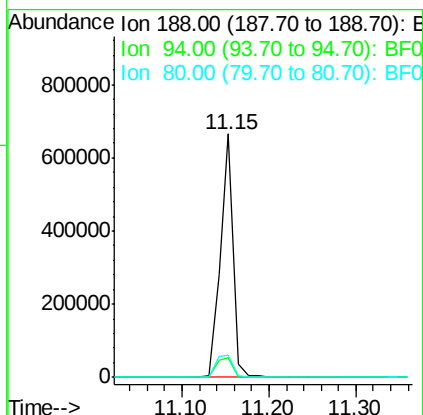

#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.77 min Scan# 1031
Delta R.T. -0.03 min
Lab File: BF083214.D
Acq: 23 Nov 2015 20:10

Tgt Ion:240 Resp: 543121
Ion Ratio Lower Upper
240 100
120 12.7 5.4 8.2#
236 26.3 20.6 31.0

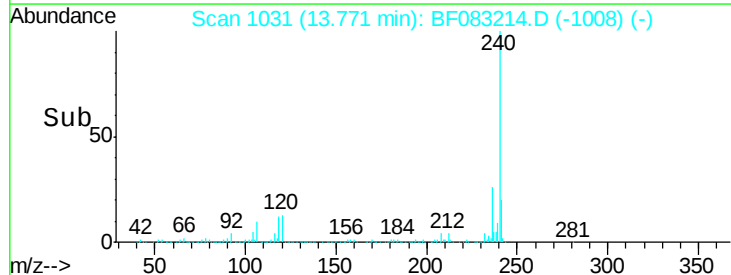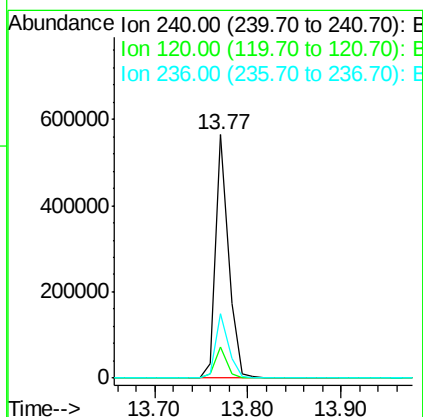

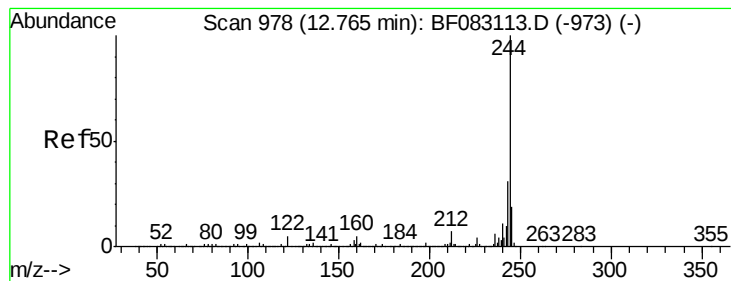

#78

Terphenyl-d14

Concen: 1.55 ng

RT: 12.73 min Scan# 940

Delta R.T. -0.03 min

Lab File: BF083214.D

Acq: 23 Nov 2015 20:10

Instrument :

BNA_F

ClientSampleId :

20151110MGP206BRV40DL2





Tgt Ion:244 Resp: 35667

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.2

122 10.8 4.3 6.5#

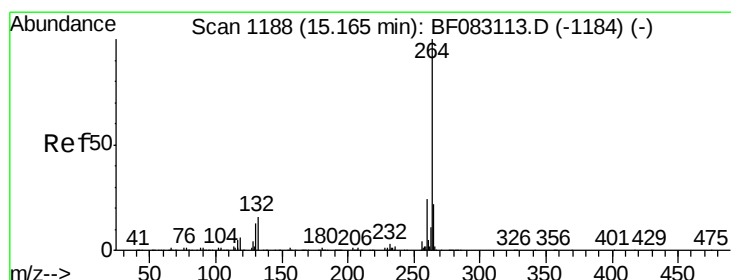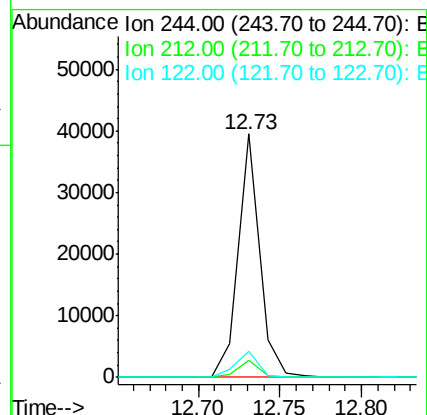

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.13 min Scan# 1150

Delta R.T. -0.03 min

Lab File: BF083214.D

Acq: 23 Nov 2015 20:10

Tgt Ion:264 Resp: 429632

Ion Ratio Lower Upper

264 100

260 23.0 19.1 28.7

265 22.0 18.2 27.4

