
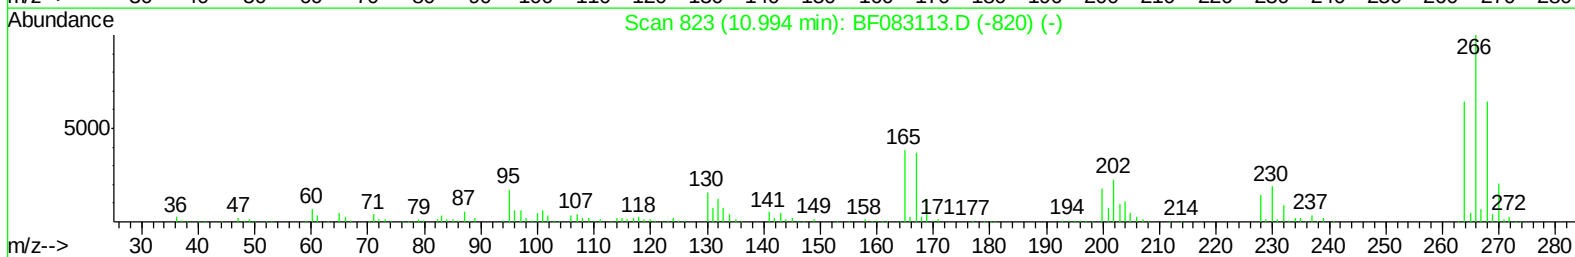
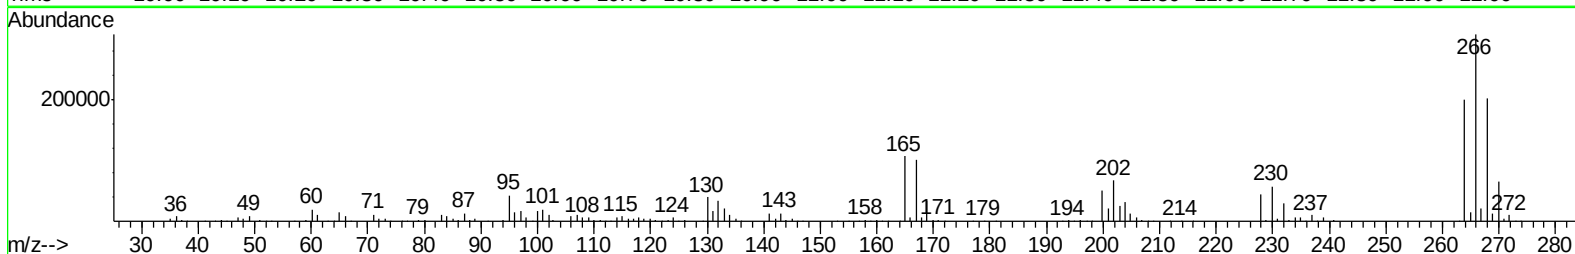


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112315\
Data File : BF083196.D
Acq On : 23 Nov 2015 10:42
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 08:13:29 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 09:22:46 2015
Response via : Initial Calibration

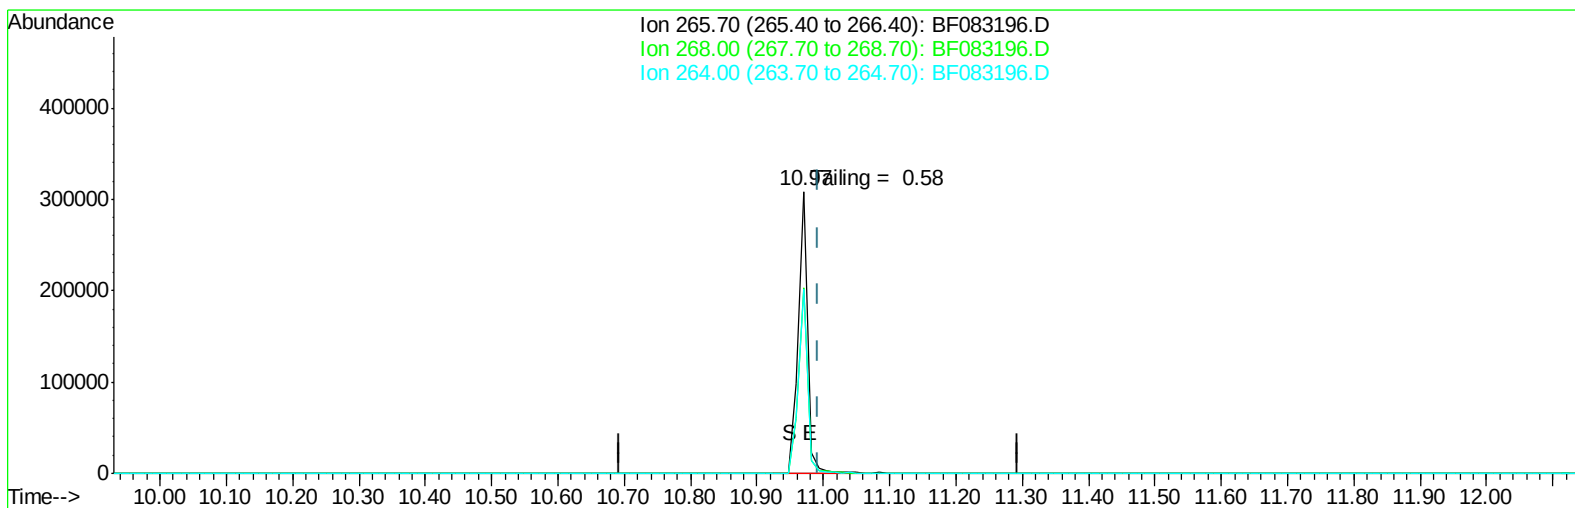

TIC: BF083196.D

(69) Pentachlorophenol (C)




10.970min (-0.023) 28644.20ng

response 307112

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	65.70
264.00	64.60	65.30
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112315\
Data File : BF083196.D
Acq On : 23 Nov 2015 10:42
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 08:13:29 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 09:22:46 2015
Response via : Initial Calibration

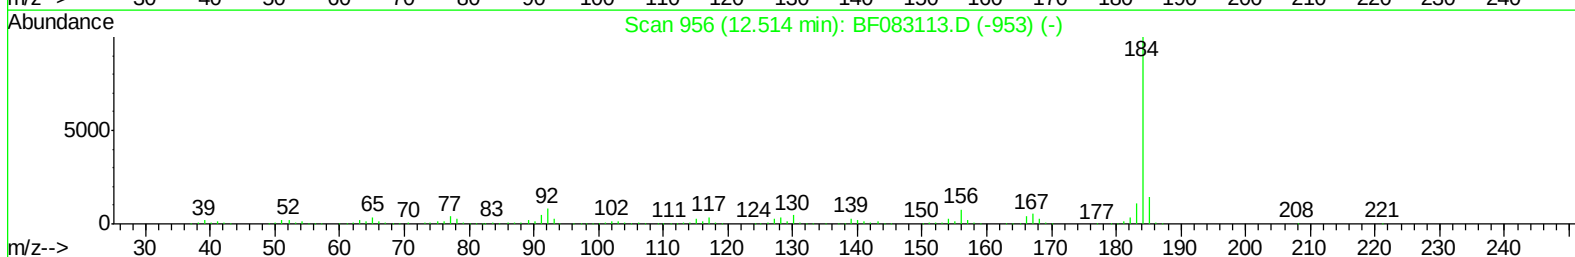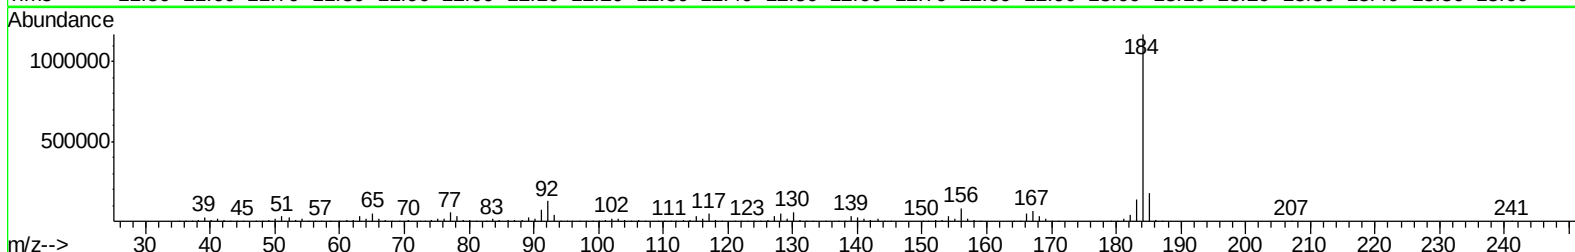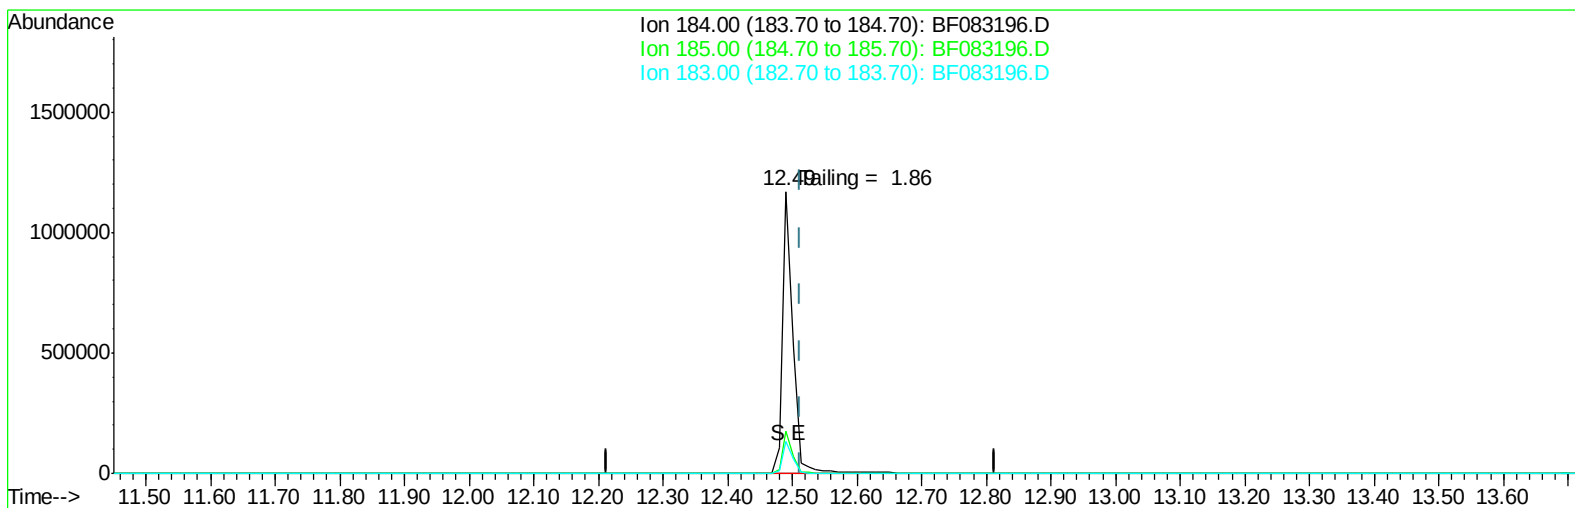

TIC: BF083196.D

(76) Benzidine

12.491min (-0.023) 0.00ng

response 1339065

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	14.82
183.00	11.00	11.39
0.00	0.00	0.00