
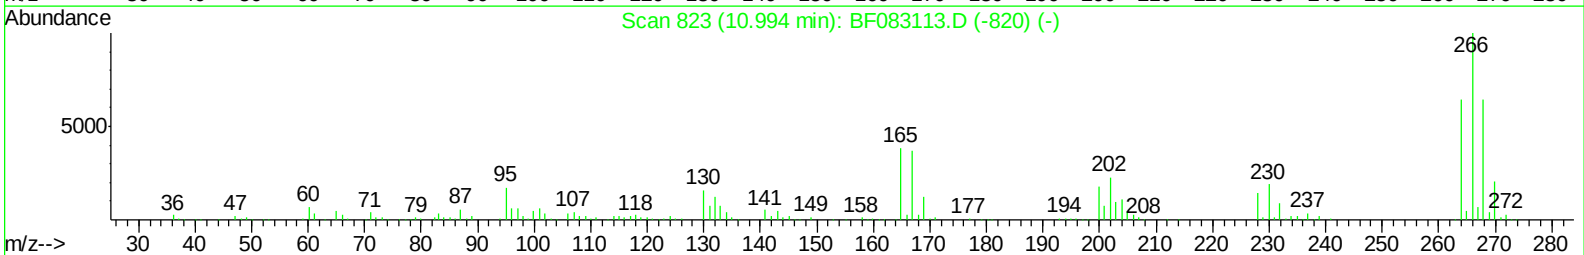
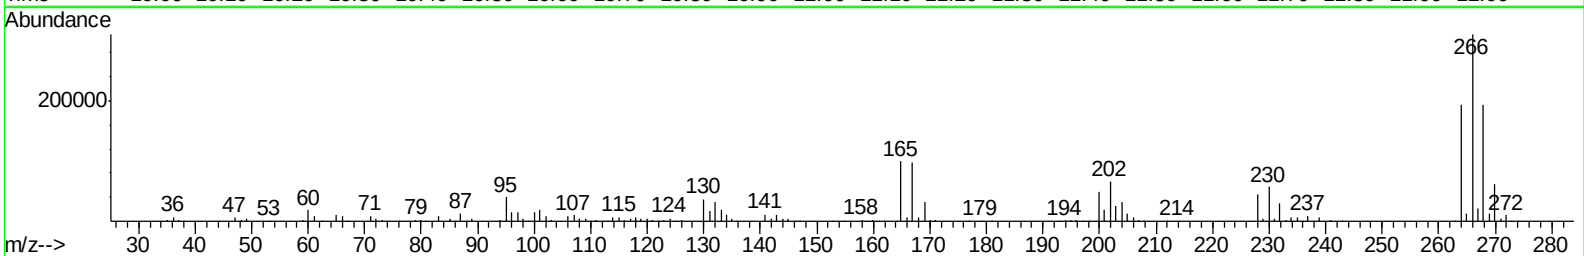


```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112315\  
Data File : BF083206.D  
Acq On    : 23 Nov 2015   16:06  
Operator  : UM/IZ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Nov 24 08:14:53 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 09:22:46 2015
Response via : Initial Calibration

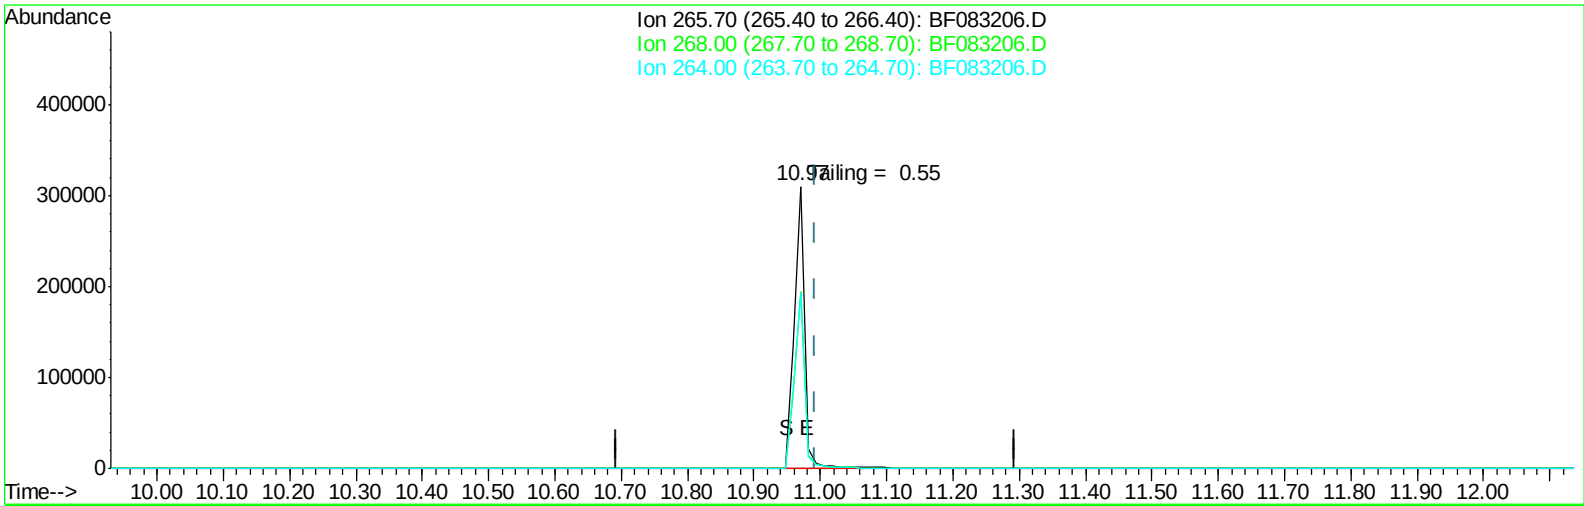

TIC: BF083206.D

(69) Pentachlorophenol (C)




10.970min (-0.023) 0.00ng

response 334465

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	62.60
264.00	64.60	62.45
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112315\
Data File : BF083206.D
Acq On : 23 Nov 2015 16:06
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 08:14:53 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 09:22:46 2015
Response via : Initial Calibration

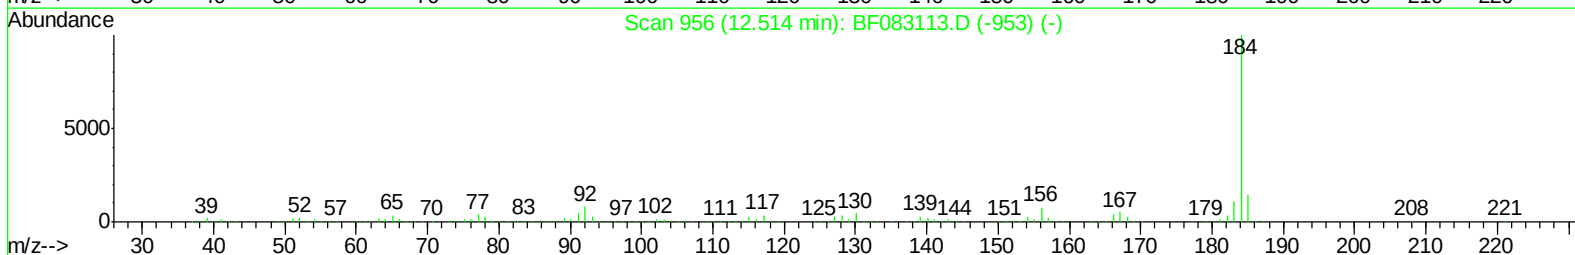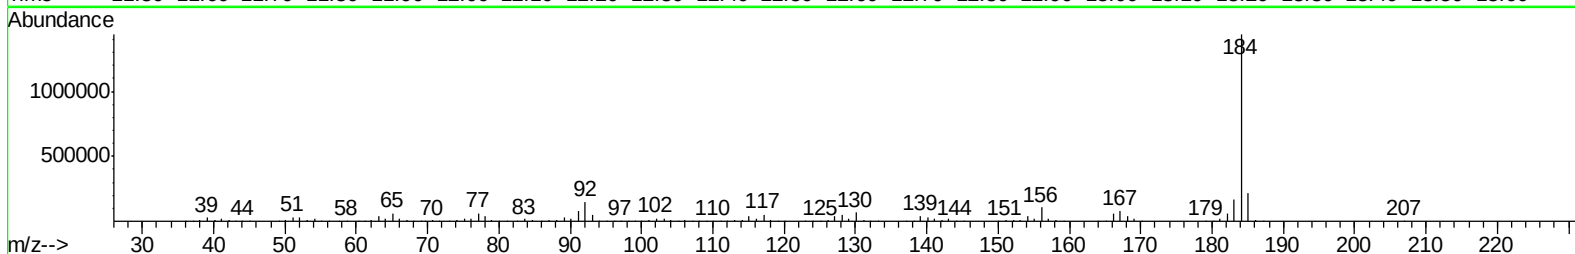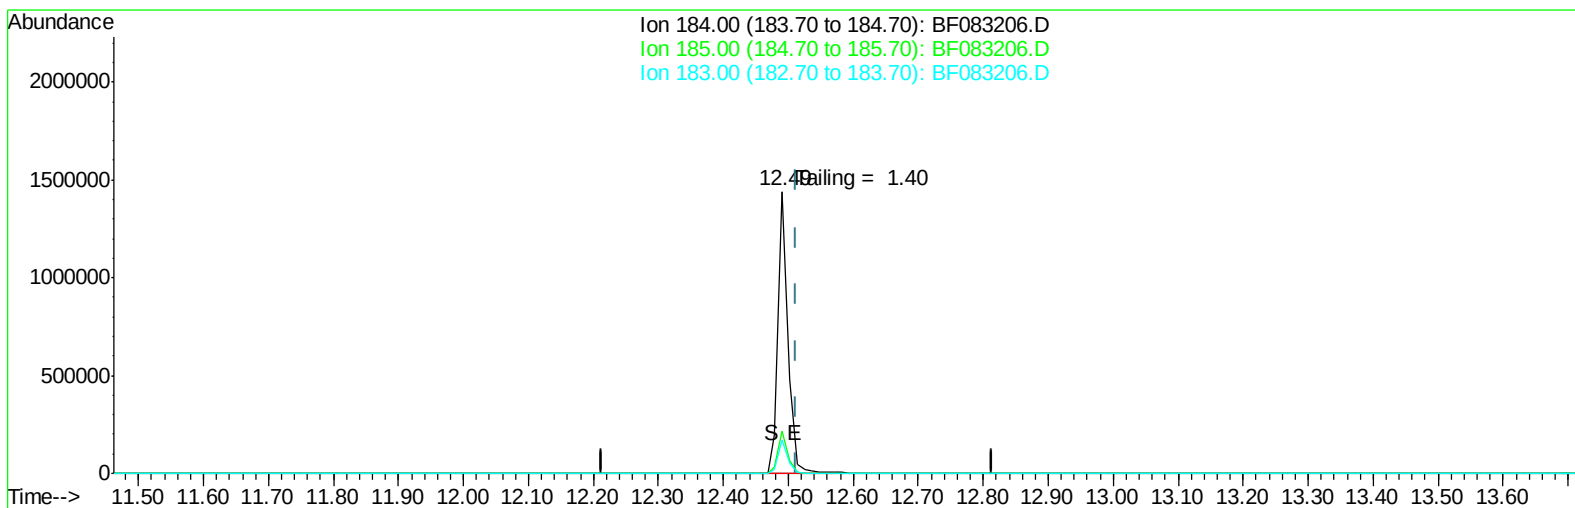

TIC: BF083206.D

(76) Benzidine

12.491min (-0.023) 0.00ng

response 1543571

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	14.96
183.00	11.00	11.78
0.00	0.00	0.00