


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112315\
 Data File : BF083206.D
 Acq On : 23 Nov 2015 16:06
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Nov 22 09:22:46 2015

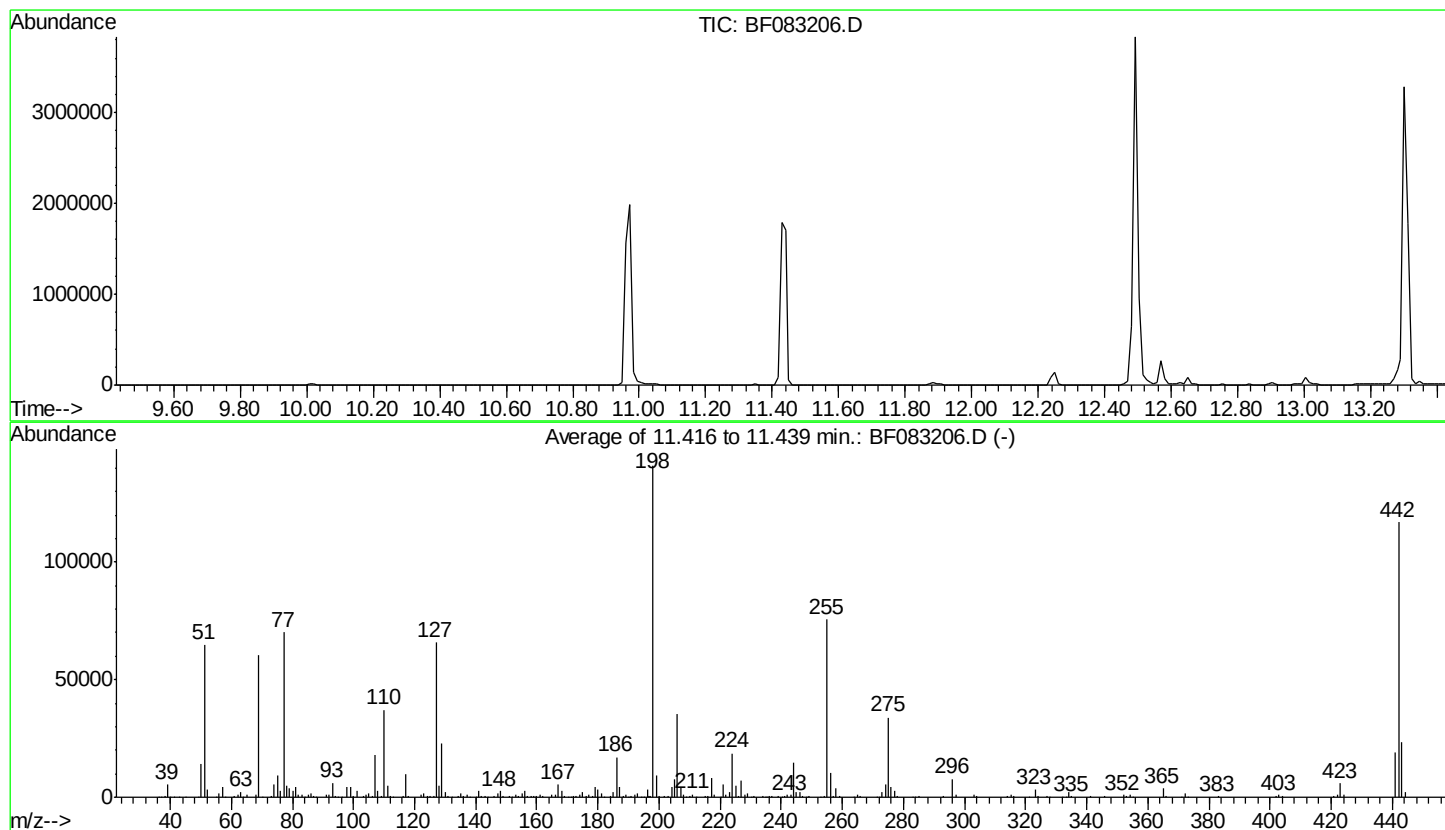

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 822

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	65052	PASS
68	69	0.00	2	1.4	874	PASS
69	198	0.00	100	42.9	60531	PASS
70	69	0.00	2	0.4	235	PASS
127	198	10	80	46.7	65792	PASS
197	198	0.00	2	0.3	398	PASS
198	198	100	100	100.0	141016	PASS
199	198	5	9	6.6	9299	PASS
275	198	10	60	24.0	33806	PASS
365	198	1	100	2.6	3716	PASS
441	442	0.01	24	16.5	19326	PASS
442	198	50	100	82.9	116848	PASS
443	442	15	24	19.9	23270	PASS