
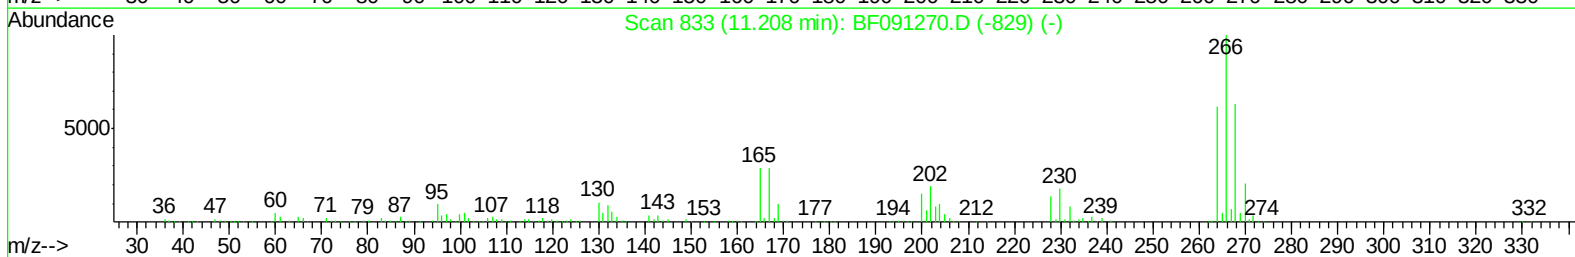
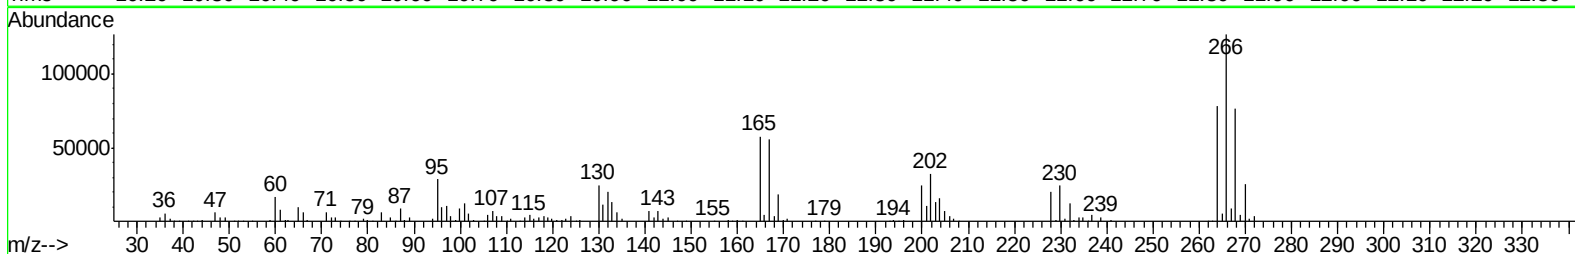


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112316\
Data File : BF091266.D
Acq On : 23 Nov 2016 9:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 00:44:20 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 13:22:53 2016
Response via : Initial Calibration

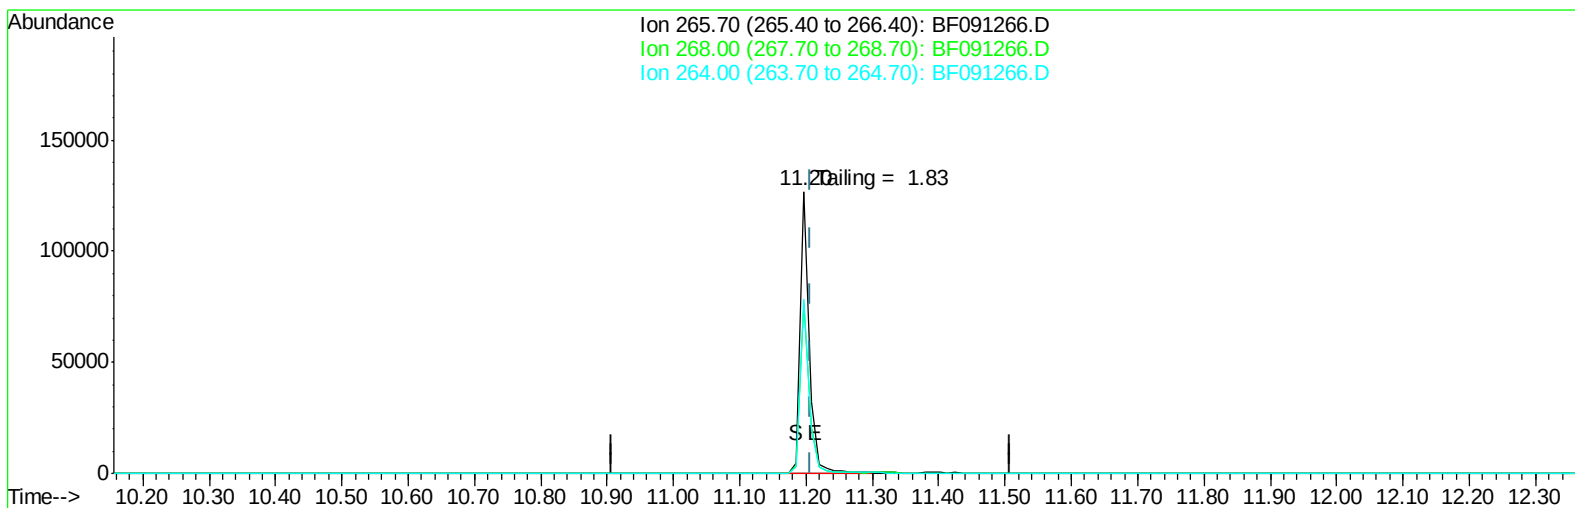

TIC: BF091266.D

(69) Pentachlorophenol (C)




11.196min (-0.011) 0.00ng

response 121996

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	60.61
264.00	60.20	62.04
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112316\
Data File : BF091266.D
Acq On : 23 Nov 2016 9:02
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 00:44:20 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 13:22:53 2016
Response via : Initial Calibration

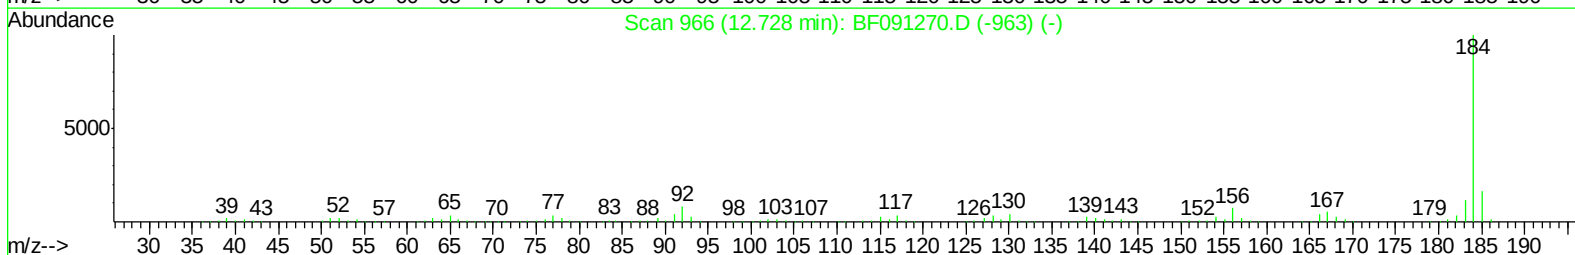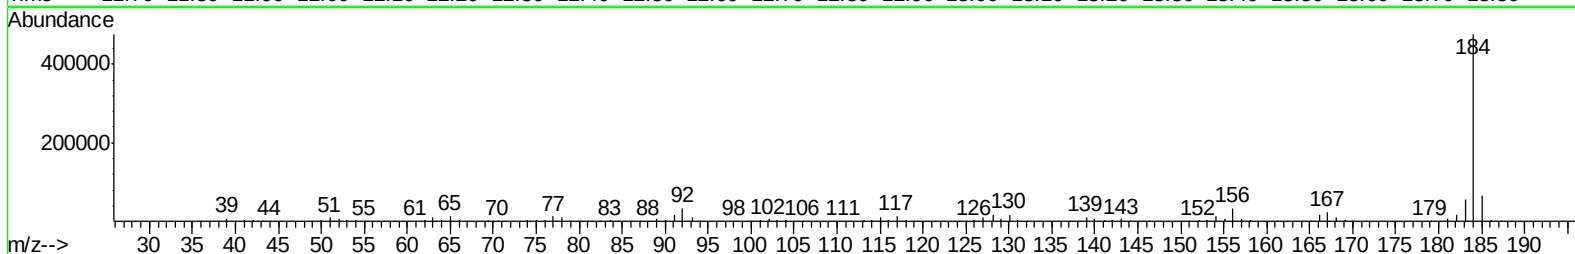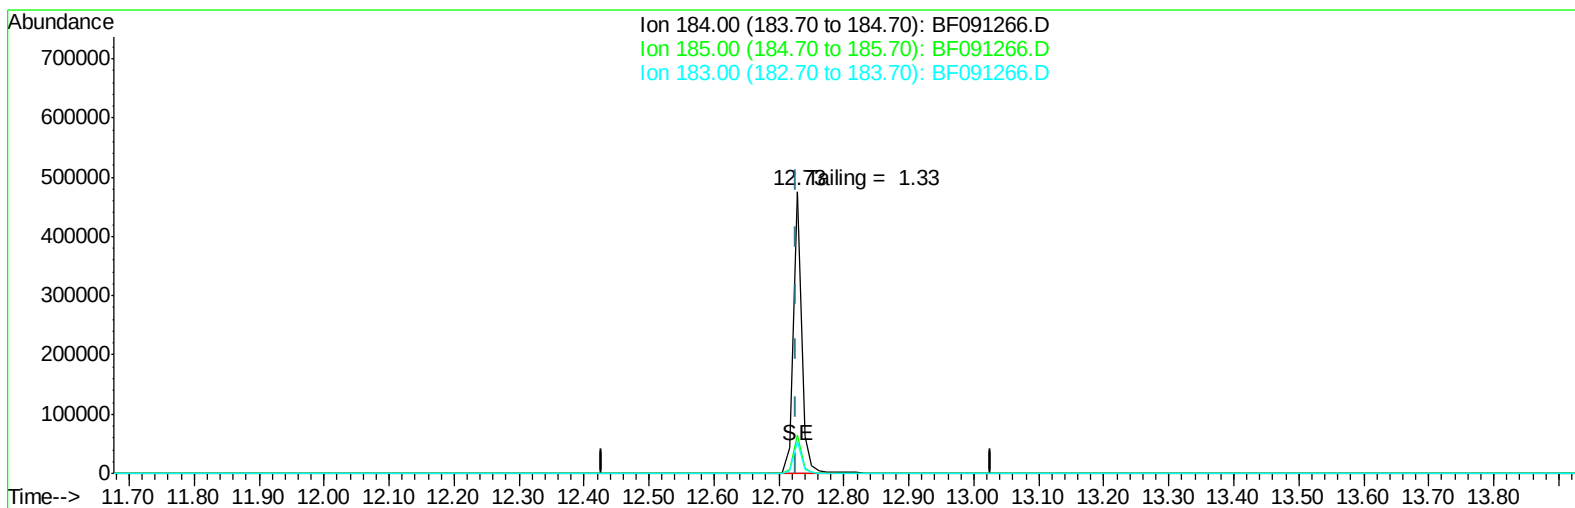

TIC: BF091266.D

(76) Benzidine

12.728min (+0.001) 0.00ng

response 424321

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	13.52
183.00	11.10	11.51
0.00	0.00	0.00