
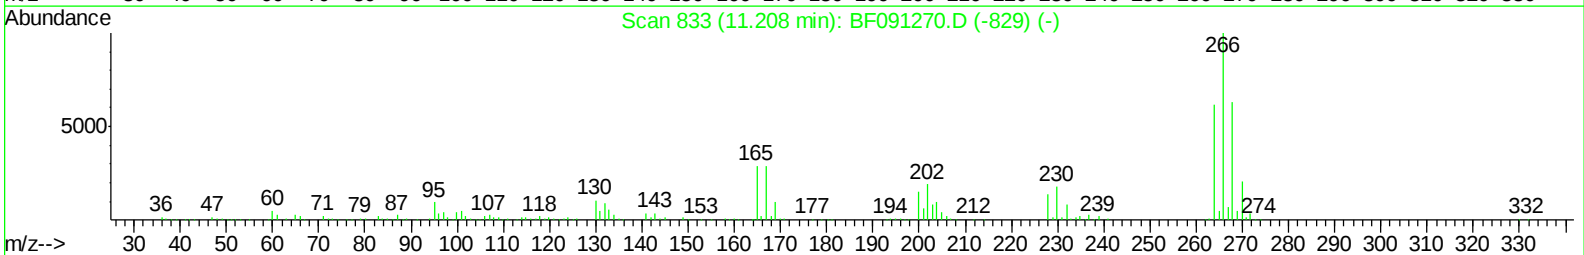
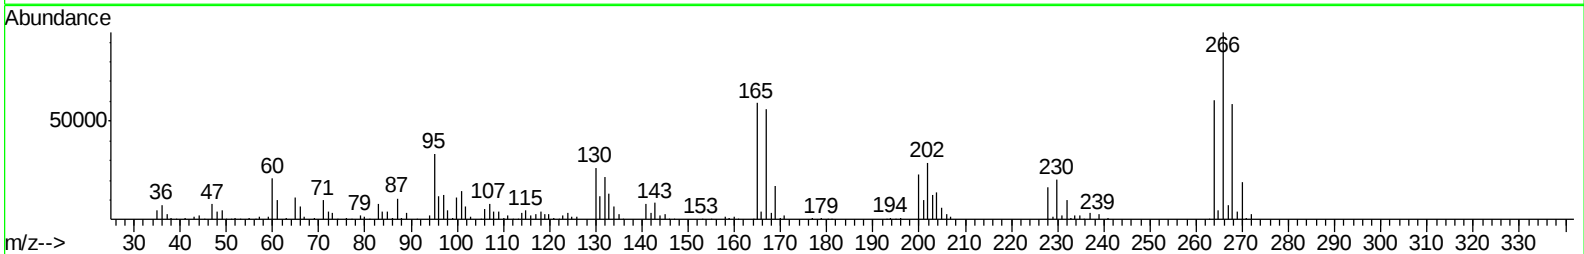


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112316\
Data File : BF091279.D
Acq On : 23 Nov 2016 16:48
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 00:45:02 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 13:22:53 2016
Response via : Initial Calibration

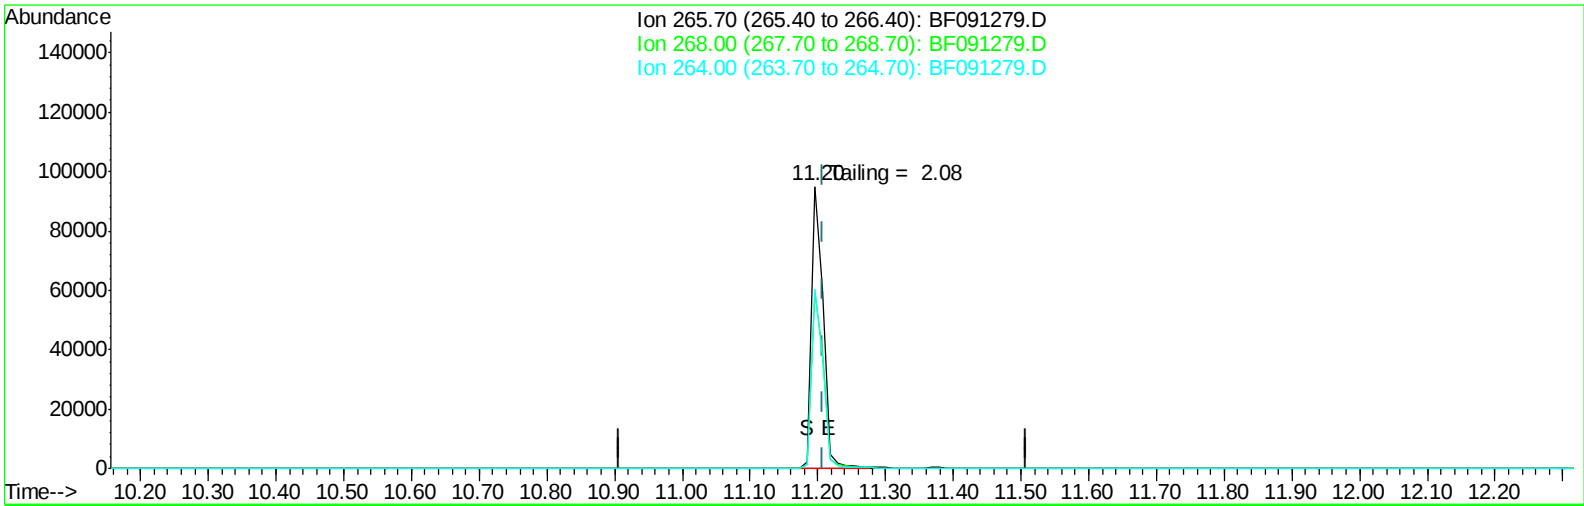

TIC: BF091279.D

(69) Pentachlorophenol (C)




11.196min (-0.011) 0.00ng

response 115023

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	62.06
264.00	60.20	63.77
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112316\
Data File : BF091279.D
Acq On : 23 Nov 2016 16:48
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 00:45:02 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 13:22:53 2016
Response via : Initial Calibration

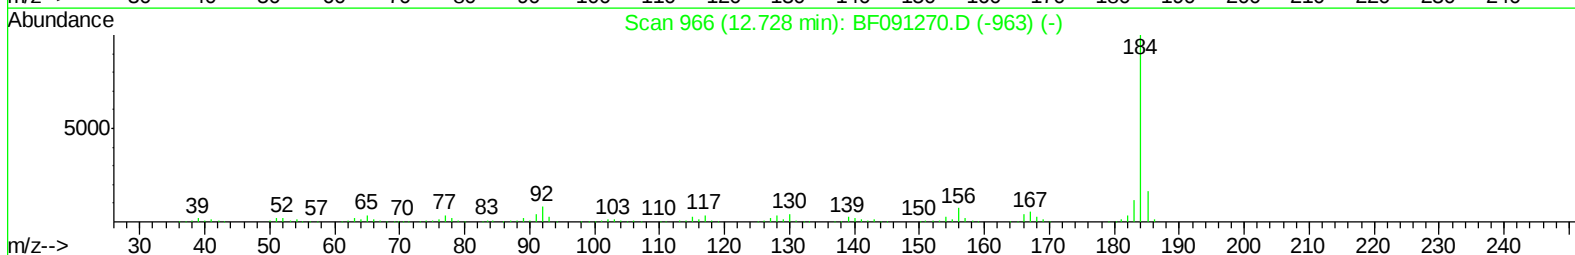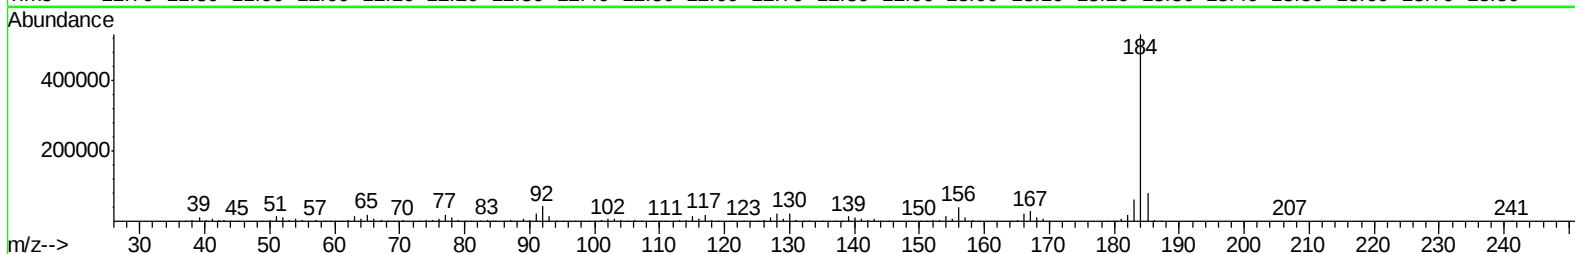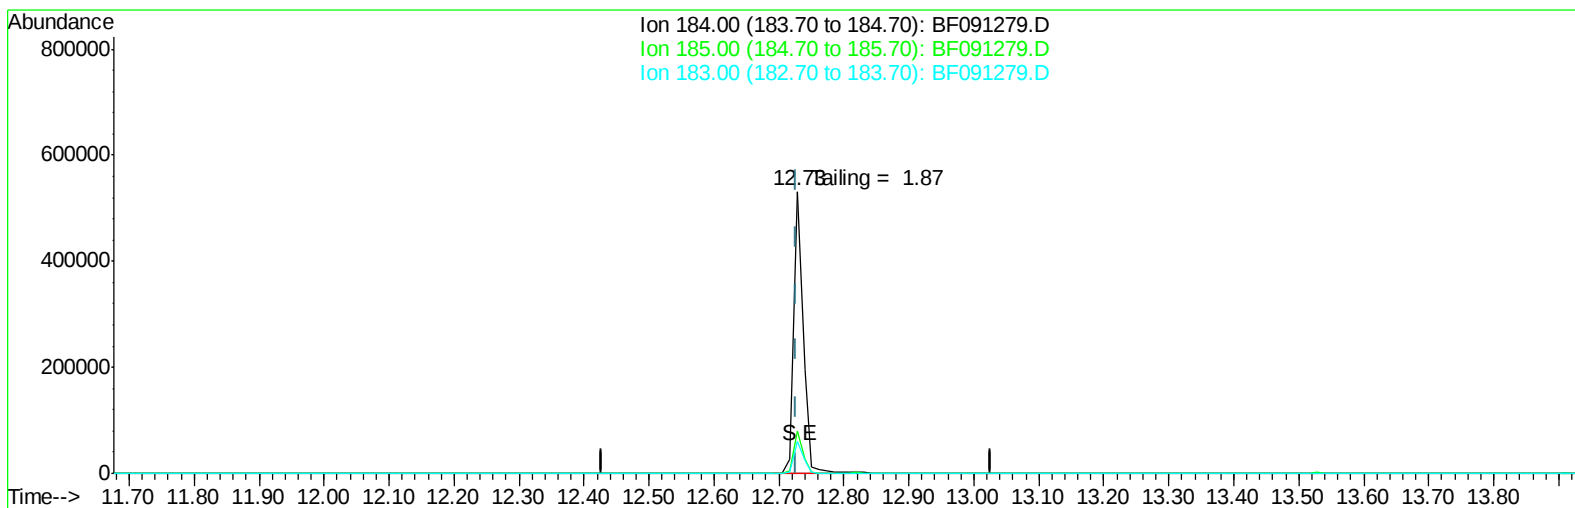

TIC: BF091279.D

(76) Benzidine

12.728min (+0.001) 28166.15ng

response 545329

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	15.01
183.00	11.10	11.49
0.00	0.00	0.00