
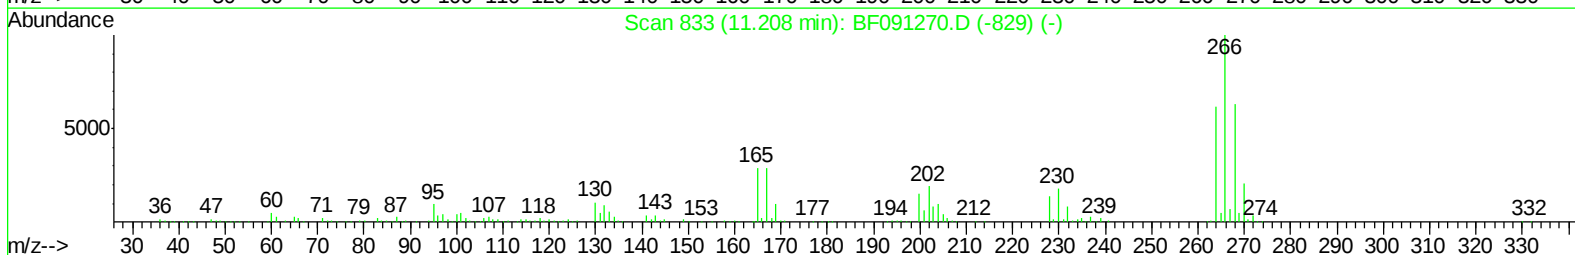
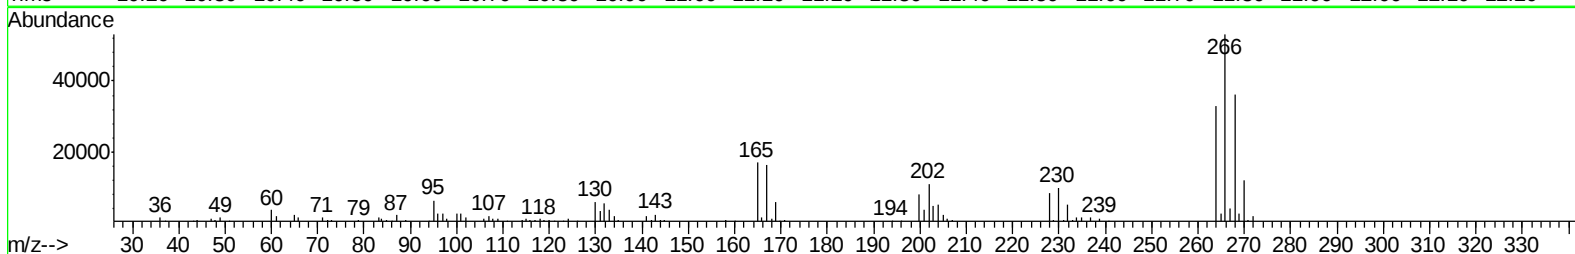


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112316\
Data File : BF091302.D
Acq On : 24 Nov 2016 8:32
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 00:45:44 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 13:22:53 2016
Response via : Initial Calibration

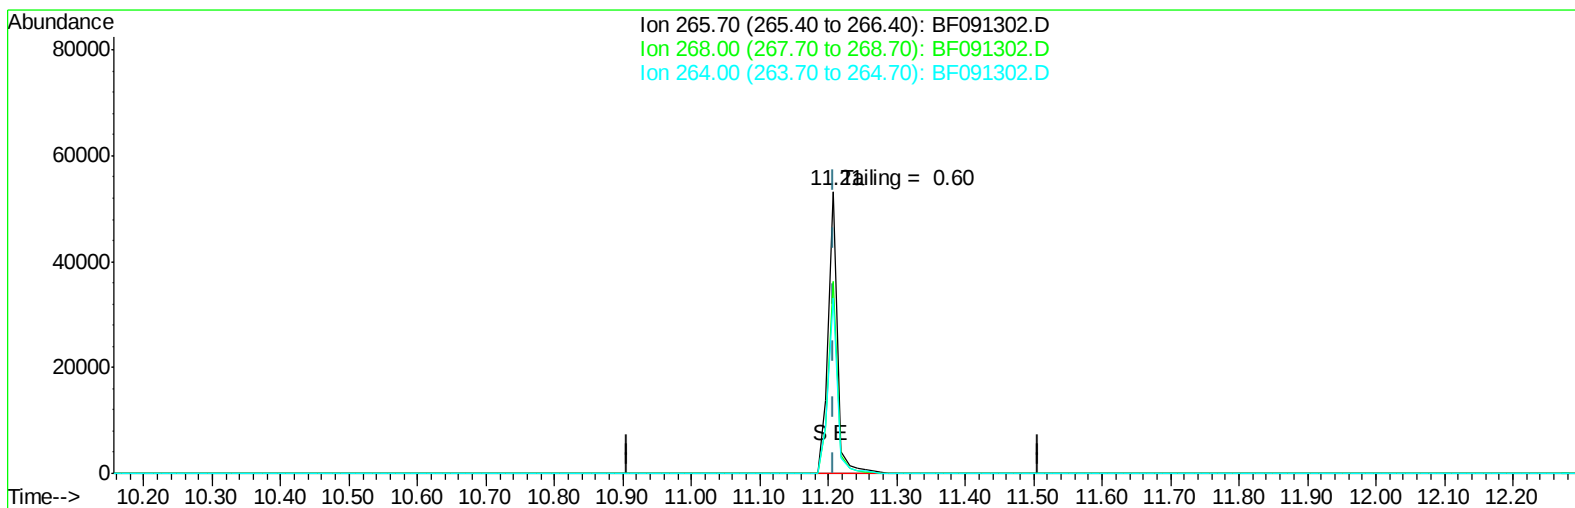

TIC: BF091302.D

(69) Pentachlorophenol (C)




11.208min (+0.000) 0.00ng

response 51305

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	68.11
264.00	60.20	62.13
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112316\
Data File : BF091302.D
Acq On : 24 Nov 2016 8:32
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 00:45:44 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 23 13:22:53 2016
Response via : Initial Calibration

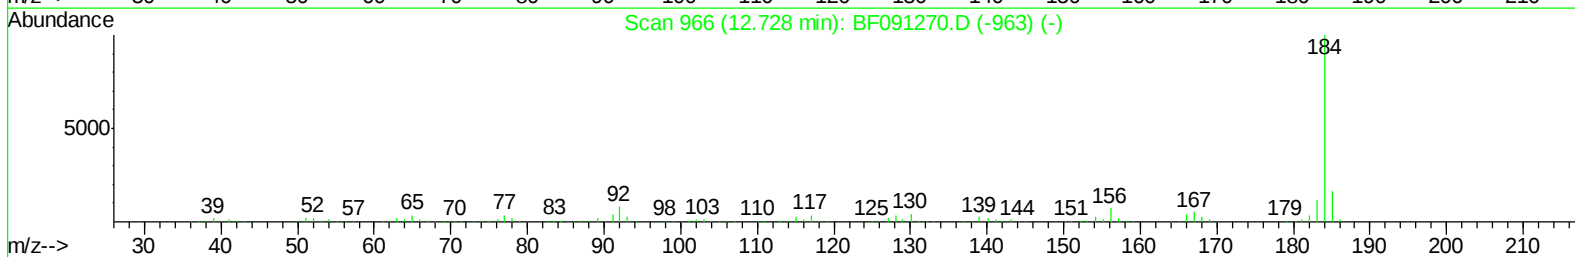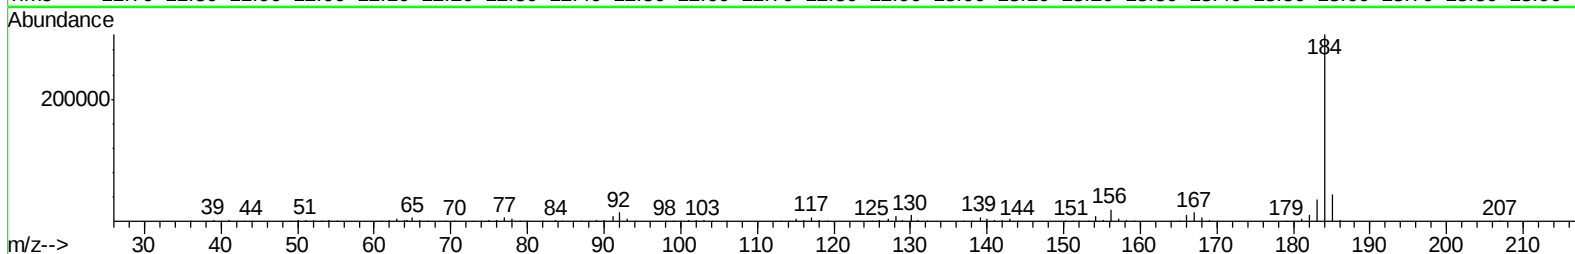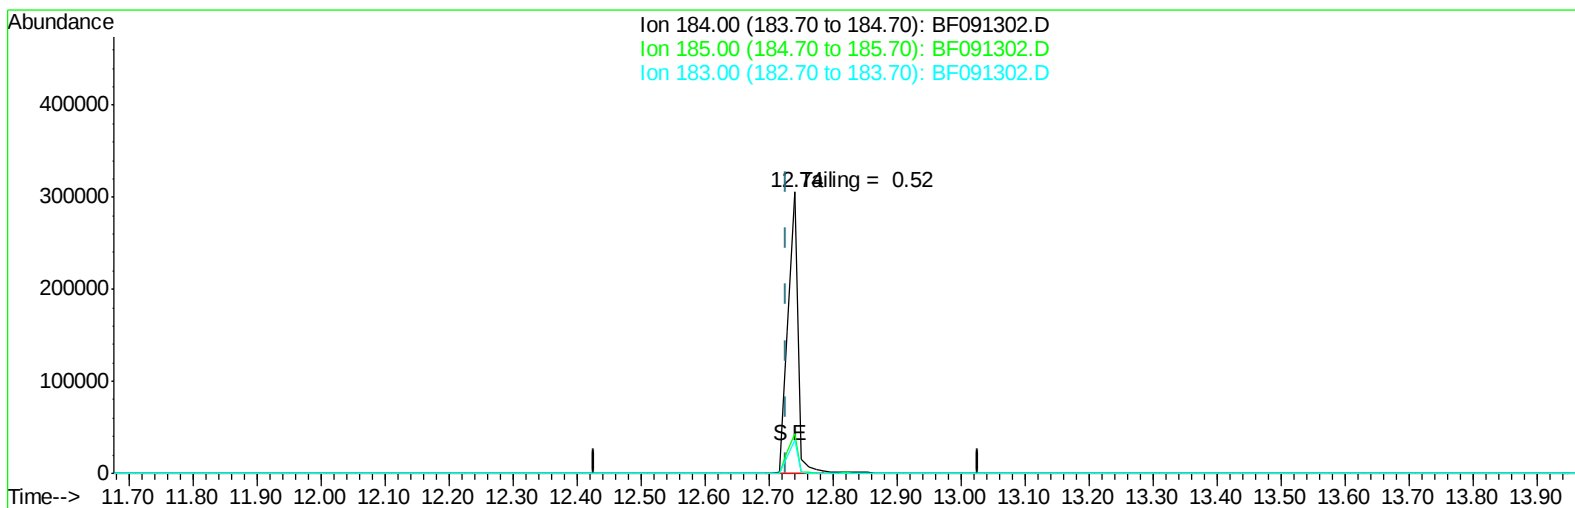

TIC: BF091302.D

(76) Benzidine

12.739min (+0.012) 0.00ng

response 343718

Ion	Exp%	Act%
184.00	100	100
185.00	16.40	14.15
183.00	11.10	11.91
0.00	0.00	0.00