


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112316\
Data File : BF091279.D
Acq On : 23 Nov 2016 16:48
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112316.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 23 13:22:53 2016

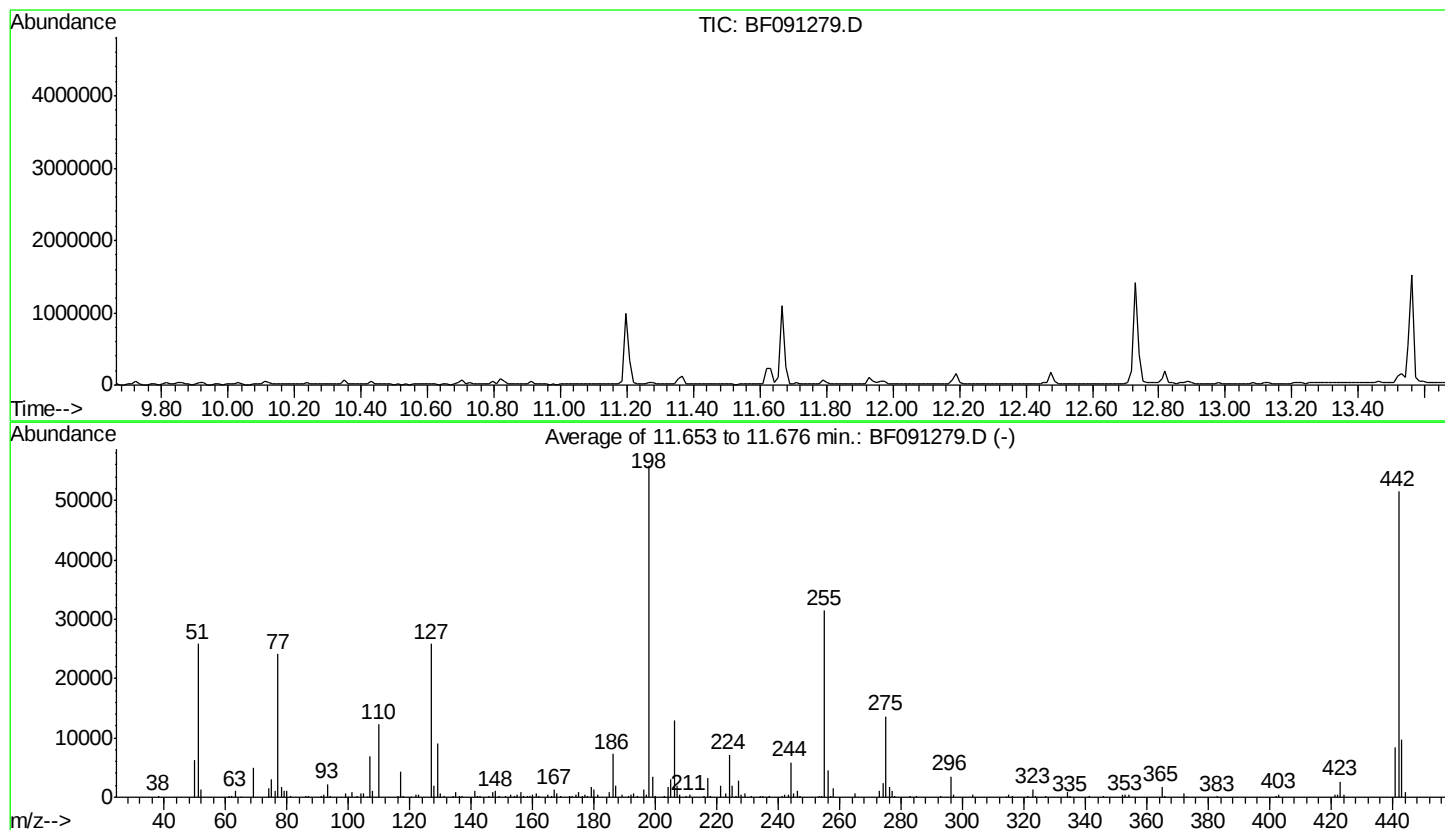

AutoFind: Scans 872, 873, 874; Background Corrected with Scan 869

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.2	25827	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	9.0	5052	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.2	25800	PASS
197	198	0.00	2	0.8	455	PASS
198	198	100	100	100.0	55860	PASS
199	198	5	9	6.3	3500	PASS
275	198	10	60	24.4	13618	PASS
365	198	1	100	3.3	1823	PASS
441	442	0.01	24	16.5	8484	PASS
442	198	50	100	92.2	51477	PASS
443	442	15	24	18.9	9710	PASS