


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112316\
 Data File : BF091302.D
 Acq On : 24 Nov 2016 8:32
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 23 13:22:53 2016

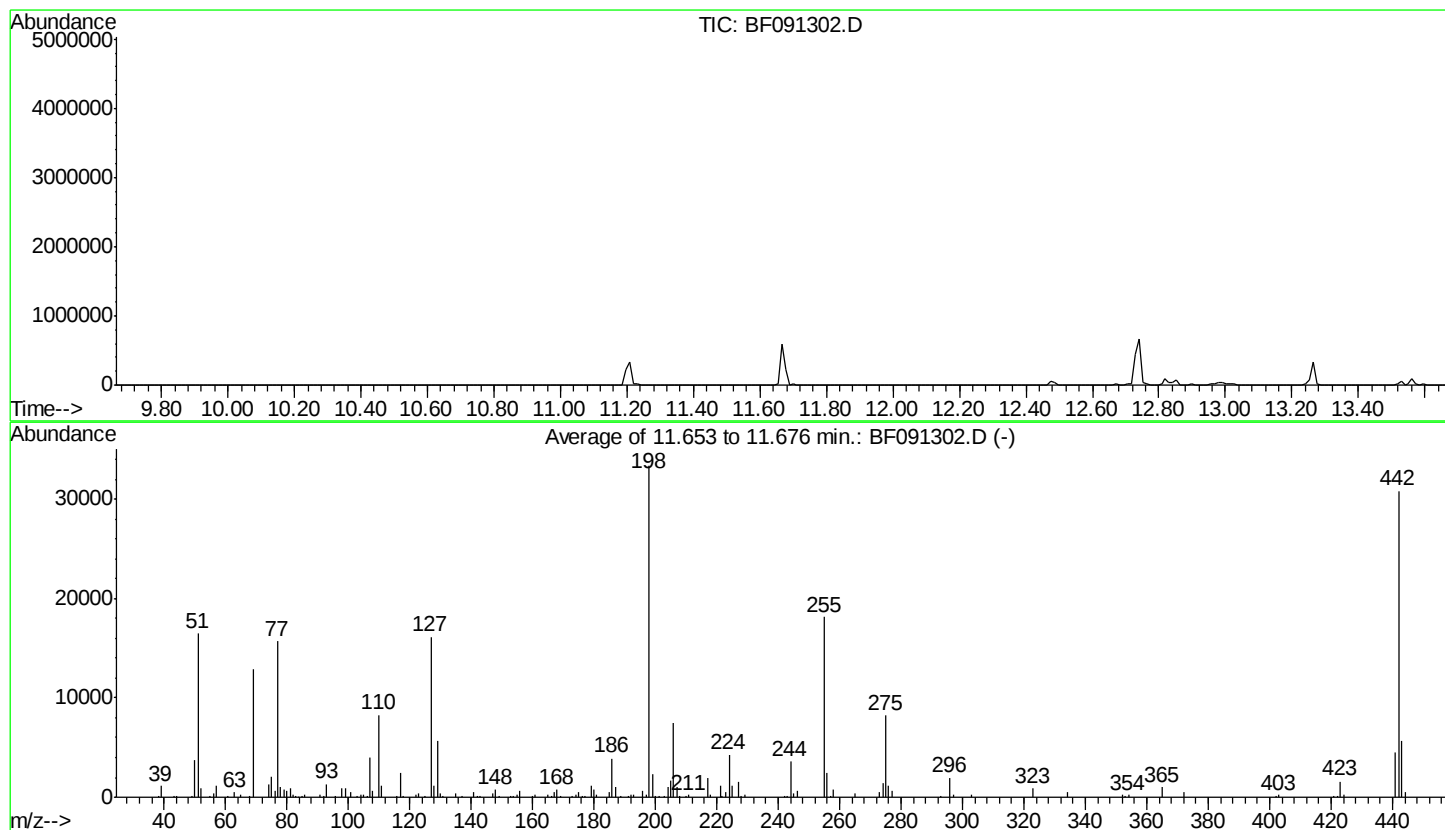

AutoFind: Scans 872, 873, 874; Background Corrected with Scan 869

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.3	16447	PASS
68	69	0.00	2	1.2	155	PASS
69	198	0.00	100	38.7	12899	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.3	16120	PASS
197	198	0.00	2	0.8	258	PASS
198	198	100	100	100.0	33360	PASS
199	198	5	9	7.0	2336	PASS
275	198	10	60	24.6	8190	PASS
365	198	1	100	3.1	1028	PASS
441	442	0.01	24	14.8	4568	PASS
442	198	50	100	92.4	30832	PASS
443	442	15	24	18.5	5700	PASS