
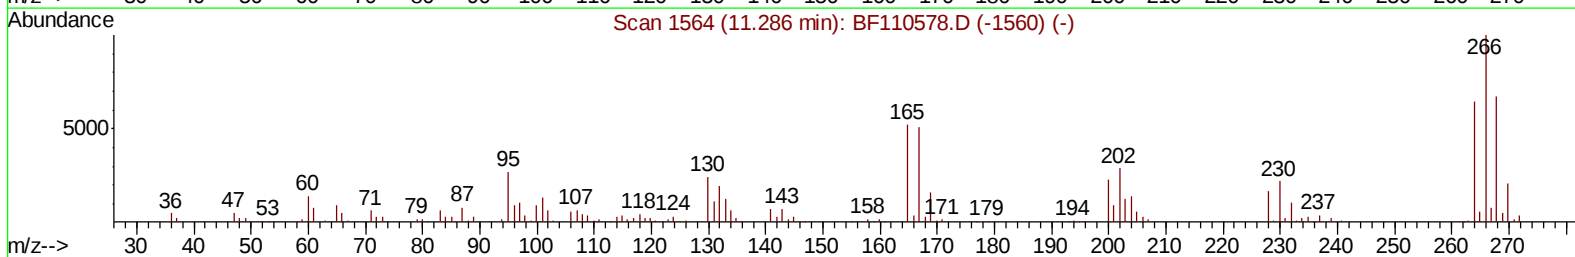
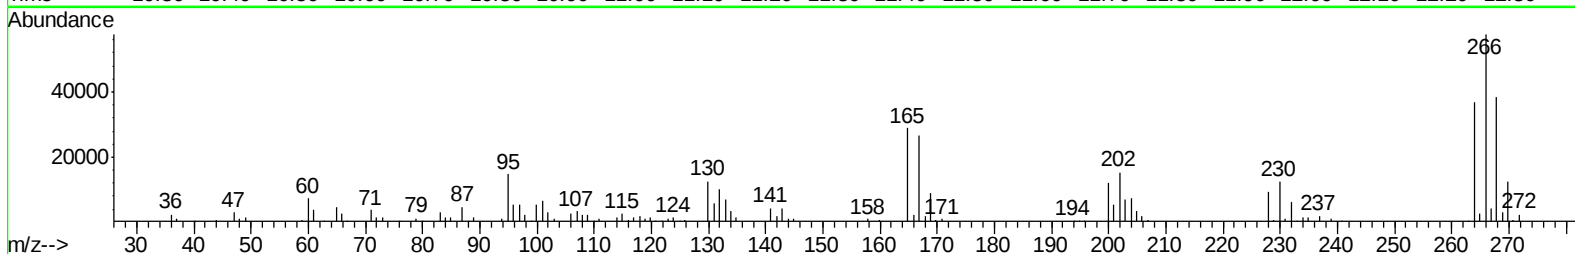


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112318\
Data File : BF110941.D
Acq On : 23 Nov 2018 10:58
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 23:35:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 12:43:10 2018
Response via : Initial Calibration

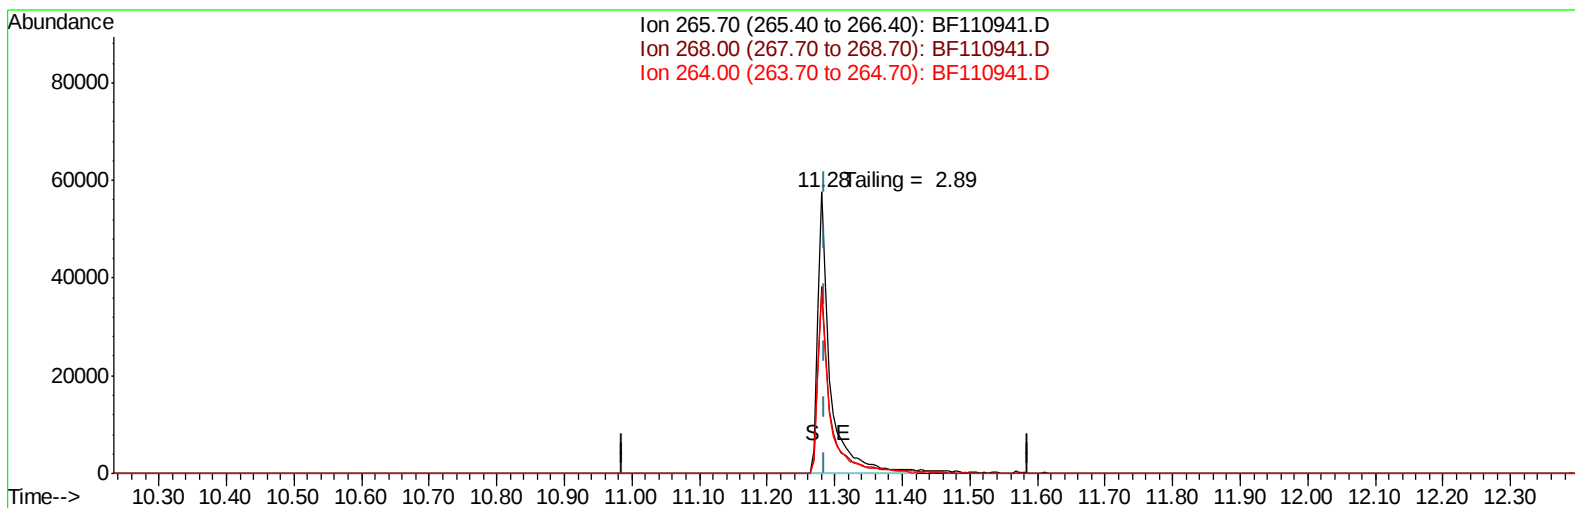

TIC: BF110941.D

(70) Pentachlorophenol (C)




11.280min (-0.006) 0.00ng

response 74689

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	66.32
264.00	63.20	64.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112318\
Data File : BF110941.D
Acq On : 23 Nov 2018 10:58
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 23 23:35:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 12:43:10 2018
Response via : Initial Calibration

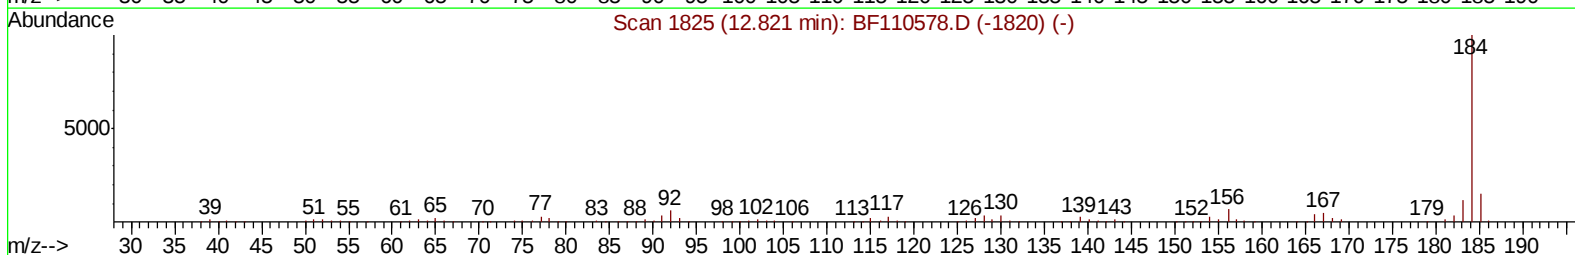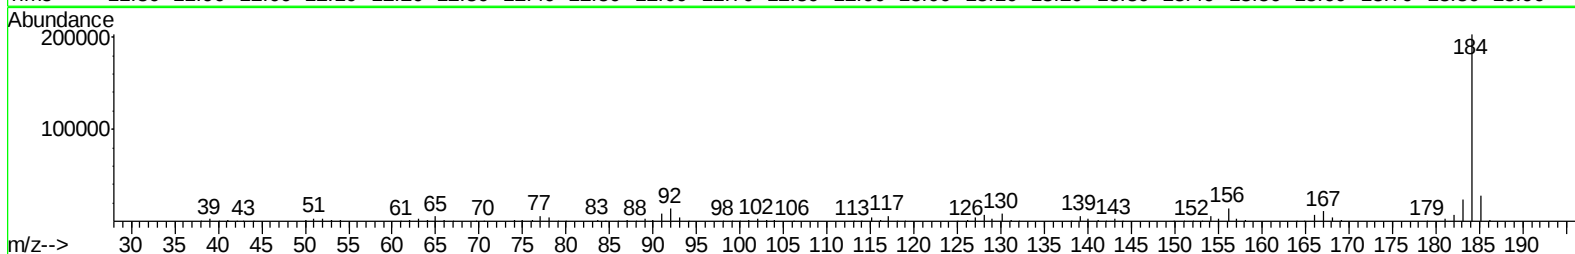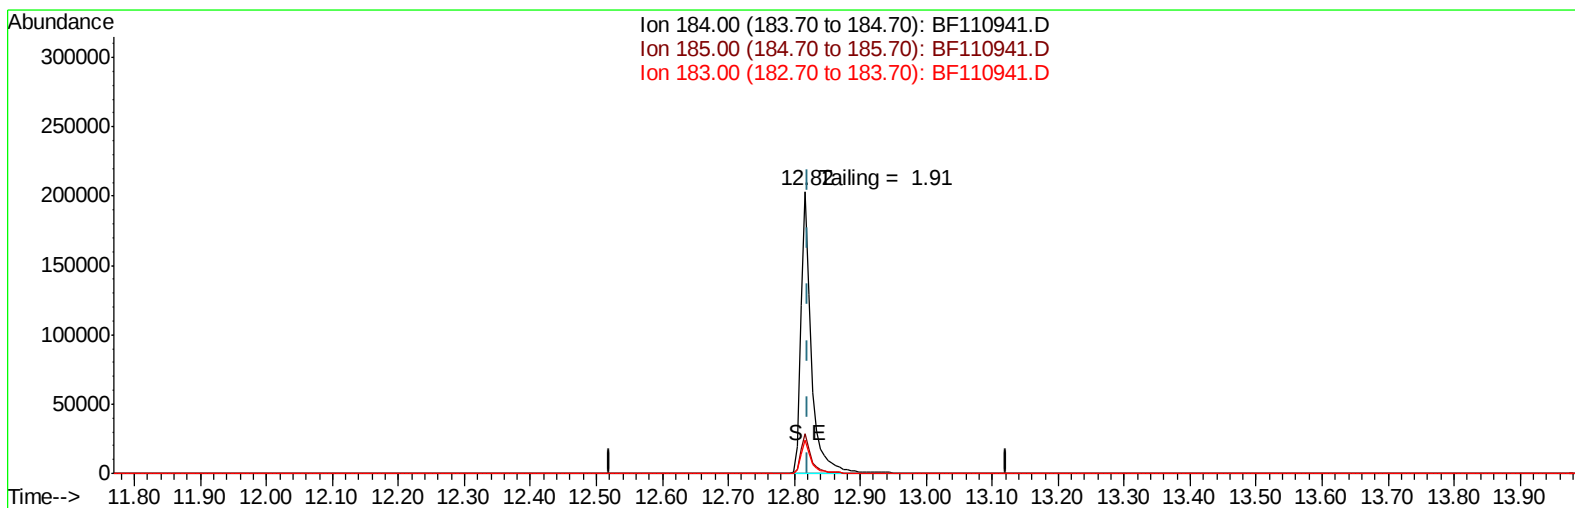

TIC: BF110941.D

(77) Benzidine

12.816min (-0.005) 0.00ng

response 226378

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.11
183.00	11.80	11.80
0.00	0.00	0.00