


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112318\
 Data File : BF110941.D
 Acq On : 23 Nov 2018 10:58
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 12:43:10 2018

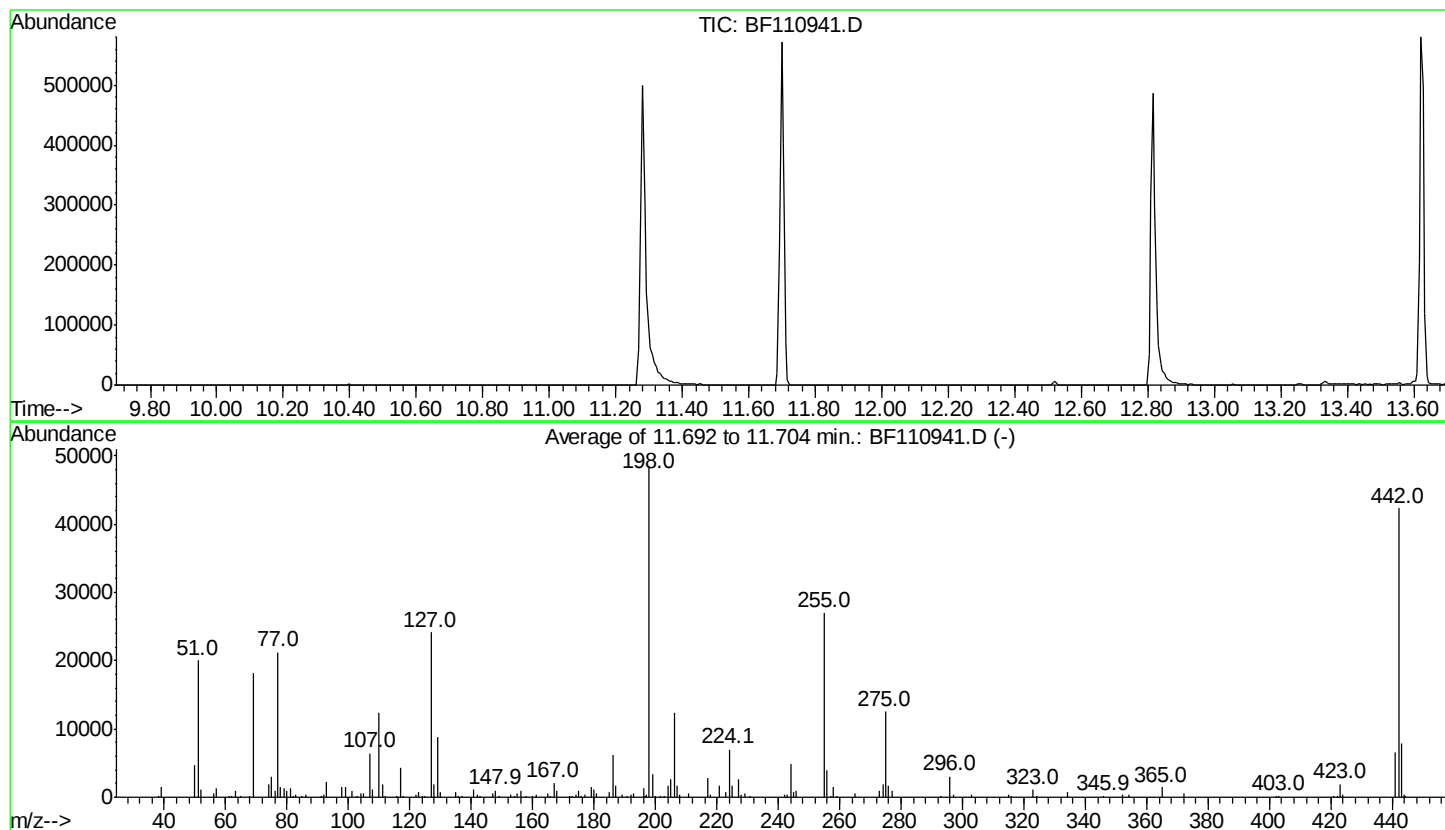

AutoFind: Scans 1633, 1634, 1635; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.3	20059	PASS
68	69	0.00	2	0.9	164	PASS
69	198	0.00	100	37.6	18258	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.6	24112	PASS
197	198	0.00	2	0.6	305	PASS
198	198	100	100	100.0	48584	PASS
199	198	5	9	6.8	3288	PASS
275	198	10	60	25.7	12509	PASS
365	198	1	100	3.1	1495	PASS
441	198	0.01	100	13.4	6522	PASS
442	198	50	100	87.2	42363	PASS
443	442	15	24	18.6	7875	PASS