

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112415\
 Data File : BF083240.D
 Acq On : 24 Nov 2015 16:48
 Operator : UM/IZ
 Sample : G4496-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 A17-COMP

Quant Time: Nov 25 00:28:27 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 22 09:22:46 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.62	152	170176	20.00	ng	-0.05
21) Naphthalene-d8	7.90	136	654274	20.00	ng	-0.06
38) Acenaphthene-d10	9.64	164	324583	20.00	ng	-0.06
63) Phenanthrene-d10	11.12	188	623747	20.00	ng	-0.06
75) Chrysene-d12	13.75	240	526474	20.00	ng	-0.06
86) Perylene-d12	15.11	264	253748	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.22	112	1446295	128.49	ng	-0.06
7) Phenol-d6	6.28	99	1862974	127.92	ng	-0.06
23) Nitrobenzene-d5	7.19	82	1348550	94.18	ng	-0.05
41) 2,4,6-Tribromophenol	10.44	330	473706	142.65	ng	-0.05
44) 2-Fluorobiphenyl	8.98	172	1996778	85.78	ng	-0.05
78) Terphenyl-d14	12.72	244	2198740	98.35	ng	-0.05
Target Compounds						
9) Benzaldehyde	6.28	77	2374	Below Cal	#	4
19) n-Nitroso-di-n-propylamine	7.19	70	177520	17.51	ng	# 72
50) 2,6-Dinitrotoluene	9.64	165	41907	7.47	ng	# 13
56) 2,4-Dinitrotoluene	9.64	165	41909	5.90	ng	# 10
66) 4-Bromophenyl-phenylether	10.43	248	30112	4.35	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112415\
Data File : BF083240.D
Acq On : 24 Nov 2015 16:48
Operator : UM/IZ
Sample : G4496-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
A17-COMP

Quant Time: Nov 25 00:28:27 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 09:22:46 2015
Response via : Initial Calibration

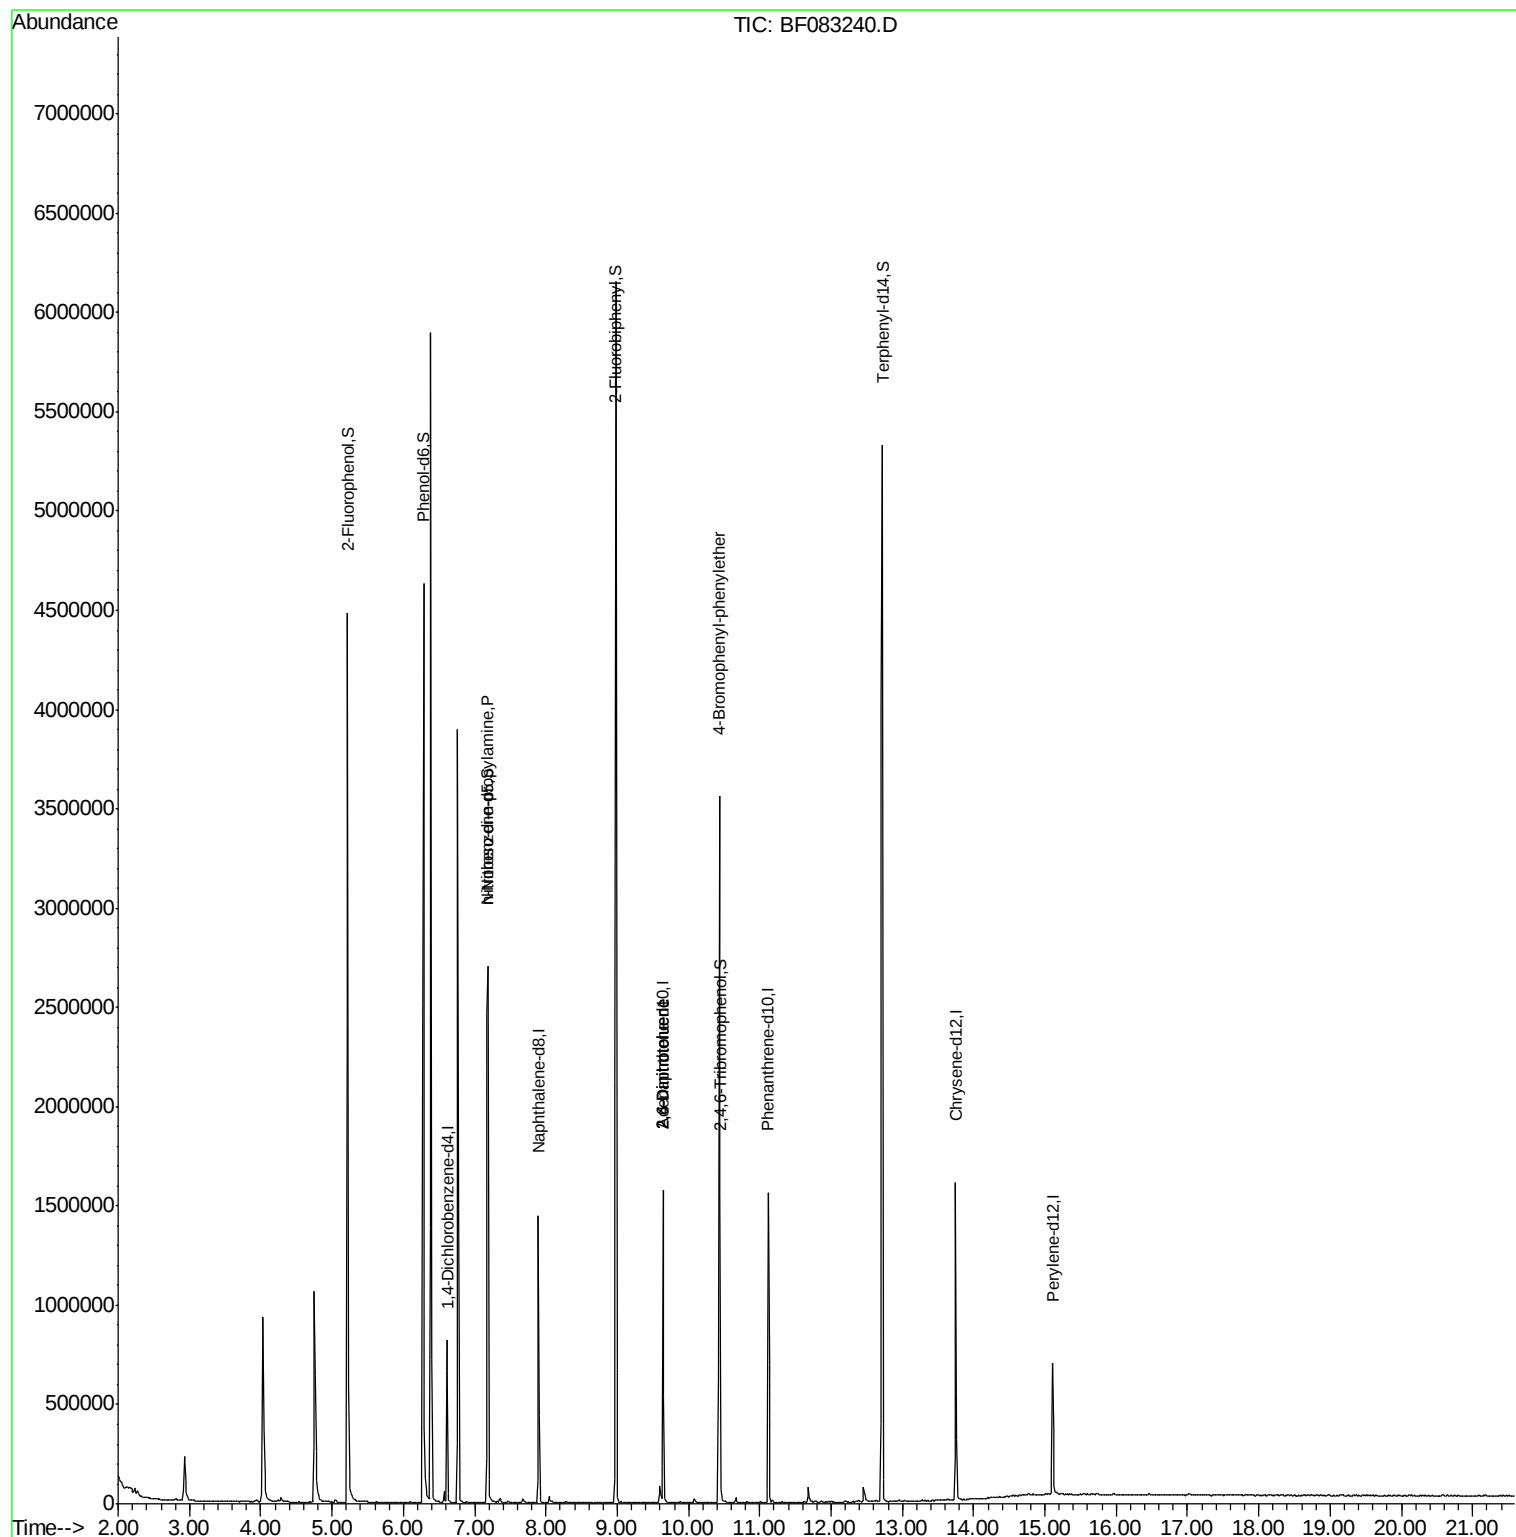

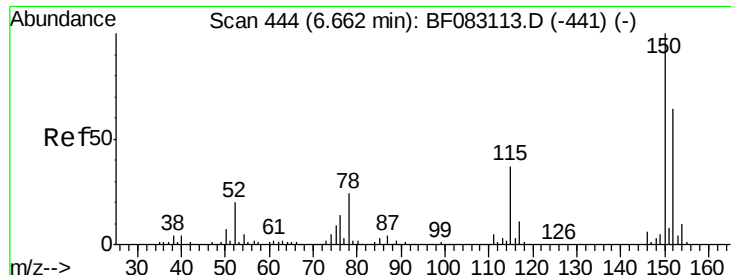


#1




1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 6.62 min Scan# 405
 Delta R.T. -0.05 min
 Lab File: BF083240.D
 Acq: 24 Nov 2015 16:48

Instrument :
 BNA_F
 ClientSampleId :
 A17-COMP

Tgt Ion:152 Resp: 170176
 Ion Ratio Lower Upper
 152 100
 150 151.3 125.8 188.8
 115 52.1 46.9 70.3

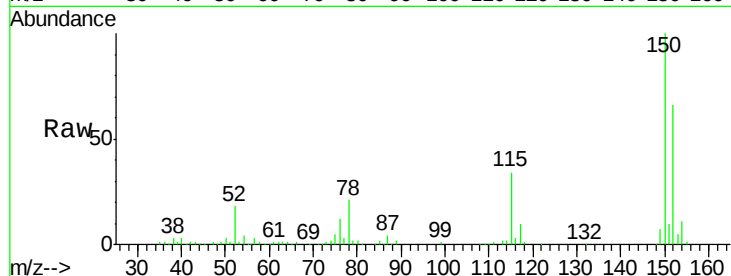


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

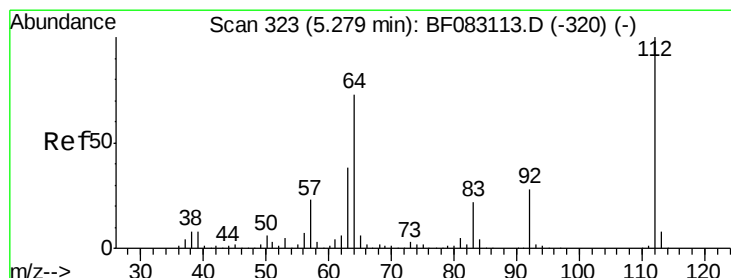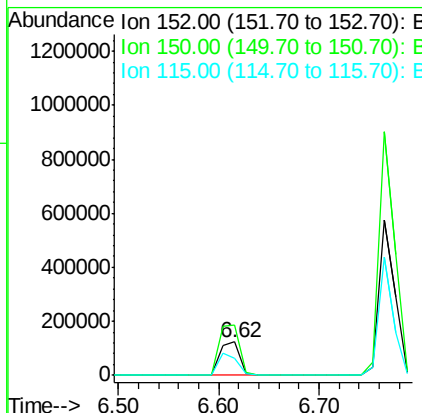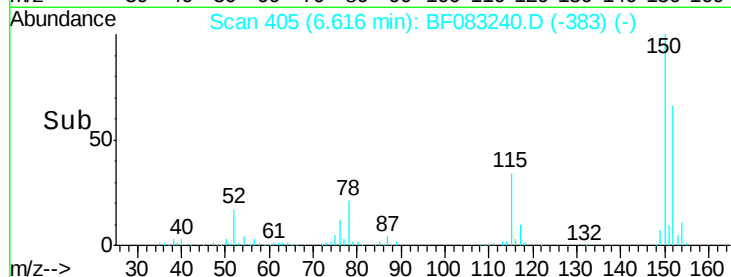



#5


2-Fluorophenol
 Concen: 128.49 ng
 RT: 5.22 min Scan# 283
 Delta R.T. -0.06 min
 Lab File: BF083240.D
 Acq: 24 Nov 2015 16:48

Tgt Ion:112 Resp: 1446295
 Ion Ratio Lower Upper
 112 100
 64 64.6 58.4 87.6
 63 32.0 30.0 45.0

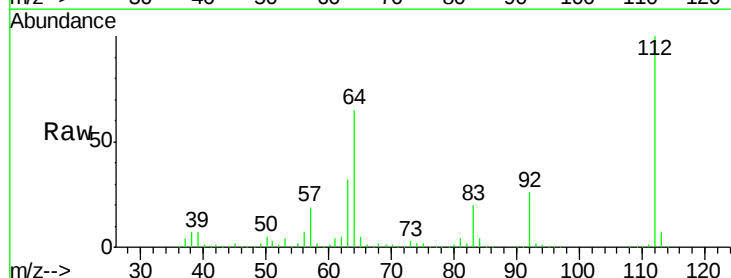

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

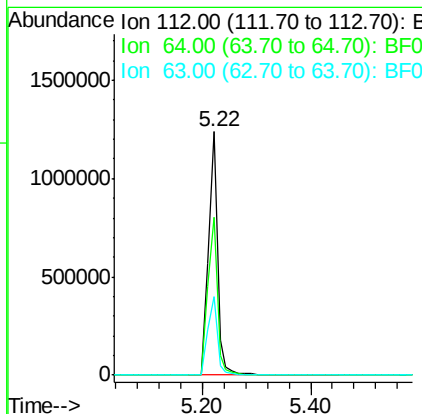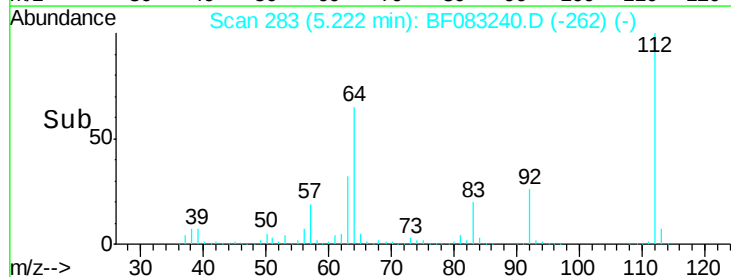

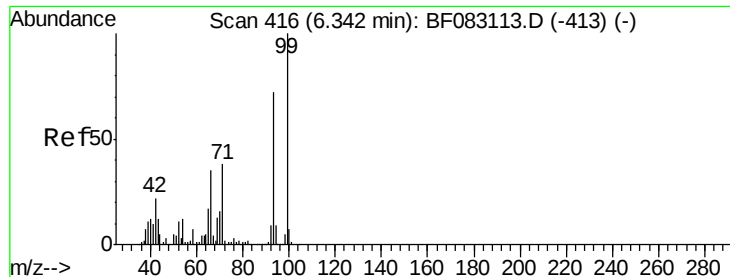

#7

Phenol-d6

Concen: 127.92 ng

RT: 6.28 min Scan# 376

Delta R.T. -0.06 min

Lab File: BF083240.D

Acq: 24 Nov 2015 16:48

Instrument :

BNA_F

ClientSampleId :

A17-COMP





Tgt Ion: 99 Resp: 1862974

Ion Ratio Lower Upper

99 100

42 19.5 17.7 26.5

71 33.0 30.2 45.4

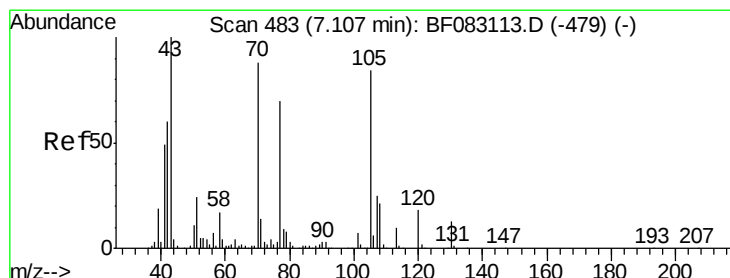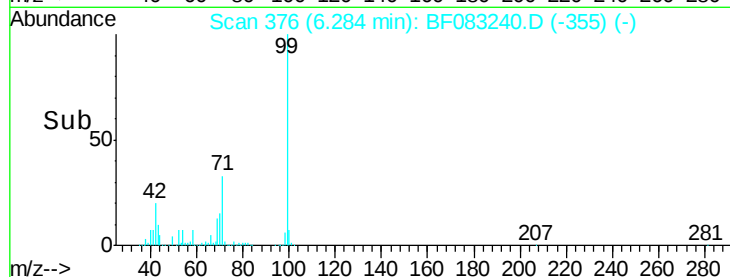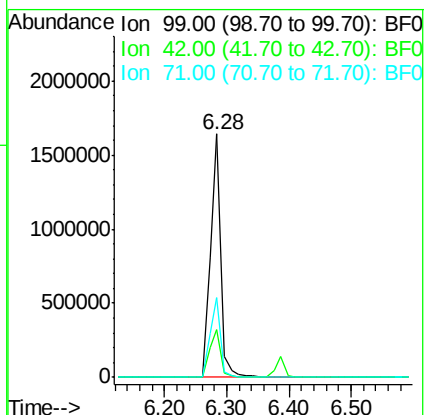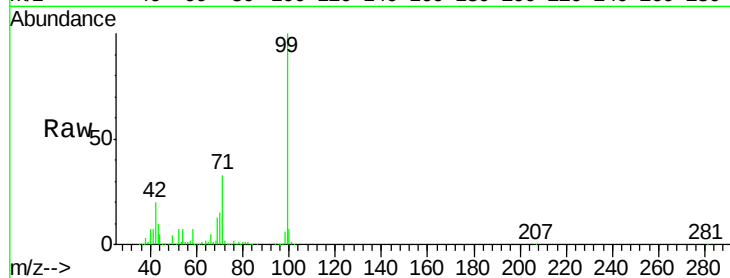

#19

n-Nitroso-di-n-propylamine

Concen: 17.51 ng

RT: 7.19 min Scan# 455

Delta R.T. 0.08 min

Lab File: BF083240.D

Acq: 24 Nov 2015 16:48

Tgt Ion: 70 Resp: 177520




Ion Ratio Lower Upper


70 100

42 45.7 54.5 81.7#

101 0.0 6.6 9.8#

130 2.1 11.5 17.3#

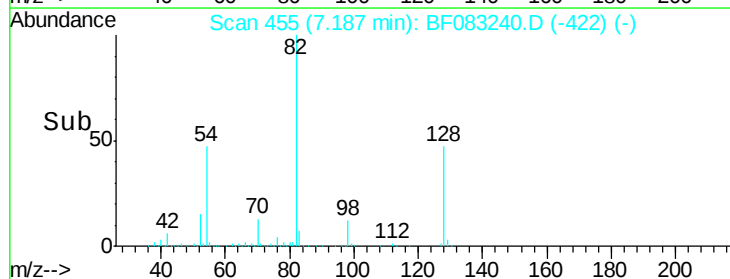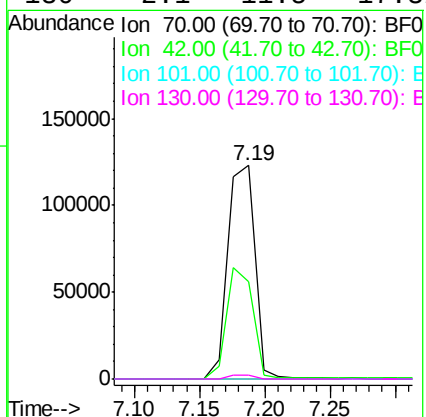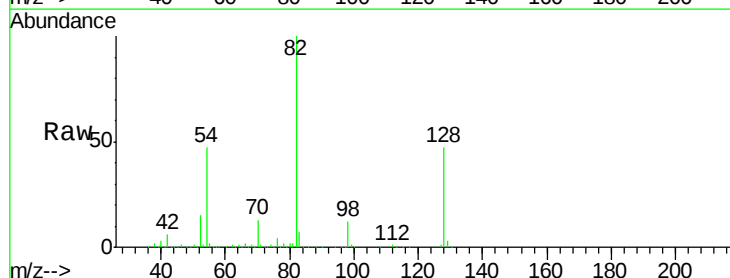

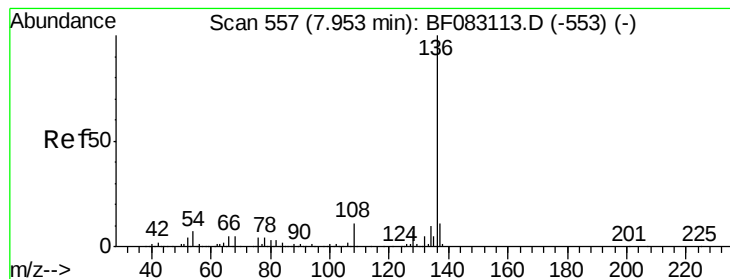

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.90 min Scan# 517

Delta R.T. -0.06 min

Lab File: BF083240.D

Acq: 24 Nov 2015 16:48

Instrument :

BNA_F

ClientSampleId :

A17-COMP

Tgt Ion:136 Resp: 654274


Ion Ratio Lower Upper

136 100

137 11.3 8.7 13.1

54 11.8 5.8 8.6#

68 8.3 3.8 5.8#

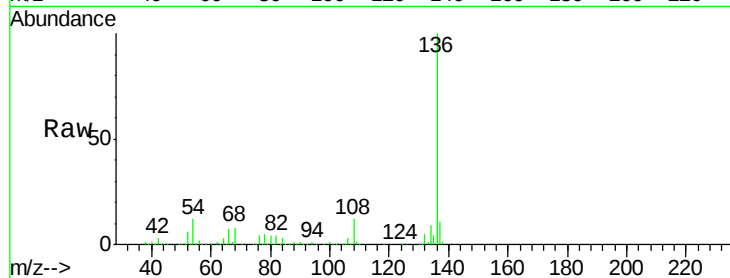


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

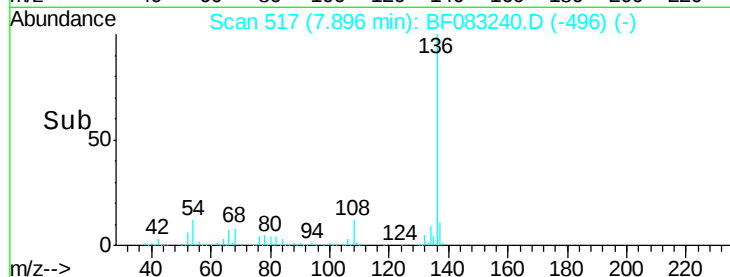

Abundance


Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

Time-->

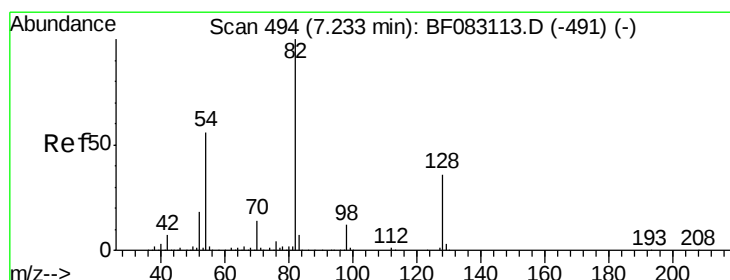

#23

Nitrobenzene-d5

Concen: 94.18 ng

RT: 7.19 min Scan# 455

Delta R.T. -0.05 min

Lab File: BF083240.D

Acq: 24 Nov 2015 16:48


Tgt Ion: 82 Resp: 1348550

Ion Ratio Lower Upper

82 100

128 46.9 28.5 42.7#


54 46.5 44.6 67.0

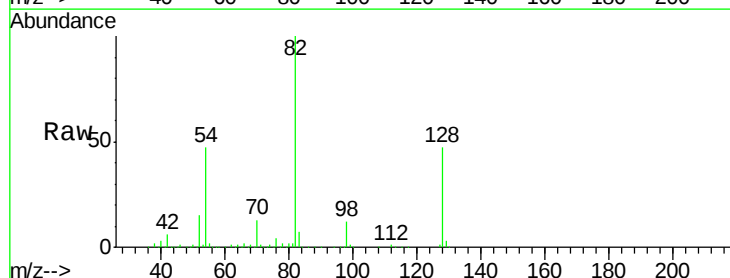

Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

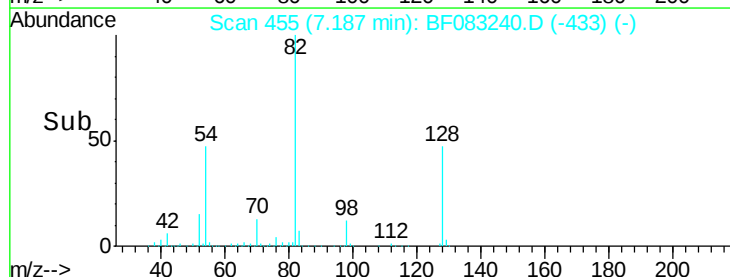


Abundance

Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0





Time-->

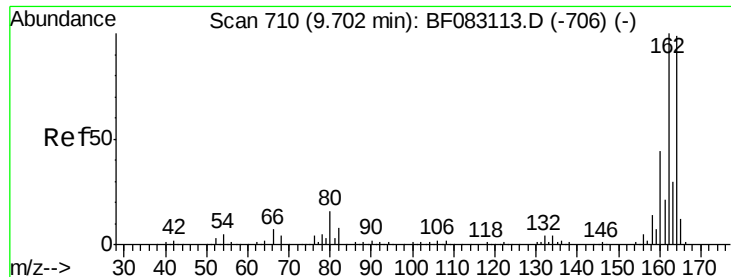

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.64 min Scan# 670
 Delta R.T. -0.06 min
 Lab File: BF083240.D
 Acq: 24 Nov 2015 16:48




Instrument :
 BNA_F
 ClientSampleId :
 A17-COMP


Tgt Ion:164 Resp: 324583
 Ion Ratio Lower Upper
 164 100
 162 102.3 81.2 121.8
 160 44.3 35.6 53.4

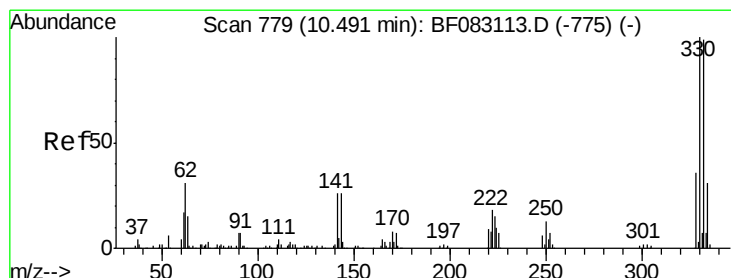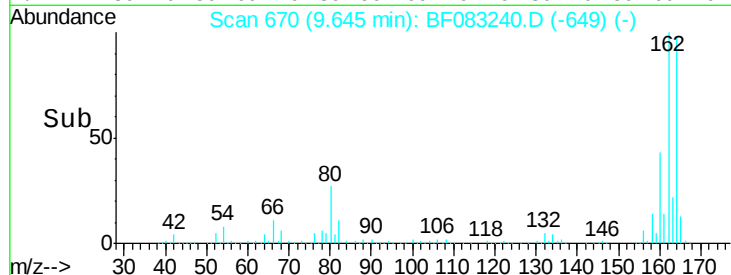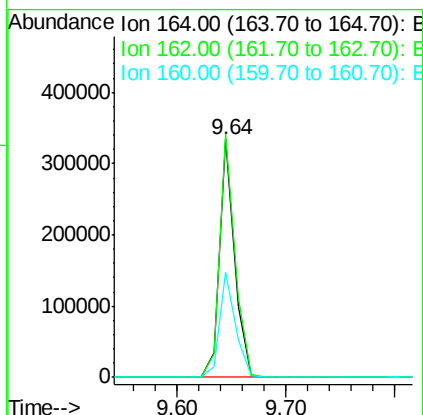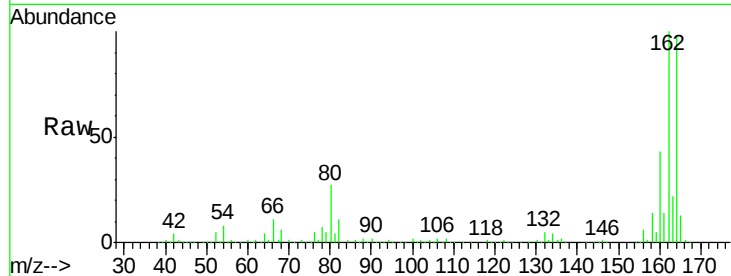

#41
 2,4,6-Tribromophenol
 Concen: 142.65 ng
 RT: 10.44 min Scan# 740
 Delta R.T. -0.05 min
 Lab File: BF083240.D
 Acq: 24 Nov 2015 16:48

Tgt Ion:330 Resp: 473706
 Ion Ratio Lower Upper
 330 100
 332 94.9 77.7 116.5
 141 35.4 29.7 44.5

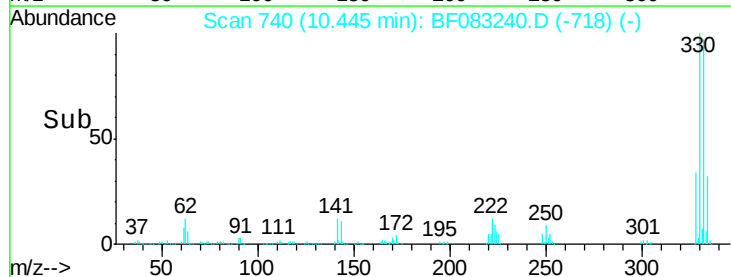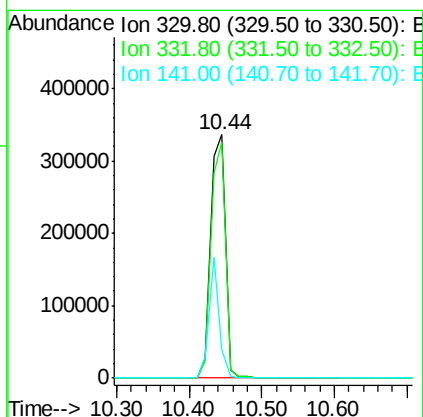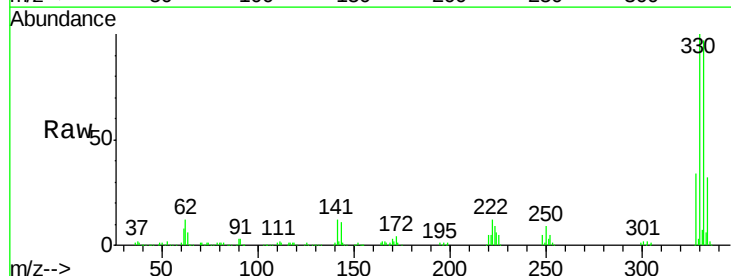


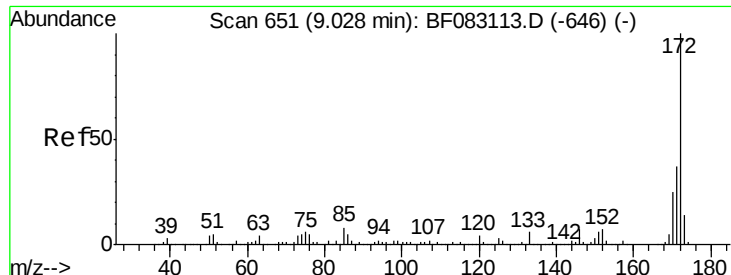




#44
 2-Fluorobiphenyl
 Concen: 85.78 ng
 RT: 8.98 min Scan# 612
 Delta R.T. -0.05 min
 Lab File: BF083240.D
 Acq: 24 Nov 2015 16:48

Instrument :
 BNA_F
 ClientSampleId :
 A17-COMP

Tgt Ion:172 Resp: 1996778
 Ion Ratio Lower Upper
 172 100
 171 37.6 29.5 44.3
 170 25.2 19.9 29.9

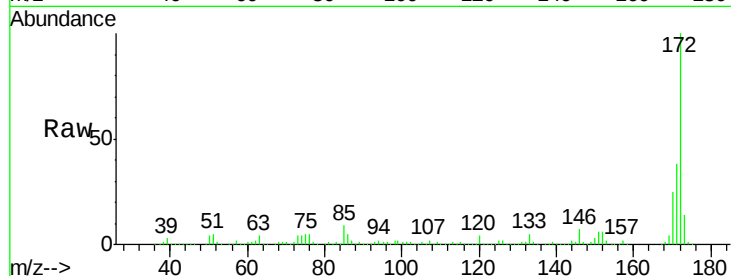


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

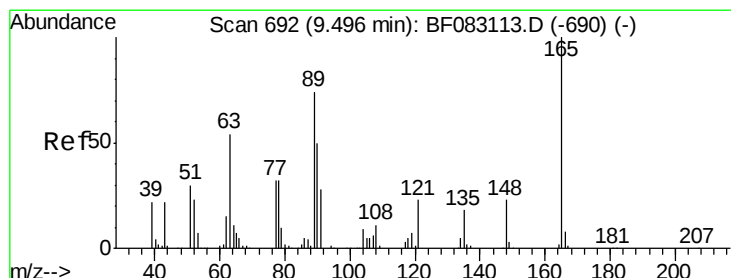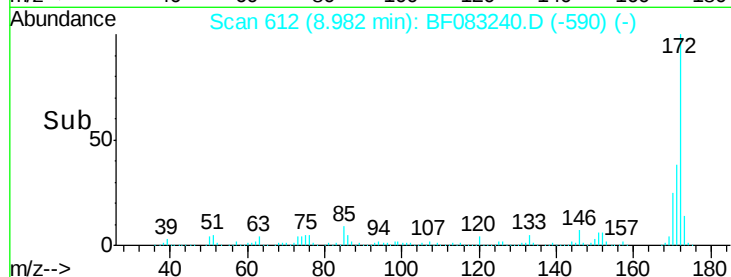
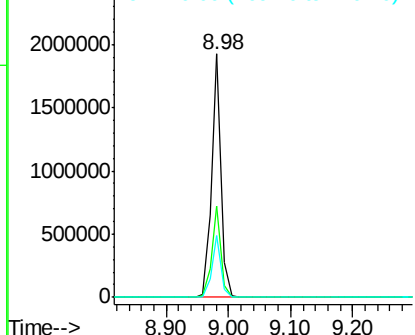



#50
 2,6-Dinitrotoluene
 Concen: 7.47 ng
 RT: 9.64 min Scan# 670
 Delta R.T. 0.15 min
 Lab File: BF083240.D
 Acq: 24 Nov 2015 16:48

Tgt Ion:165 Resp: 41907
 Ion Ratio Lower Upper
 165 100
 63 1.8 62.5 93.7#
 89 1.7 59.1 88.7#

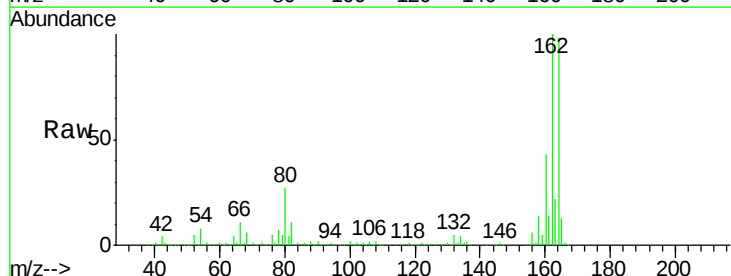

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0

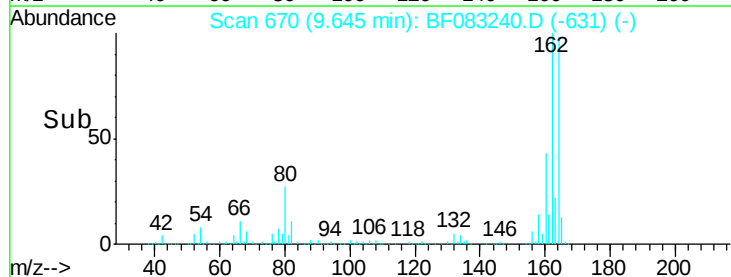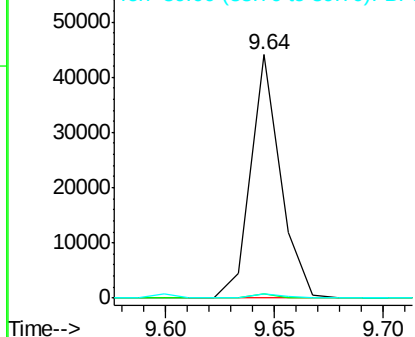


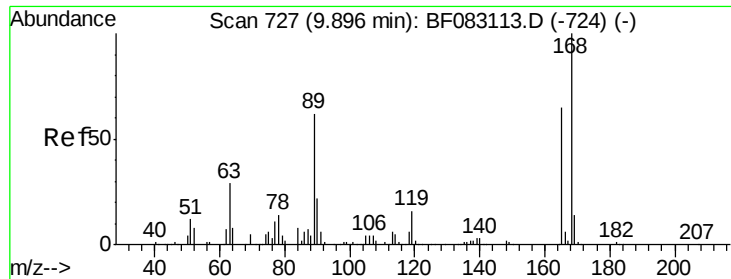




#56
2,4-Dinitrotoluene
Concen: 5.90 ng
RT: 9.64 min Scan# 670
Delta R.T. -0.25 min
Lab File: BF083240.D
Acq: 24 Nov 2015 16:48

Instrument :
BNA_F
ClientSampleId :
A17-COMP

Tgt Ion:165 Resp: 41909
Ion Ratio Lower Upper
165 100
63 1.8 54.5 81.7#
89 1.7 77.3 115.9#
182 0.0 1.8 2.6#

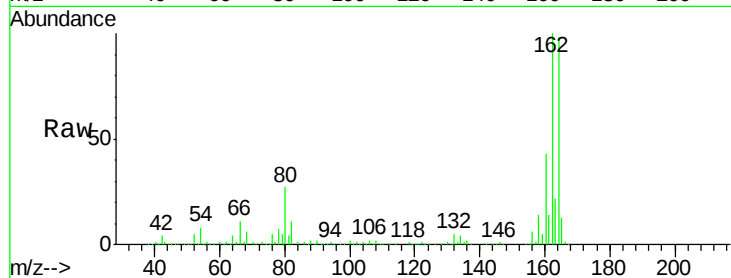


Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF0
Ion 89.00 (88.70 to 89.70): BF0
Ion 182.00 (181.70 to 182.70): E

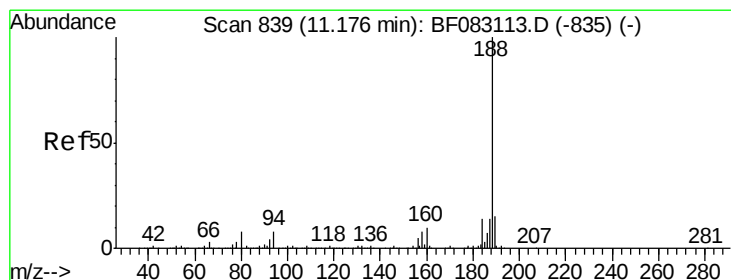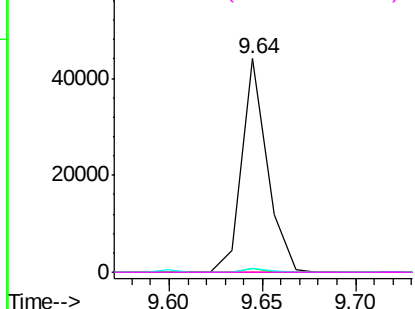
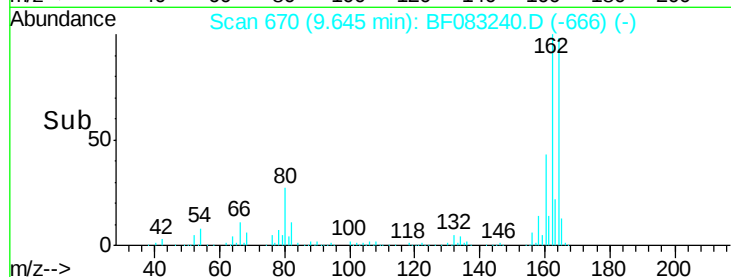



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.12 min Scan# 799
Delta R.T. -0.06 min
Lab File: BF083240.D
Acq: 24 Nov 2015 16:48

Tgt Ion:188 Resp: 623747
Ion Ratio Lower Upper
188 100
94 13.6 6.0 9.0#
80 15.9 6.7 10.1#

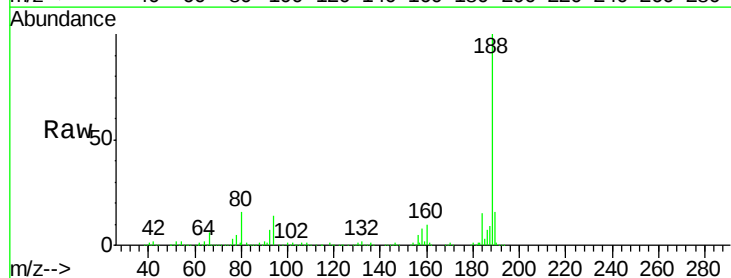

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

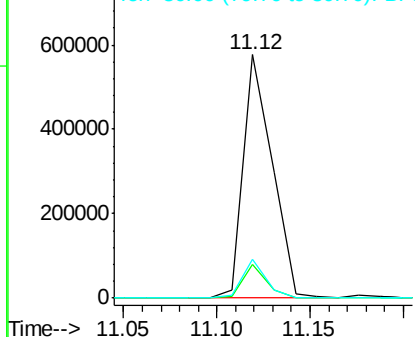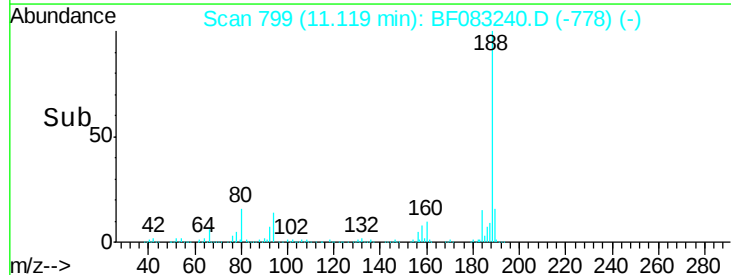

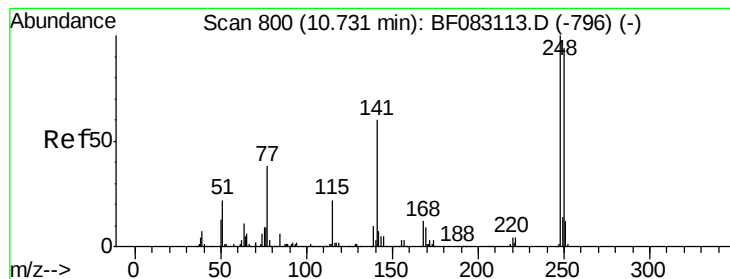

#66

4-Bromophenyl-phenylether

Concen: 4.35 ng

RT: 10.43 min Scan# 739

Delta R.T. -0.30 min

Lab File: BF083240.D

Acq: 24 Nov 2015 16:48

Instrument :

BNA_F

ClientSampleId :

A17-COMP


Tgt Ion:248 Resp: 30112

Ion Ratio Lower Upper

248 100

250 200.8 75.4 113.2#




141 671.8 48.1 72.1#

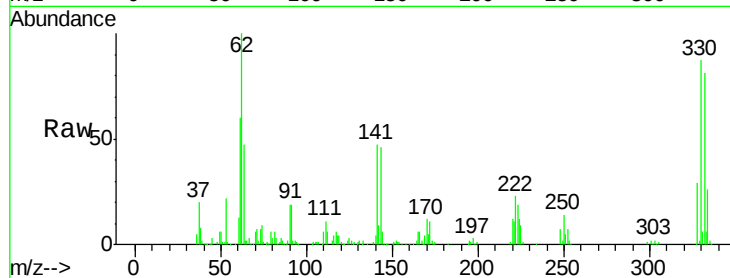

Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

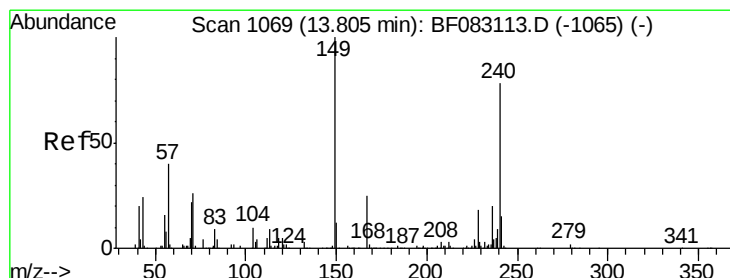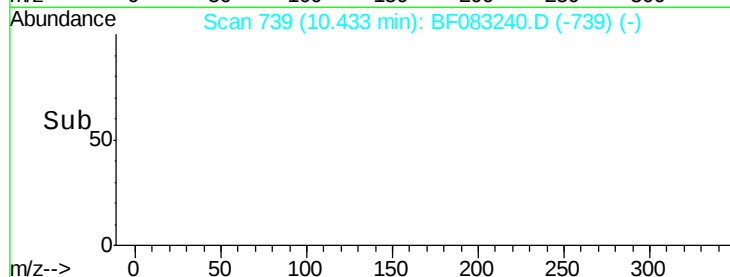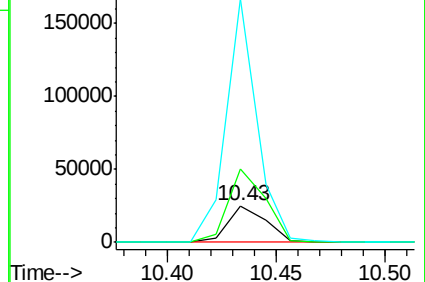

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.75 min Scan# 1029

Delta R.T. -0.06 min

Lab File: BF083240.D

Acq: 24 Nov 2015 16:48


Tgt Ion:240 Resp: 526474

Ion Ratio Lower Upper

240 100

120 12.2 5.4 8.2#



236 25.4 20.6 31.0

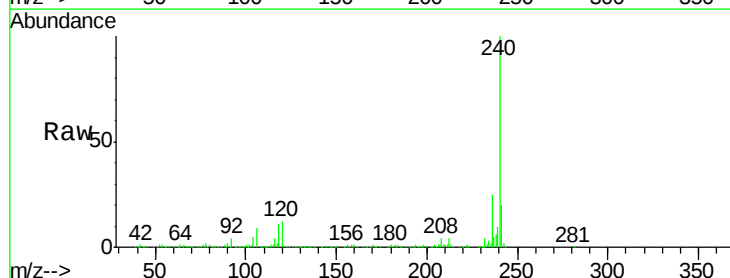


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



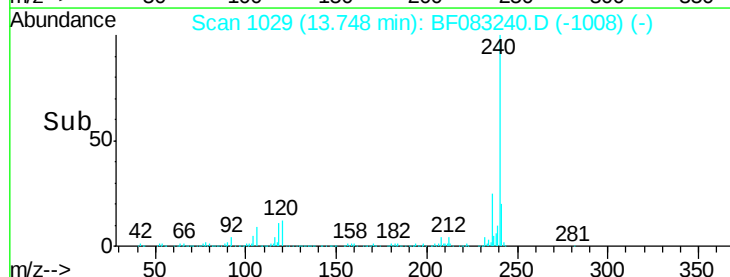
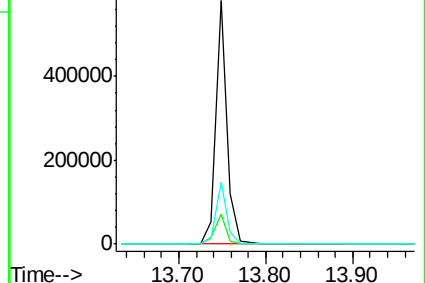


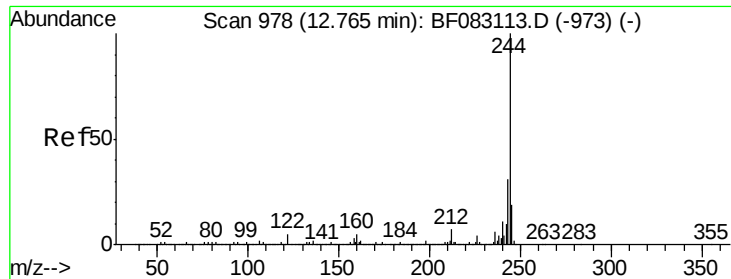

#78
 Terphenyl-d14
 Concen: 98.35 ng
 RT: 12.72 min Scan# 939
 Delta R.T. -0.05 min
 Lab File: BF083240.D
 Acq: 24 Nov 2015 16:48

Instrument :
 BNA_F
 ClientSampleId :
 A17-COMP

Tgt Ion:244 Resp: 2198740
 Ion Ratio Lower Upper
 244 100
 212 7.4 5.4 8.2
 122 8.9 4.3 6.5#

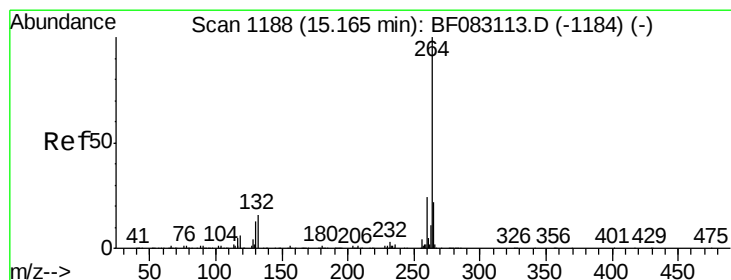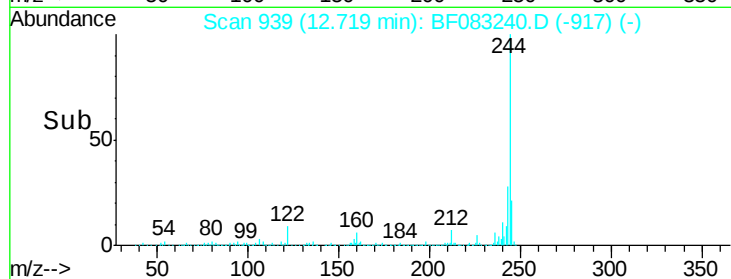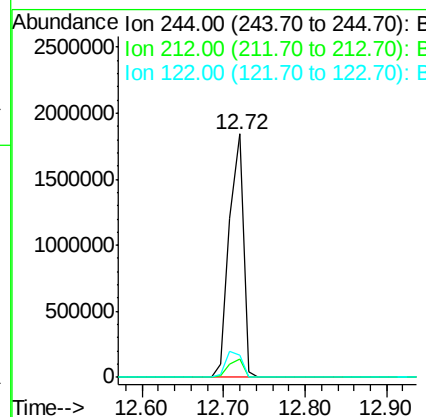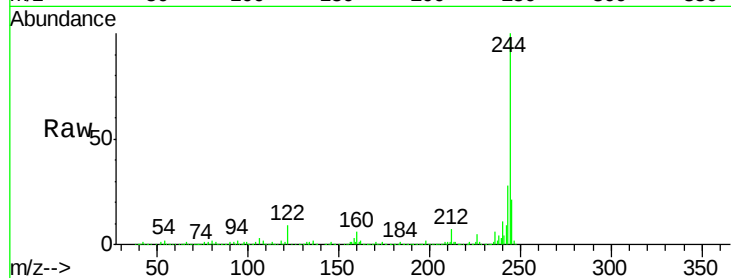

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.11 min Scan# 1148
 Delta R.T. -0.06 min
 Lab File: BF083240.D
 Acq: 24 Nov 2015 16:48

Tgt Ion:264 Resp: 253748
 Ion Ratio Lower Upper
 264 100
 260 24.0 19.1 28.7
 265 22.1 18.2 27.4

