
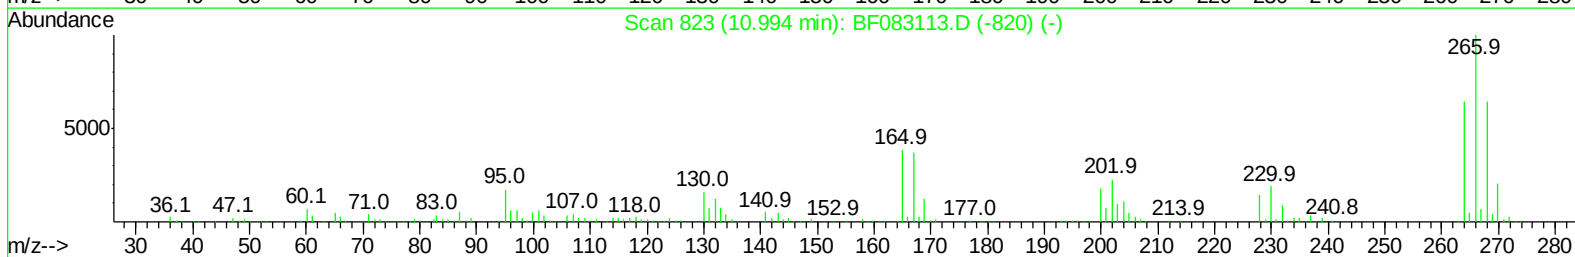
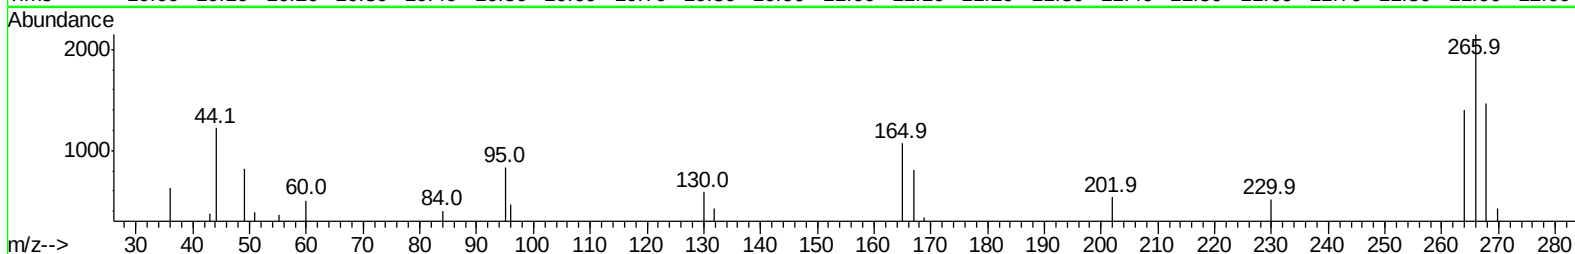


Data Path : Z:\HPCHEM1\BNA F\Data\BF112415\
Data File : BF083241.D
Acq On : 24 Nov 2015 17:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 07:34:36 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 09:22:46 2015
Response via : Initial Calibration

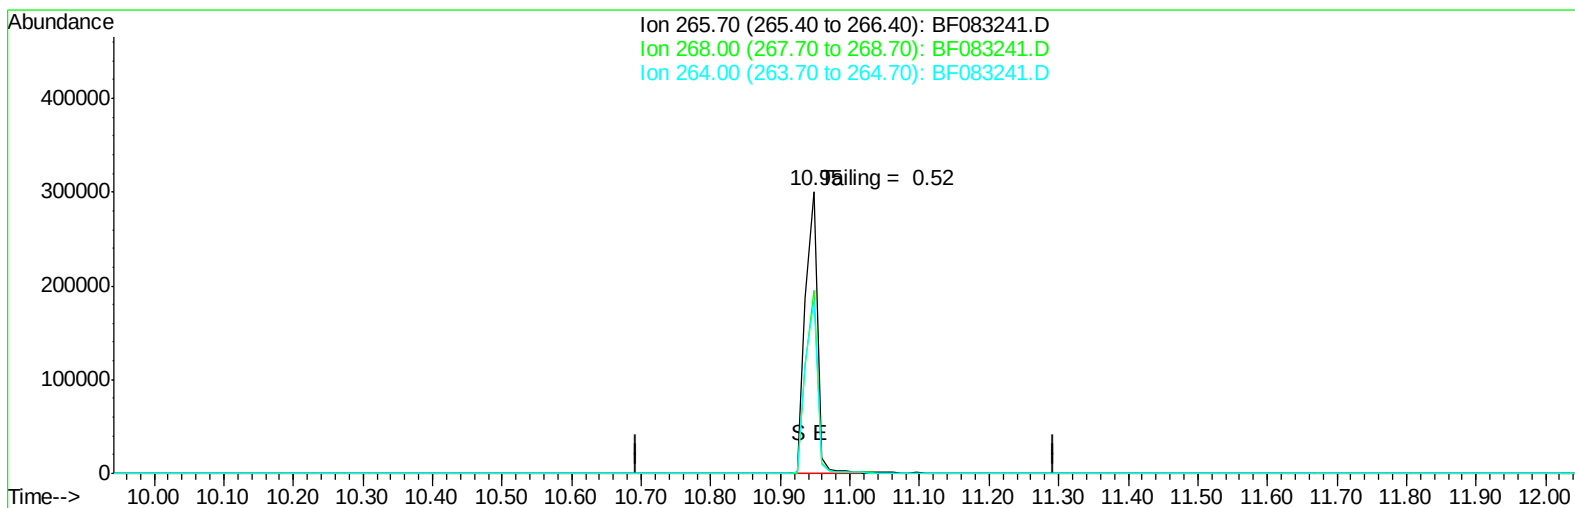

TIC: BF083241.D

(69) Pentachlorophenol (C)




10.994min (-10.994) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	64.20	0.00#
264.00	64.60	0.00#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF112415\
Data File : BF083241.D
Acq On : 24 Nov 2015 17:17
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 25 07:34:36 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 09:22:46 2015
Response via : Initial Calibration

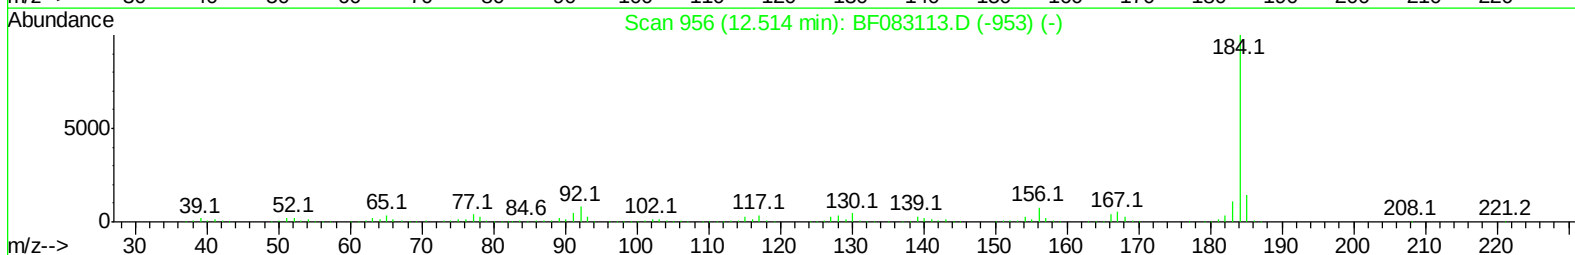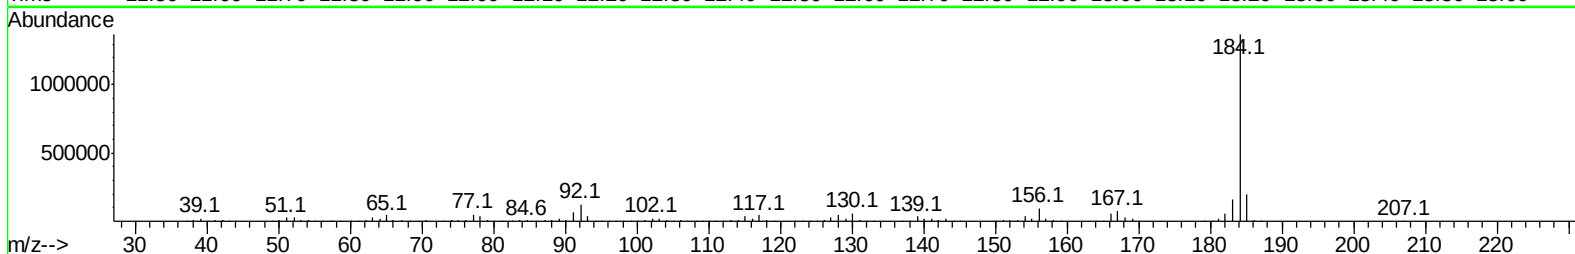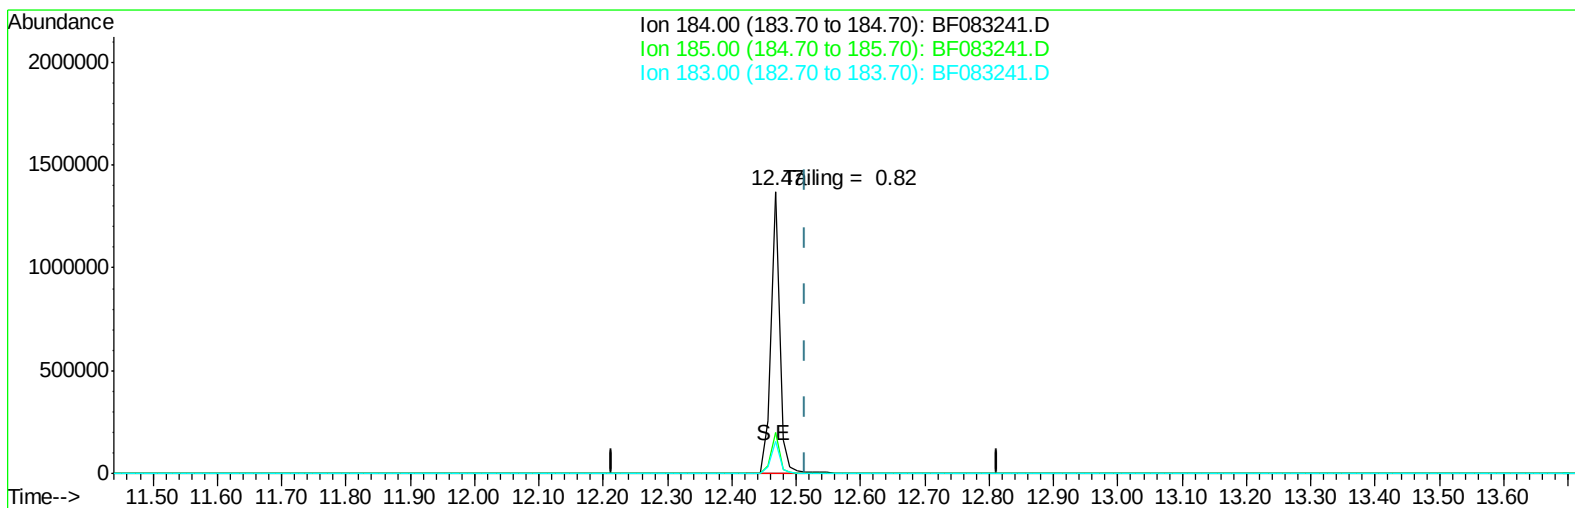

TIC: BF083241.D

(76) Benzidine

12.468min (-0.046) 0.00ng

response 1288055

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	14.53
183.00	11.00	11.55
0.00	0.00	0.00