
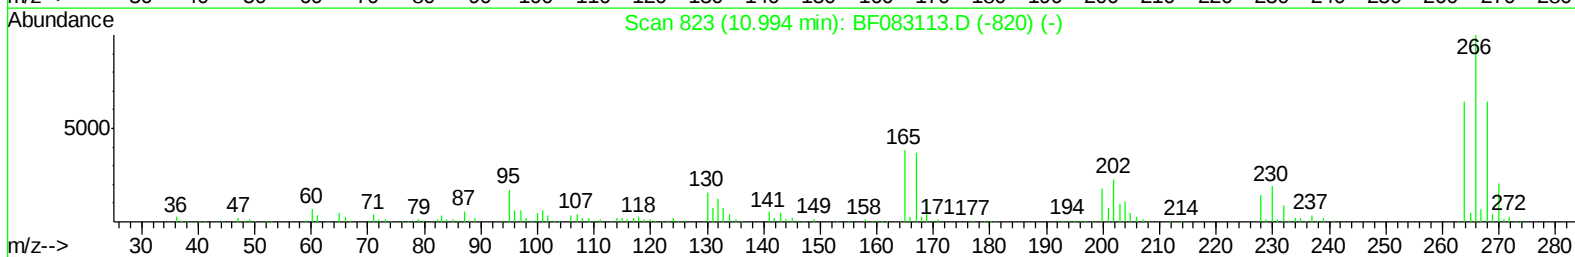
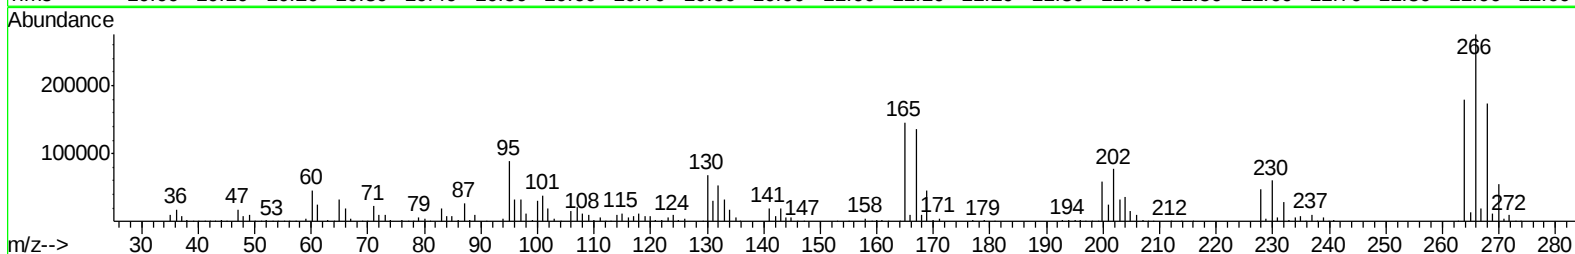


Data Path : Z:\HPCHEM1\BNA F\Data\BF112415\
Data File : BF083231.D
Acq On : 24 Nov 2015 10:56
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 11:29:21 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 09:22:46 2015
Response via : Initial Calibration

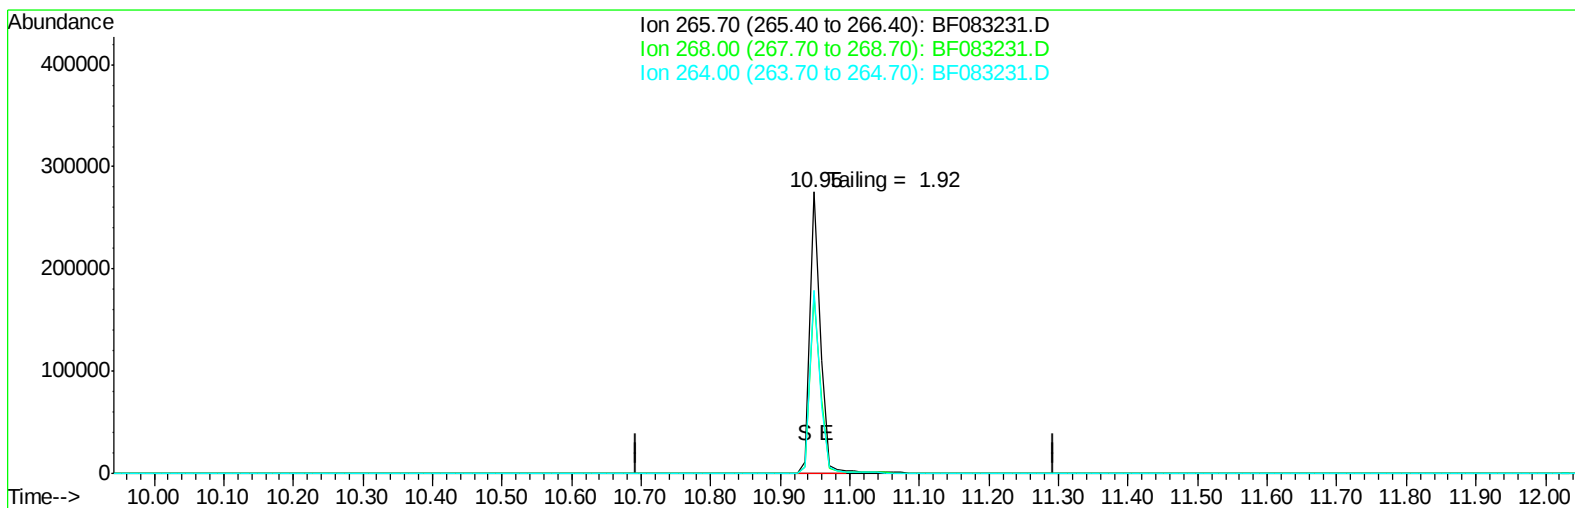

TIC: BF083231.D

(69) Pentachlorophenol (C)




10.948min (-0.046) 26708.10ng m

response 281677

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	63.14
264.00	64.60	64.97
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF112415\
Data File : BF083231.D
Acq On : 24 Nov 2015 10:56
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 24 11:29:21 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF112115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 09:22:46 2015
Response via : Initial Calibration

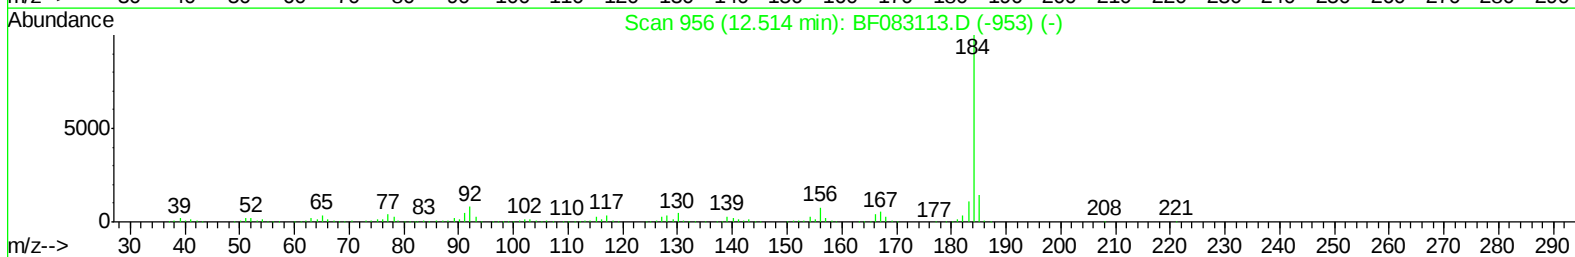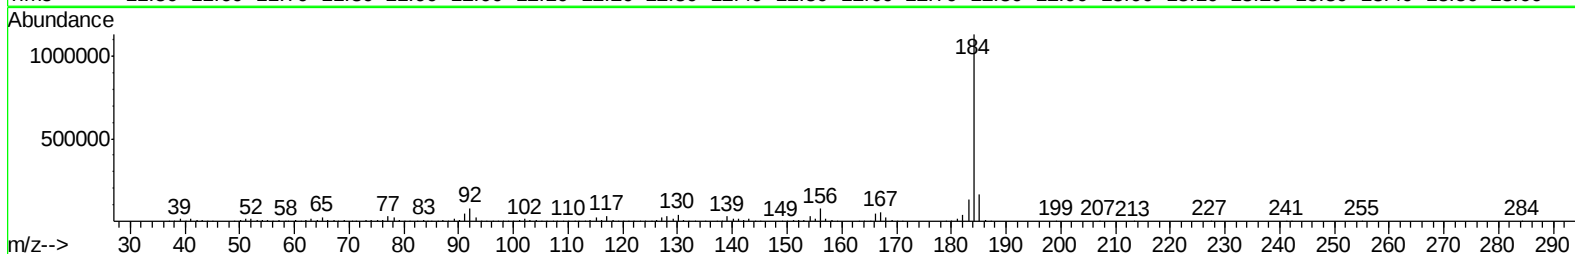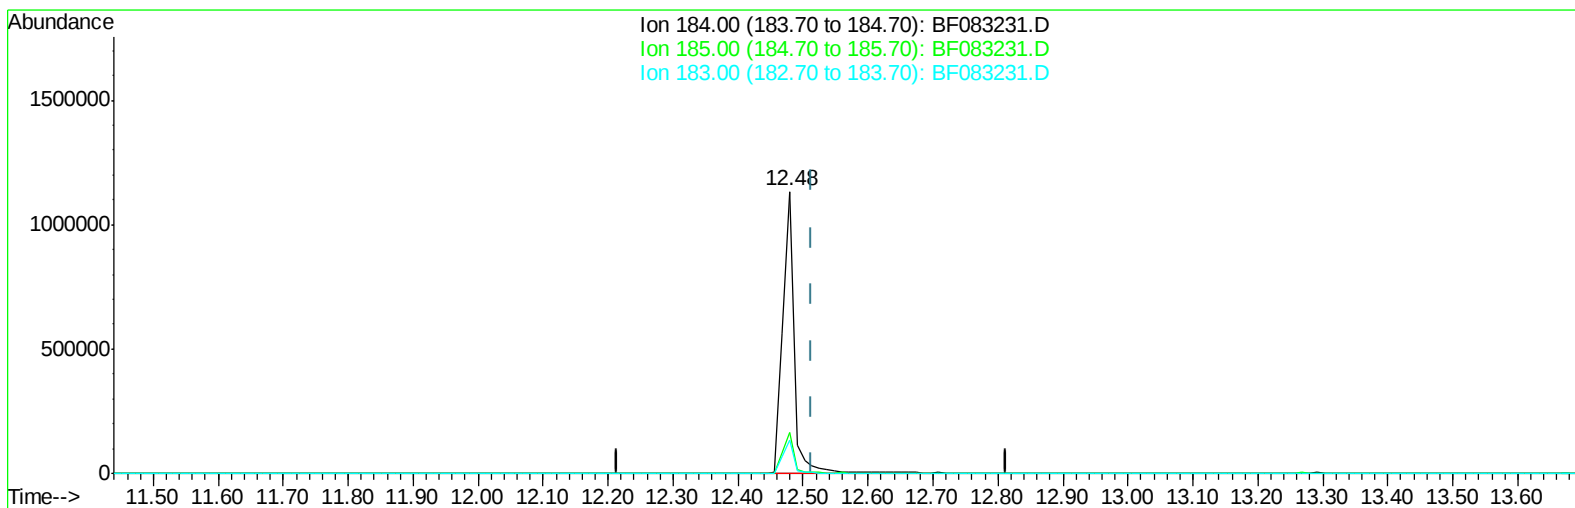

TIC: BF083231.D

(76) Benzidine

12.479min (-0.034) 0.00ng

response 1365927

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	14.50
183.00	11.00	11.75
0.00	0.00	0.00