


Data Path : Z:\HPCHEM1\BNA_F\Data\BF112415\
 Data File : BF083231.D
 Acq On : 24 Nov 2015 10:56
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF112115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Nov 22 09:22:46 2015

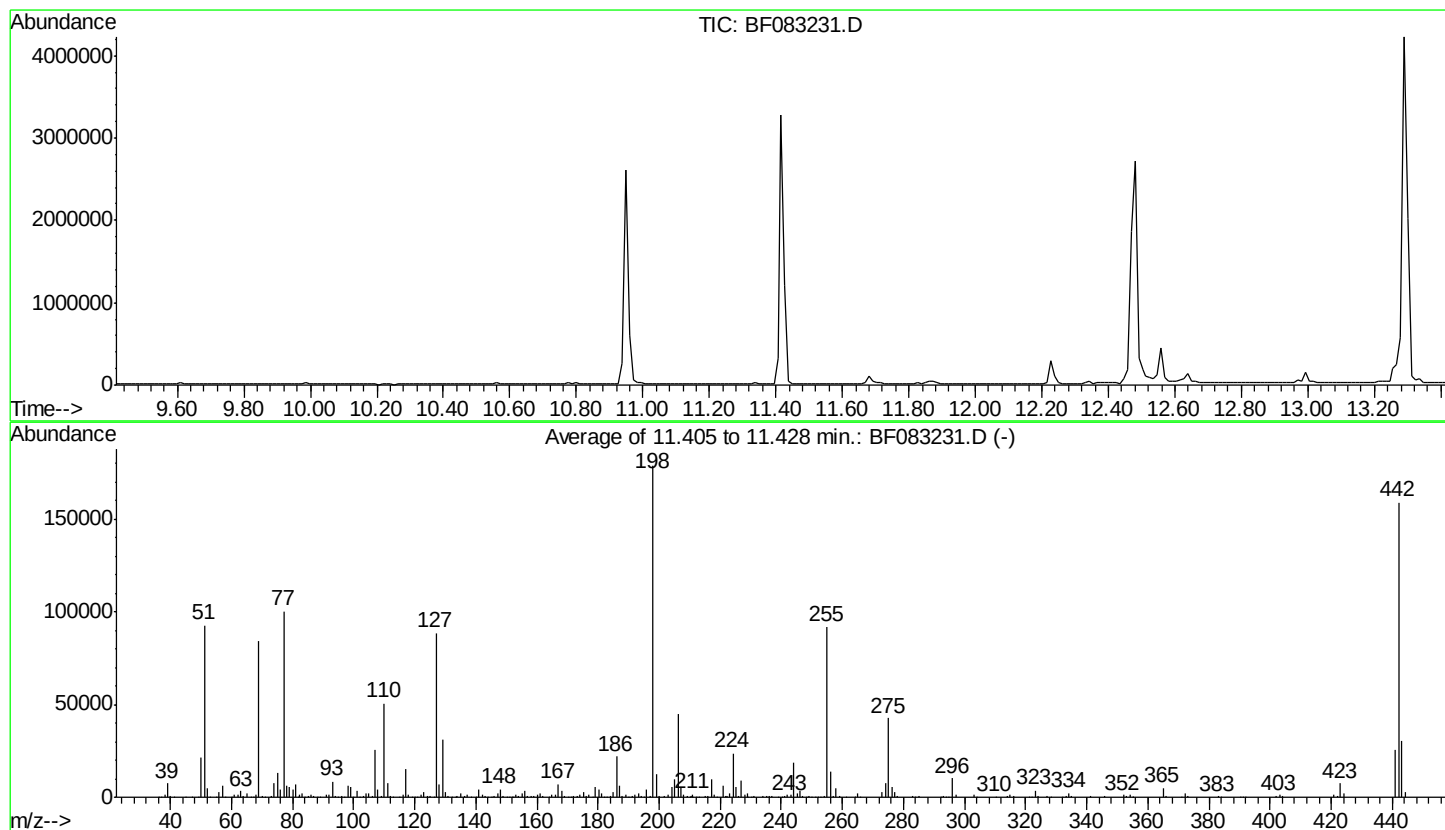

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 821

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.8	92467	PASS
68	69	0.00	2	1.6	1321	PASS
69	198	0.00	100	47.1	84195	PASS
70	69	0.00	2	0.5	447	PASS
127	198	10	80	49.5	88472	PASS
197	198	0.00	2	0.6	1014	PASS
198	198	100	100	100.0	178648	PASS
199	198	5	9	6.9	12347	PASS
275	198	10	60	23.8	42454	PASS
365	198	1	100	2.7	4847	PASS
441	442	0.01	24	16.0	25357	PASS
442	198	50	100	88.9	158875	PASS
443	442	15	24	19.2	30441	PASS