


Data Path : Z:\HPCHEM1\BNA\_F\Data\BF112415\  
Data File : BF083241.D  
Acq On : 24 Nov 2015 17:17  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF112115.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Sun Nov 22 09:22:46 2015

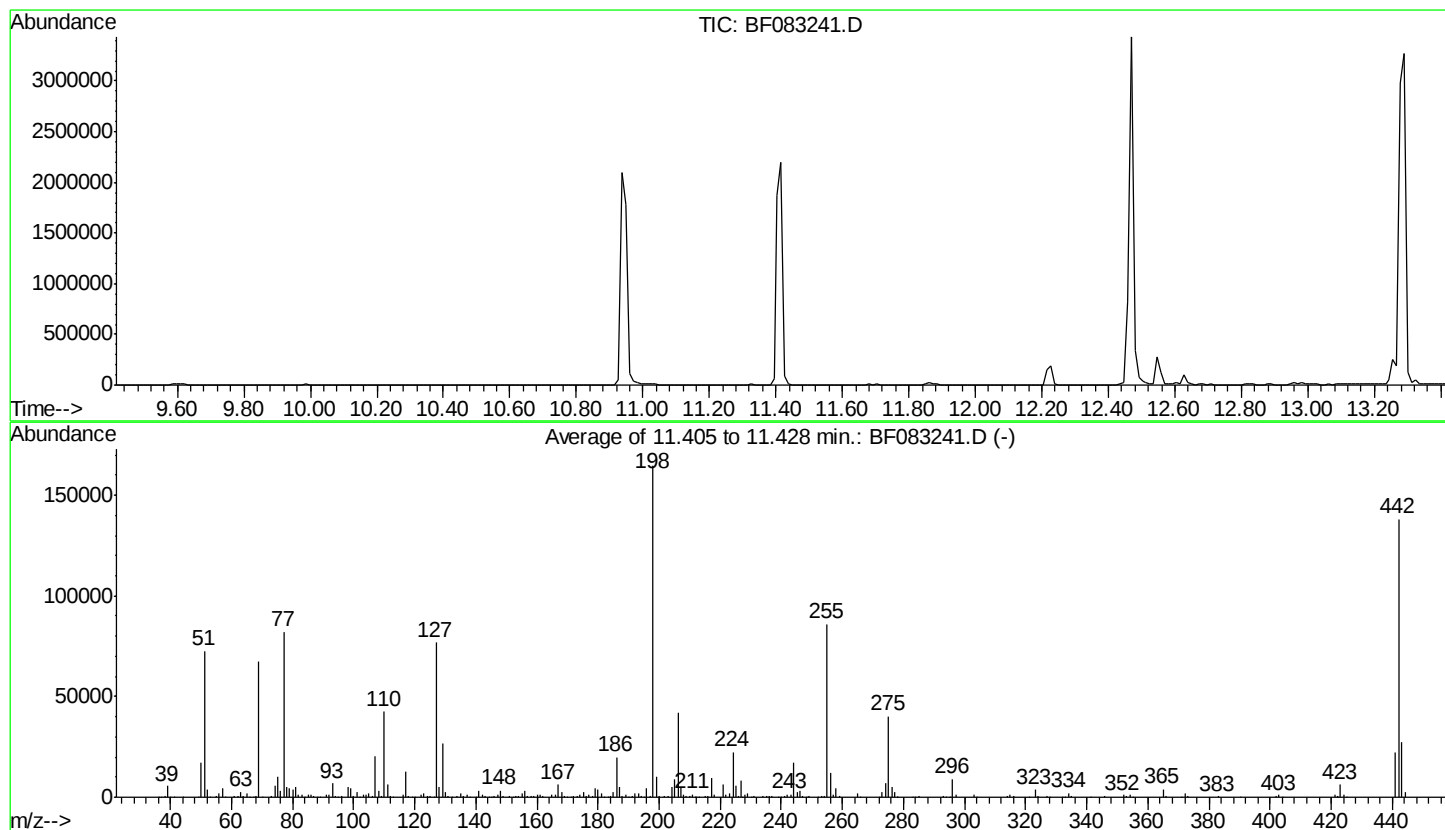

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 820

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 44.1      | 72663   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.4       | 965     | PASS             |
| 69          | 198          | 0.00         | 100          | 41.0      | 67447   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 343     | PASS             |
| 127         | 198          | 10           | 80           | 46.6      | 76714   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.3       | 425     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 164679  | PASS             |
| 199         | 198          | 5            | 9            | 6.3       | 10332   | PASS             |
| 275         | 198          | 10           | 60           | 24.4      | 40147   | PASS             |
| 365         | 198          | 1            | 100          | 2.5       | 4087    | PASS             |
| 441         | 442          | 0.01         | 24           | 15.9      | 22004   | PASS             |
| 442         | 198          | 50           | 100          | 83.8      | 138013  | PASS             |
| 443         | 442          | 15           | 24           | 19.8      | 27314   | PASS             |