

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112515\
 Data File : BF083286.D
 Acq On : 25 Nov 2015 21:20
 Operator : UM/IZ
 Sample : G4567-02 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 STOCKPILE-COMPOSITE2

Quant Time: Nov 26 01:16:42 2015
 Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF112115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Nov 22 09:22:46 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	155834	20.00	ng	0.08
21) Naphthalene-d8	7.87	136	592943	20.00	ng	-0.08
38) Acenaphthene-d10	9.62	164	279467	20.00	ng	-0.08
63) Phenanthrene-d10	11.10	188	420627	20.00	ng	-0.08
75) Chrysene-d12	13.73	240	370779	20.00	ng	-0.08
86) Perylene-d12	15.09	264	425841	20.00	ng	-0.08

System Monitoring Compounds						
5) 2-Fluorophenol	5.18	112	326242	31.65	ng	-0.10
7) Phenol-d6	6.25	99	462259	34.66	ng	-0.09
23) Nitrobenzene-d5	7.15	82	289773	22.33	ng	-0.08
41) 2,4,6-Tribromophenol	10.41	330	74468	26.05	ng	-0.08
44) 2-Fluorobiphenyl	8.96	172	423566	21.13	ng	-0.07
78) Terphenyl-d14	12.68	244	289342	18.38	ng	-0.08

Target Compounds				Qvalue		
9) Benzaldehyde	6.26	77	1890	Below Cal	#	1
18) Hexachloroethane	7.27	117	15524	3.43	ng	# 1
19) n-Nitroso-di-n-propylamine	7.15	70	44668	4.81	ng	# 76
31) Naphthalene	7.90	128	459100	14.35	ng	# 100
33) 4-Chloroaniline	7.90	127	62284	5.02	ng	# 28
37) 2-Methylnaphthalene	8.59	142	183398	8.83	ng	96
48) Acenaphthylene	9.48	152	795854	27.49	ng	99
49) Dimethylphthalate	9.36	163	98052	4.56	ng	99
51) Acenaphthene	9.66	154	148311	8.42	ng	97
57) Fluorene	10.17	166	122943	5.97	ng	# 85
65) n-Nitrosodiphenylamine	10.54	169	93177	6.51	ng	86
70) Phenanthrene	11.18	178	450417	18.59	ng	97
71) Anthracene	11.18	178	450417	18.22	ng	98
74) Fluoranthene	12.31	202	1541415	62.15	ng	96
77) Pyrene	12.54	202	2856659	112.77	ng	98
80) Benzo(a)anthracene	13.76	228	1087673	47.43	ng	93
82) Chrysene	13.76	228	1087673	51.15	ng	97
85) Indeno(1,2,3-cd)pyrene	16.31	276	419438	21.68	ng	98
87) Benzo(b)fluoranthene	14.72	252	1184424	40.71	ng	# 92
88) Benzo(k)fluoranthene	14.72	252	1184424	54.64	ng	# 94
89) Benzo(a)pyrene	15.03	252	1052350	43.81	ng	# 92
90) Dibenzo(a,h)anthracene	16.50	278	134334	6.16	ng	92
91) Benzo(g,h,i)perylene	16.67	276	432321	20.29	ng	# 93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112515\  
Data File : BF083286.D  
Acq On    : 25 Nov 2015   21:20  
Operator  : UM/IZ  
Sample    : G4567-02 5X  
Misc      :  
ALS Vial  : 13      Sample Multiplier: 1
```



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.74 min Scan# 416

Delta R.T. 0.08 min

Lab File: BF083286.D

Acq: 25 Nov 2015 21:20

Instrument :

BNA_F

ClientSampleId :

STOCKPILE-COMPOSITE2


Tgt Ion:152 Resp: 155834

Ion Ratio Lower Upper

152 100

150 152.9 125.8 188.8




115 67.5 46.9 70.3



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E



#5

2-Fluorophenol

Concen: 31.65 ng

RT: 5.18 min Scan# 279

Delta R.T. -0.10 min

Lab File: BF083286.D

Acq: 25 Nov 2015 21:20


Tgt Ion:112 Resp: 326242

Ion Ratio Lower Upper

112 100

64 62.8 58.4 87.6



63 30.2 30.0 45.0




Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0



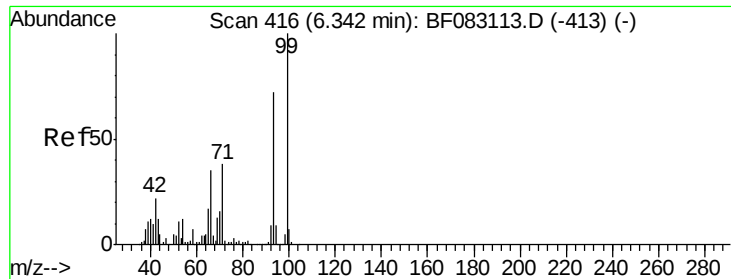

#7

Phenol-d6

Concen: 34.66 ng

RT: 6.25 min Scan# 373

Delta R.T. -0.09 min

Lab File: BF083286.D

Acq: 25 Nov 2015 21:20

Instrument :

BNA_F

ClientSampleId :

STOCKPILE-COMPOSITE2


Tgt Ion: 99 Resp: 462259

Ion Ratio Lower Upper

99 100

42 18.6 17.7 26.5




71 30.9 30.2 45.4



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0



#18

Hexachloroethane

Concen: 3.43 ng

RT: 7.27 min Scan# 462

Delta R.T. 0.09 min

Lab File: BF083286.D

Acq: 25 Nov 2015 21:20


Tgt Ion: 117 Resp: 15524

Ion Ratio Lower Upper

117 100

119 0.0 76.8 115.2#



201 0.0 88.6 133.0#






Abundance Ion 117.00 (116.70 to 117.70): E

Ion 119.00 (118.70 to 119.70): E

Ion 201.00 (200.70 to 201.70): E









#19
n-Nitroso-di-n-propylamine
Concen: 4.81 ng
RT: 7.15 min Scan# 452
Delta R.T. 0.05 min
Lab File: BF083286.D
Acq: 25 Nov 2015 21:20


Instrument :
BNA_F
ClientSampleId :
STOCKPILE-COMPOSITE2


Tgt Ion: 70 Resp: 44668
Ion Ratio Lower Upper
70 100
42 50.5 54.5 81.7#
101 0.0 6.6 9.8#
130 1.4 11.5 17.3#



#21
Naphthalene-d8
Concen: 20.00 ng
RT: 7.87 min Scan# 515
Delta R.T. -0.08 min
Lab File: BF083286.D
Acq: 25 Nov 2015 21:20

Tgt Ion: 136 Resp: 592943
Ion Ratio Lower Upper
136 100
137 11.4 8.7 13.1
54 12.2 5.8 8.6#
68 8.5 3.8 5.8#





#23

Nitrobenzene-d5

Concen: 22.33 ng

RT: 7.15 min Scan# 452

Delta R.T. -0.08 min

Lab File: BF083286.D

Acq: 25 Nov 2015 21:20

Instrument :

BNA_F

ClientSampleId :

STOCKPILE-COMPOSITE2


Tgt Ion: 82 Resp: 289773

Ion Ratio Lower Upper

82 100

128 35.3 28.5 42.7




54 55.8 44.6 67.0



Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0



#31

Naphthalene

Concen: 14.35 ng

RT: 7.90 min Scan# 517

Delta R.T. -0.08 min

Lab File: BF083286.D

Acq: 25 Nov 2015 21:20


Tgt Ion: 128 Resp: 459100

Ion Ratio Lower Upper

128 100

129 11.2 9.0 13.4



127 13.2 10.6 15.8




Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E









#33
4-Chloroaniline
Concen: 5.02 ng
RT: 7.90 min Scan# 517
Delta R.T. -0.14 min
Lab File: BF083286.D
Acq: 25 Nov 2015 21:20




Instrument :
BNA_F
ClientSampleId :
STOCKPILE-COMPOSITE2


Tgt Ion:127 Resp: 62284
Ion Ratio Lower Upper
127 100
129 85.1 25.7 38.5#
65 0.0 35.5 53.3#
92 0.0 19.4 29.2#



#37
2-Methylnaphthalene
Concen: 8.83 ng
RT: 8.59 min Scan# 578
Delta R.T. -0.07 min
Lab File: BF083286.D
Acq: 25 Nov 2015 21:20

Tgt Ion:142 Resp: 183398
Ion Ratio Lower Upper
142 100
141 87.6 70.3 105.5
115 35.0 33.4 50.2









#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.62 min Scan# 668
 Delta R.T. -0.08 min
 Lab File: BF083286.D
 Acq: 25 Nov 2015 21:20

Instrument :
 BNA_F
 ClientSampleId :
 STOCKPILE-COMPOSITE2

Tgt Ion:164 Resp: 279467
 Ion Ratio Lower Upper
 164 100
 162 100.4 81.2 121.8
 160 43.1 35.6 53.4




Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E






#41
 2,4,6-Tribromophenol
 Concen: 26.05 ng
 RT: 10.41 min Scan# 737
 Delta R.T. -0.08 min
 Lab File: BF083286.D
 Acq: 25 Nov 2015 21:20

Tgt Ion:330 Resp: 74468
 Ion Ratio Lower Upper
 330 100
 332 96.4 77.7 116.5
 141 45.2 29.7 44.5#



Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E









#44
2-Fluorobiphenyl
Concen: 21.13 ng
RT: 8.96 min Scan# 610
Delta R.T. -0.07 min
Lab File: BF083286.D
Acq: 25 Nov 2015 21:20




Instrument :
BNA_F
ClientSampleId :
STOCKPILE-COMPOSITE2


Tgt Ion:172 Resp: 423566
Ion Ratio Lower Upper
172 100
171 33.7 29.5 44.3
170 22.9 19.9 29.9



#48
Acenaphthylene
Concen: 27.49 ng
RT: 9.48 min Scan# 656
Delta R.T. -0.08 min
Lab File: BF083286.D
Acq: 25 Nov 2015 21:20

Tgt Ion:152 Resp: 795854
Ion Ratio Lower Upper
152 100
151 20.4 16.3 24.5
153 14.0 10.8 16.2









#49
Dimethylphthalate
Concen: 4.56 ng
RT: 9.36 min Scan# 645
Delta R.T. -0.09 min
Lab File: BF083286.D
Acq: 25 Nov 2015 21:20




Instrument :
BNA_F
ClientSampleId :
STOCKPILE-COMPOSITE2


Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.5	2.6	4.0
164	10.2	8.6	12.8



#51
Acenaphthene
Concen: 8.42 ng
RT: 9.66 min Scan# 671
Delta R.T. -0.08 min
Lab File: BF083286.D
Acq: 25 Nov 2015 21:20

Tgt Ion	Ratio	Lower	Upper
154	100		
153	114.8	89.6	134.4
152	56.7	43.3	64.9









#57
Fluorene
 Concen: 5.97 ng
 RT: 10.17 min Scan# 716
 Delta R.T. -0.07 min
 Lab File: BF083286.D
 Acq: 25 Nov 2015 21:20




Instrument :
 BNA_F
 ClientSampleId :
 STOCKPILE-COMPOSITE2


Tgt Ion	Resp	Lower	Upper
166	100		
165	112.6	78.0	117.0
167	18.8	11.3	16.9#



#63
Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.10 min Scan# 797
 Delta R.T. -0.08 min
 Lab File: BF083286.D
 Acq: 25 Nov 2015 21:20

Tgt Ion	Resp	Lower	Upper
188	100		
94	14.0	6.0	9.0#
80	16.6	6.7	10.1#









#65
n-Nitrosodiphenylamine
Concen: 6.51 ng
RT: 10.54 min Scan# 748
Delta R.T. 0.17 min
Lab File: BF083286.D
Acq: 25 Nov 2015 21:20




Instrument :
BNA_F
ClientSampleId :
STOCKPILE-COMPOSITE2


Tgt Ion:169 Resp: 93177
Ion Ratio Lower Upper
169 100
168 55.0 53.8 80.6
167 43.9 29.8 44.8



#70
Phenanthrene
Concen: 18.59 ng
RT: 11.18 min Scan# 804
Delta R.T. -0.02 min
Lab File: BF083286.D
Acq: 25 Nov 2015 21:20

Tgt Ion:178 Resp: 450417
Ion Ratio Lower Upper
178 100
176 18.9 16.2 24.2
179 17.6 12.8 19.2









#71
 Anthracene
 Concen: 18.22 ng
 RT: 11.18 min Scan# 804
 Delta R.T. -0.07 min
 Lab File: BF083286.D
 Acq: 25 Nov 2015 21:20




Instrument :
 BNA_F
 ClientSampleId :
 STOCKPILE-COMPOSITE2


Tgt Ion:178 Resp: 450417
 Ion Ratio Lower Upper
 178 100
 176 18.9 15.6 23.4
 179 17.6 13.2 19.8



#74
 Fluoranthene
 Concen: 62.15 ng
 RT: 12.31 min Scan# 903
 Delta R.T. -0.07 min
 Lab File: BF083286.D
 Acq: 25 Nov 2015 21:20

Tgt Ion:202 Resp: 1541415
 Ion Ratio Lower Upper
 202 100
 101 15.2 0.0 32.3
 203 19.0 0.0 38.4





#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.73 min Scan# 1027

Delta R.T. -0.08 min

Lab File: BF083286.D

Acq: 25 Nov 2015 21:20

Instrument :

BNA_F

ClientSampleId :

STOCKPILE-COMPOSITE2


Tgt Ion:240 Resp: 370779

Ion Ratio Lower Upper

240 100

120 16.0 5.4 8.2#




236 25.8 20.6 31.0



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E



#77

Pyrene

Concen: 112.77 ng

RT: 12.54 min Scan# 923

Delta R.T. -0.07 min

Lab File: BF083286.D

Acq: 25 Nov 2015 21:20


Tgt Ion:202 Resp: 2856659

Ion Ratio Lower Upper

202 100

200 22.8 17.8 26.6



203 20.3 15.0 22.4




Abundance Ion 202.00 (201.70 to 202.70): E

Ion 200.00 (199.70 to 200.70): E

Ion 203.00 (202.70 to 203.70): E





#78

Terphenyl-d14

Concen: 18.38 ng

RT: 12.68 min Scan# 936

Delta R.T. -0.08 min

Lab File: BF083286.D

Acq: 25 Nov 2015 21:20

Instrument :

BNA_F

ClientSampleId :

STOCKPILE-COMPOSITE2


Tgt Ion:244 Resp: 289342

Ion Ratio Lower Upper

244 100

212 7.5 5.4 8.2




122 11.0 4.3 6.5#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E



#80

Benzo(a)anthracene

Concen: 47.43 ng

RT: 13.76 min Scan# 1030

Delta R.T. -0.03 min

Lab File: BF083286.D

Acq: 25 Nov 2015 21:20


Tgt Ion:228 Resp: 1087673

Ion Ratio Lower Upper

228 100

226 32.4 22.6 33.8



229 23.8 16.6 24.8




Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E





#82

Chrysene

Concen: 51.15 ng

RT: 13.76 min Scan# 1030

Delta R.T. -0.07 min

Lab File: BF083286.D

Acq: 25 Nov 2015 21:20

Instrument :

BNA_F

ClientSampleId :

STOCKPILE-COMPOSITE2


Tgt Ion:228 Resp: 1087673

Ion Ratio Lower Upper

228 100

226 32.4 25.5 38.3




229 23.8 16.6 25.0



Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E



#85

Indeno(1,2,3-cd)pyrene

Concen: 21.68 ng

RT: 16.31 min Scan# 1253

Delta R.T. -0.14 min

Lab File: BF083286.D

Acq: 25 Nov 2015 21:20


Tgt Ion:276 Resp: 419438

Ion Ratio Lower Upper

276 100

138 24.0 18.0 27.0



277 25.6 20.2 30.4




Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E









#86
Perylene-d12
Concen: 20.00 ng
RT: 15.09 min Scan# 1146
Delta R.T. -0.08 min
Lab File: BF083286.D
Acq: 25 Nov 2015 21:20




Instrument :
BNA_F
ClientSampleId :
STOCKPILE-COMPOSITE2


Tgt Ion:264 Resp: 425841
Ion Ratio Lower Upper
264 100
260 24.3 19.1 28.7
265 26.9 18.2 27.4



#87
Benzo(b)fluoranthene
Concen: 40.71 ng
RT: 14.72 min Scan# 1114
Delta R.T. -0.08 min
Lab File: BF083286.D
Acq: 25 Nov 2015 21:20

Tgt Ion:252 Resp: 1184424
Ion Ratio Lower Upper
252 100
253 24.1 17.7 26.5
125 13.7 5.6 8.4#









#88
Benzo(k)fluoranthene
Concen: 54.64 ng
RT: 14.72 min Scan# 1114
Delta R.T. -0.10 min
Lab File: BF083286.D
Acq: 25 Nov 2015 21:20




Instrument :
BNA_F
ClientSampleId :
STOCKPILE-COMPOSITE2


Tgt Ion:252 Resp: 1184424
Ion Ratio Lower Upper
252 100
253 24.1 18.2 27.2
125 13.7 6.8 10.2#



#89
Benzo(a)pyrene
Concen: 43.81 ng
RT: 15.03 min Scan# 1141
Delta R.T. -0.09 min
Lab File: BF083286.D
Acq: 25 Nov 2015 21:20

Tgt Ion:252 Resp: 1052350
Ion Ratio Lower Upper
252 100
253 23.6 17.5 26.3
125 13.7 5.4 8.0#





#90

Dibenzo(a,h)anthracene

Concen: 6.16 ng

RT: 16.50 min Scan# 1270

Delta R.T. 0.05 min

Lab File: BF083286.D

Acq: 25 Nov 2015 21:20

Instrument :

BNA_F

ClientSampleId :

STOCKPILE-COMPOSITE2


Tgt Ion:278 Resp: 134334

Ion Ratio Lower Upper

278 100

139 16.1 10.7 16.1




279 28.3 19.3 28.9



Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E



#91

Benzo(g,h,i)perylene

Concen: 20.29 ng

RT: 16.67 min Scan# 1285

Delta R.T. -0.15 min

Lab File: BF083286.D

Acq: 25 Nov 2015 21:20


Tgt Ion:276 Resp: 432321

Ion Ratio Lower Upper

276 100

277 24.2 18.7 28.1

138 23.8 13.9 20.9#



Abundance Ion 276.00 (275.70 to 276.70): E

Ion 277.00 (276.70 to 277.70): E

Ion 138.00 (137.70 to 138.70): E

