
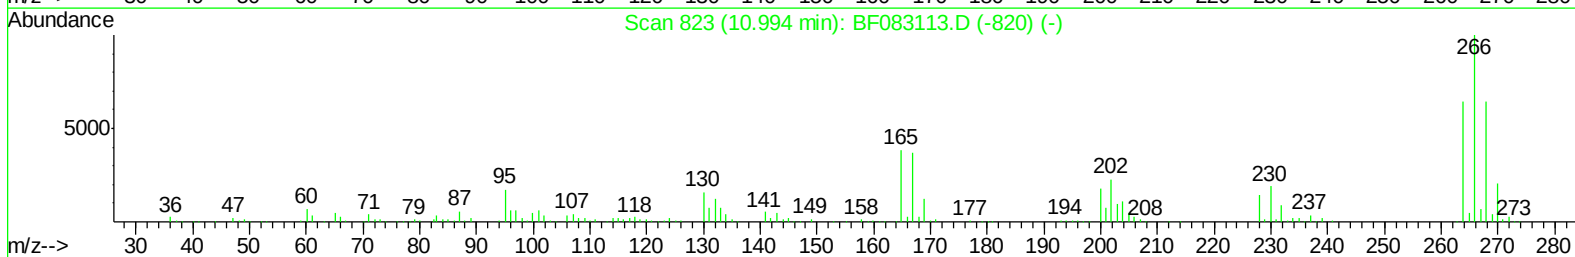
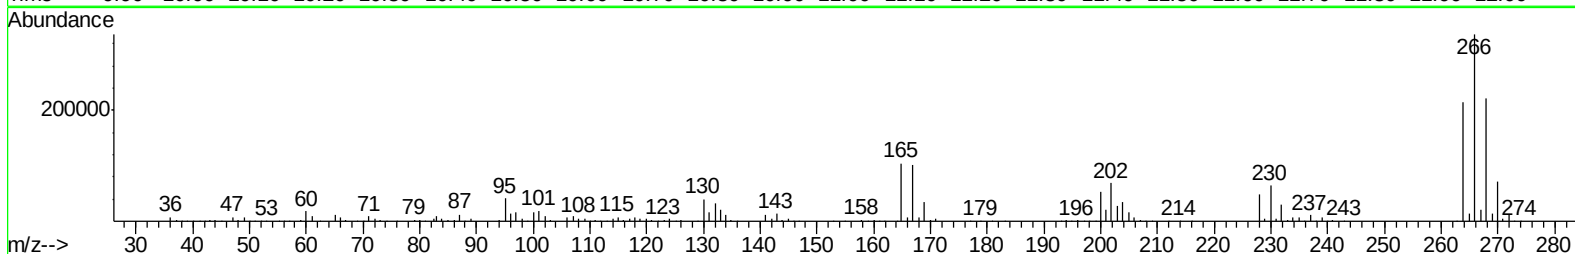


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112515\
Data File : BF083267.D
Acq On : 25 Nov 2015 11:57
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 07:02:06 2015
Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF112115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 09:22:46 2015
Response via : Initial Calibration

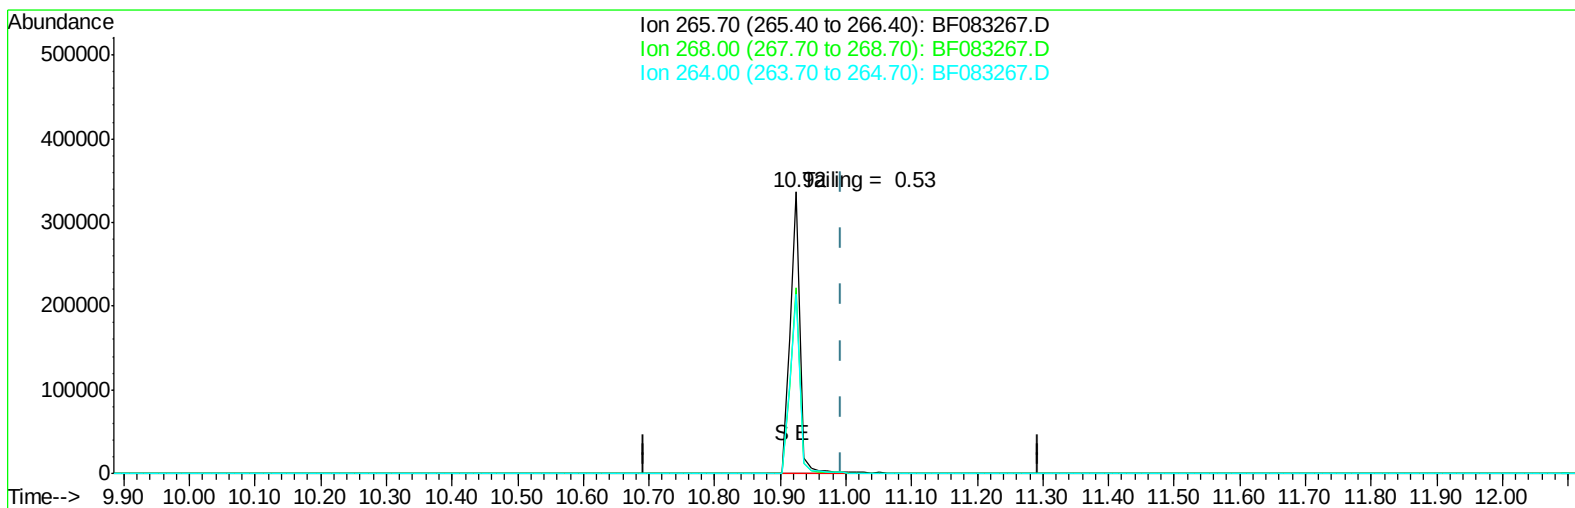

TIC: BF083267.D

(69) Pentachlorophenol (C)




10.925min (-0.069) 6446.16ng

response 371426

Ion	Exp%	Act%
265.70	100	100
268.00	64.20	66.10
264.00	64.60	63.46
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF112515\
Data File : BF083267.D
Acq On : 25 Nov 2015 11:57
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 07:02:06 2015
Quant Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF112115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Nov 22 09:22:46 2015
Response via : Initial Calibration

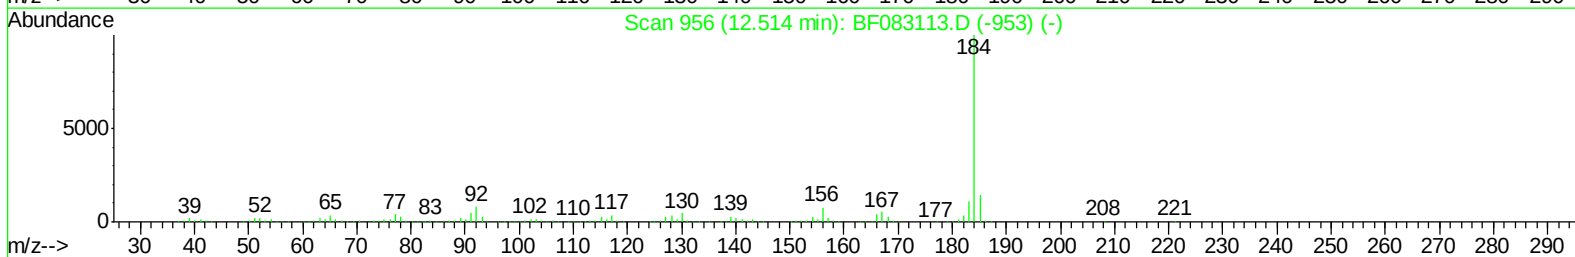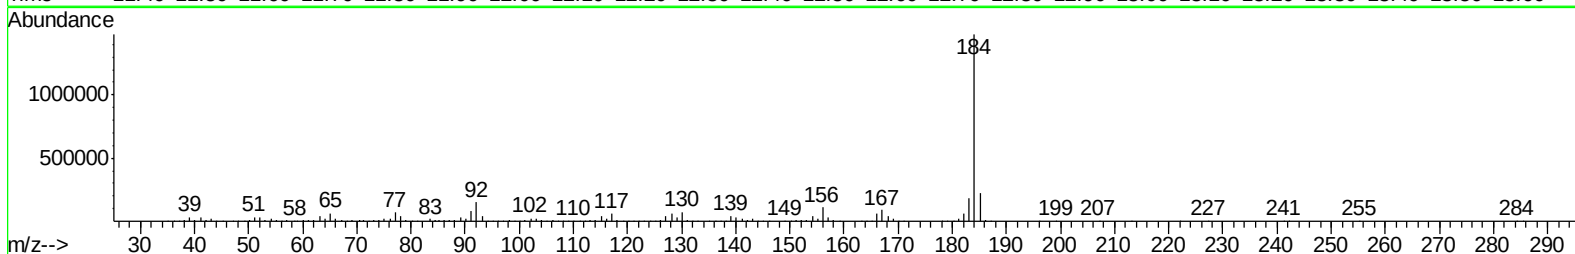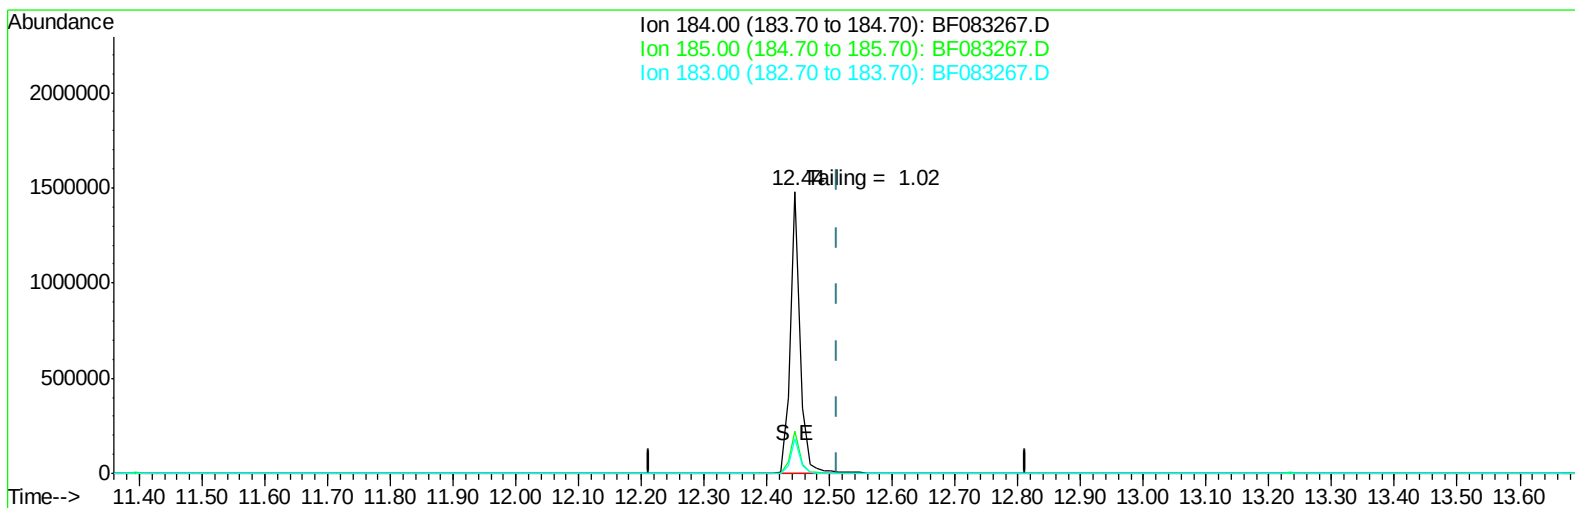

TIC: BF083267.D

(76) Benzidine

12.445min (-0.069) 2125.49ng

response 1636424

Ion	Exp%	Act%
184.00	100	100
185.00	14.60	15.07
183.00	11.00	12.07
0.00	0.00	0.00