


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF112515\  
Data File : BF083267.D  
Acq On : 25 Nov 2015 11:57  
Operator : UM/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\Methods\8270-BF112115.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Sun Nov 22 09:22:46 2015

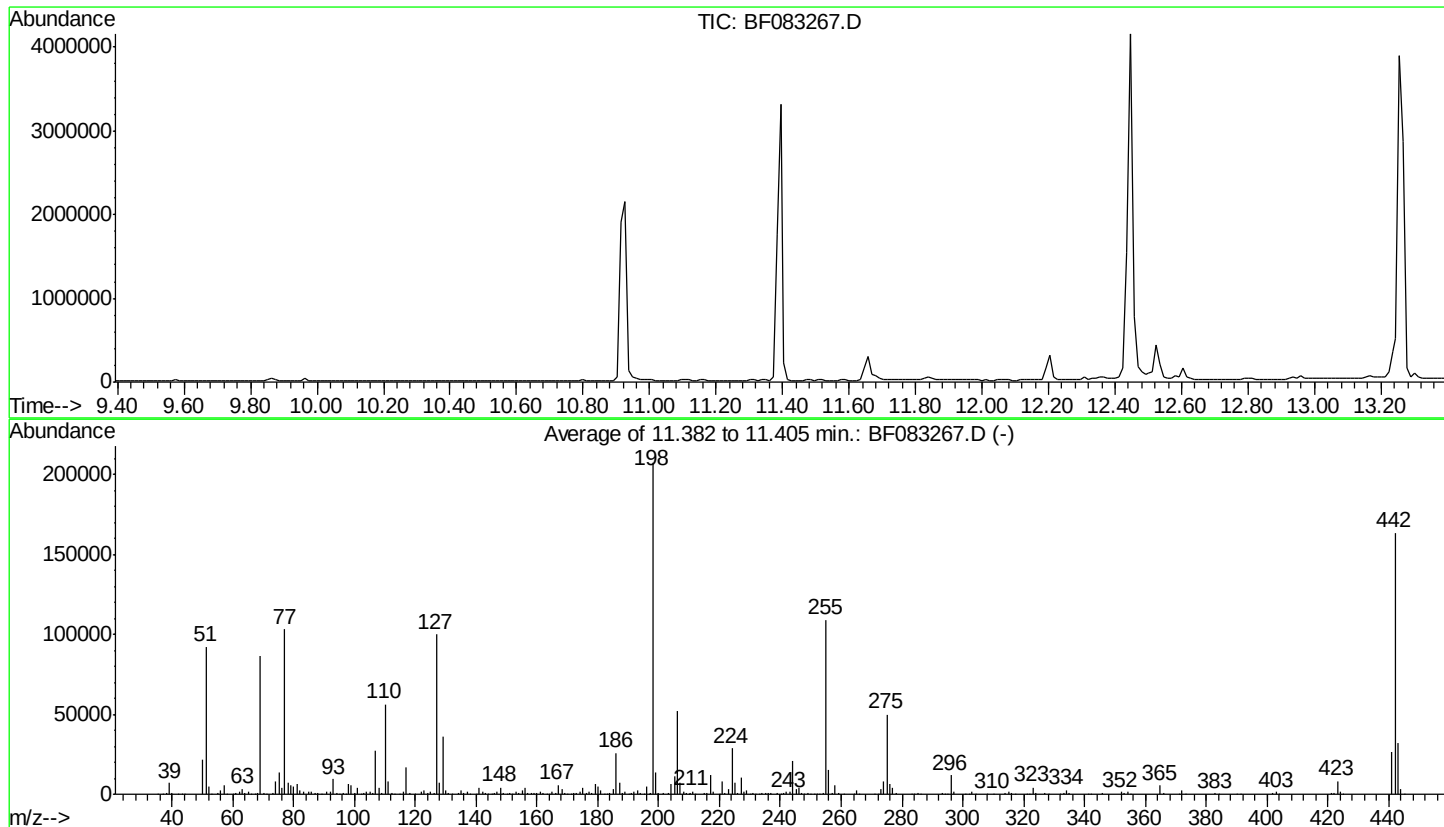

AutoFind: Scans 822, 823, 824; Background Corrected with Scan 818

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 44.6      | 92563   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.3       | 1150    | PASS             |
| 69          | 198          | 0.00         | 100          | 41.7      | 86562   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 527     | PASS             |
| 127         | 198          | 10           | 80           | 48.1      | 99926   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.4       | 829     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 207549  | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 13631   | PASS             |
| 275         | 198          | 10           | 60           | 24.1      | 50100   | PASS             |
| 365         | 198          | 1            | 100          | 2.5       | 5269    | PASS             |
| 441         | 442          | 0.01         | 24           | 16.0      | 26246   | PASS             |
| 442         | 198          | 50           | 100          | 78.9      | 163674  | PASS             |
| 443         | 442          | 15           | 24           | 19.4      | 31774   | PASS             |