


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF112515\  
 Data File : BF083274.D  
 Acq On : 25 Nov 2015 15:27  
 Operator : UM/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\Methods\8270-BF112115.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Sun Nov 22 09:22:46 2015

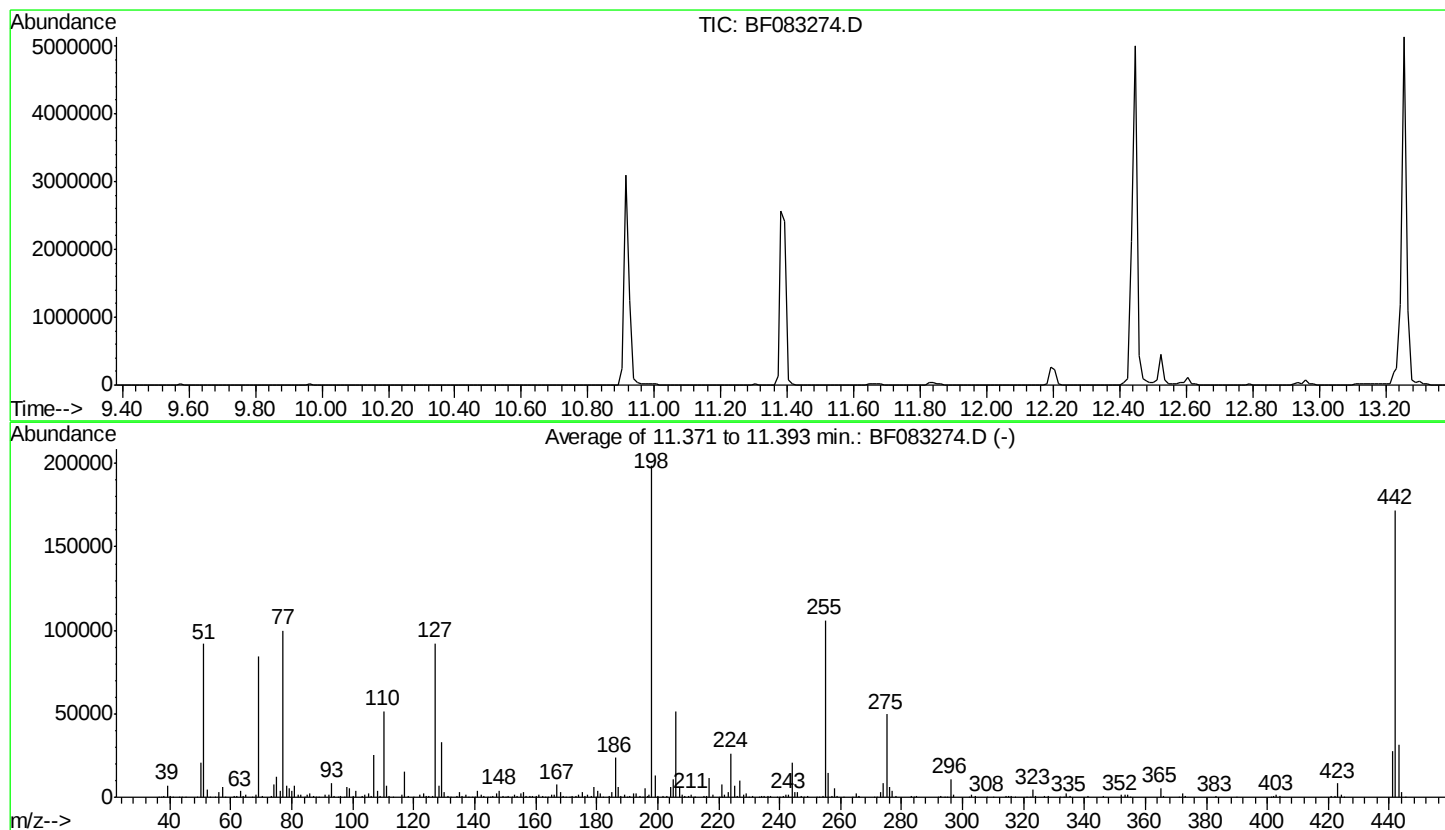

AutoFind: Scans 821, 822, 823; Background Corrected with Scan 818

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 46.2         | 91784      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.6          | 1316       | PASS                |
| 69             | 198             | 0.00            | 100             | 42.5         | 84448      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 410        | PASS                |
| 127            | 198             | 10              | 80              | 46.4         | 92281      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.6          | 1210       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 198693     | PASS                |
| 199            | 198             | 5               | 9               | 6.7          | 13227      | PASS                |
| 275            | 198             | 10              | 60              | 25.0         | 49665      | PASS                |
| 365            | 198             | 1               | 100             | 2.7          | 5445       | PASS                |
| 441            | 442             | 0.01            | 24              | 15.9         | 27344      | PASS                |
| 442            | 198             | 50              | 100             | 86.5         | 171952     | PASS                |
| 443            | 442             | 15              | 24              | 18.2         | 31228      | PASS                |