


Data Path : Z:\HPCHEM1\BNA F\Data\BF112515\
 Data File : BF083299.D
 Acq On : 26 Nov 2015 4:26
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\Methods\8270-BF112115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sun Nov 22 09:22:46 2015

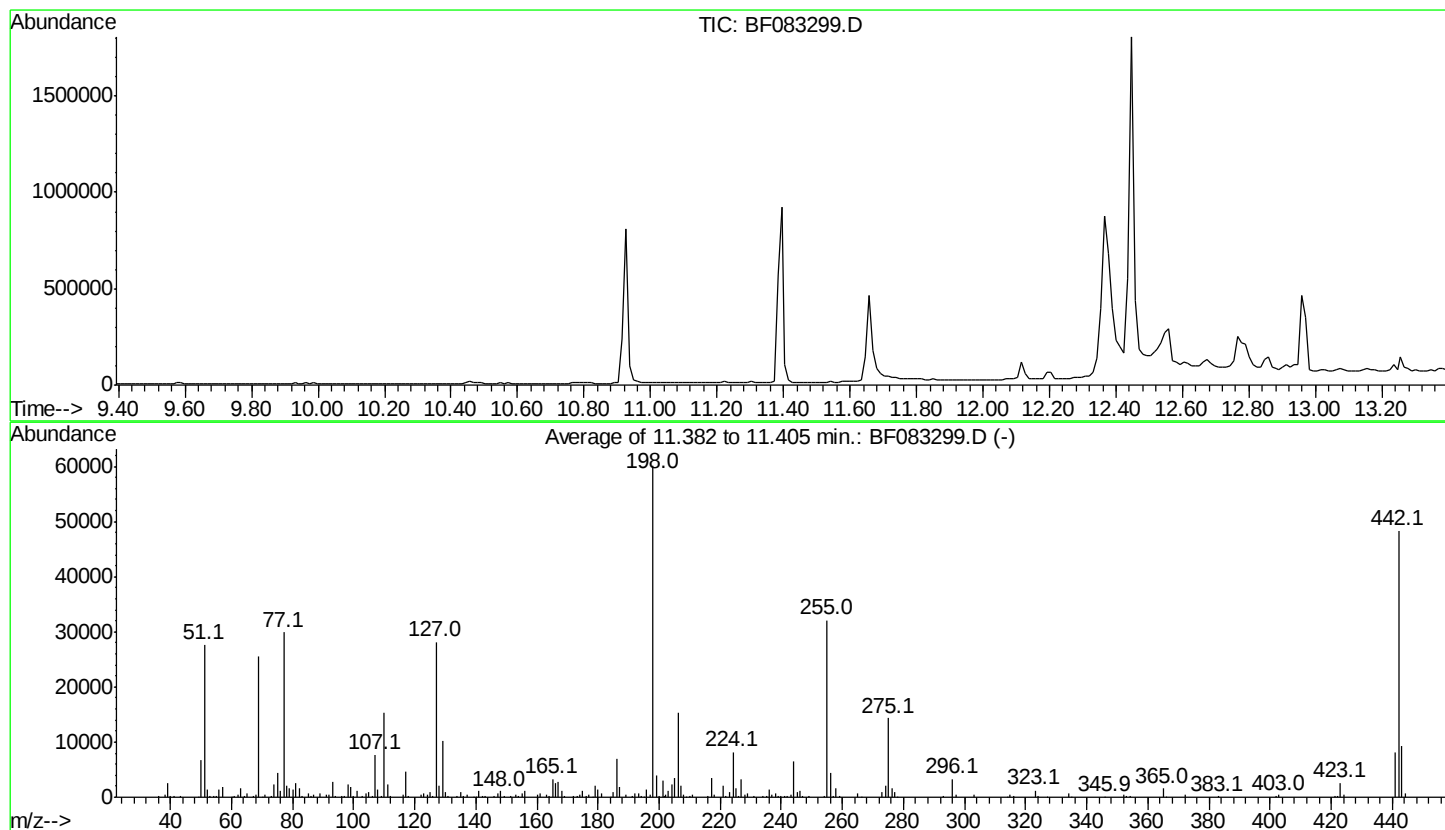

AutoFind: Scans 822, 823, 824; Background Corrected with Scan 818

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	27748	PASS
68	69	0.00	2	2.0	499	PASS
69	198	0.00	100	42.3	25444	PASS
70	69	0.00	2	0.4	102	PASS
127	198	10	80	46.9	28182	PASS
197	198	0.00	2	0.6	377	PASS
198	198	100	100	100.0	60139	PASS
199	198	5	9	6.7	4012	PASS
275	198	10	60	23.8	14305	PASS
365	198	1	100	2.6	1562	PASS
441	442	0.01	24	17.0	8213	PASS
442	198	50	100	80.3	48320	PASS
443	442	15	24	19.3	9330	PASS