
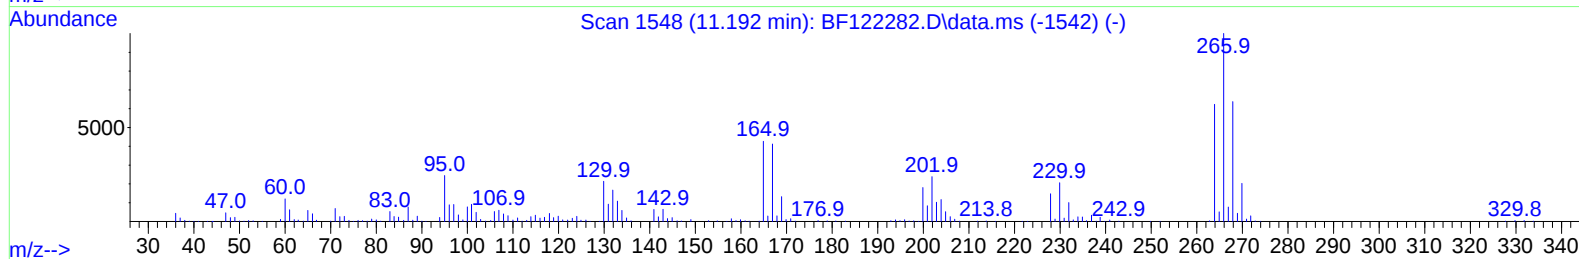
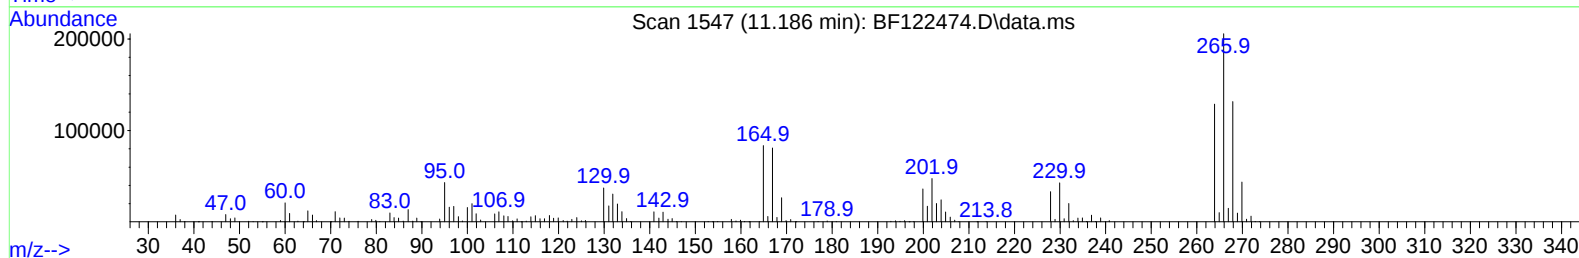


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112520\
Data File : BF122474.D
Acq On : 25 Nov 2020 9:04
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 01:56:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 14:38:56 2020
Response via : Initial Calibration

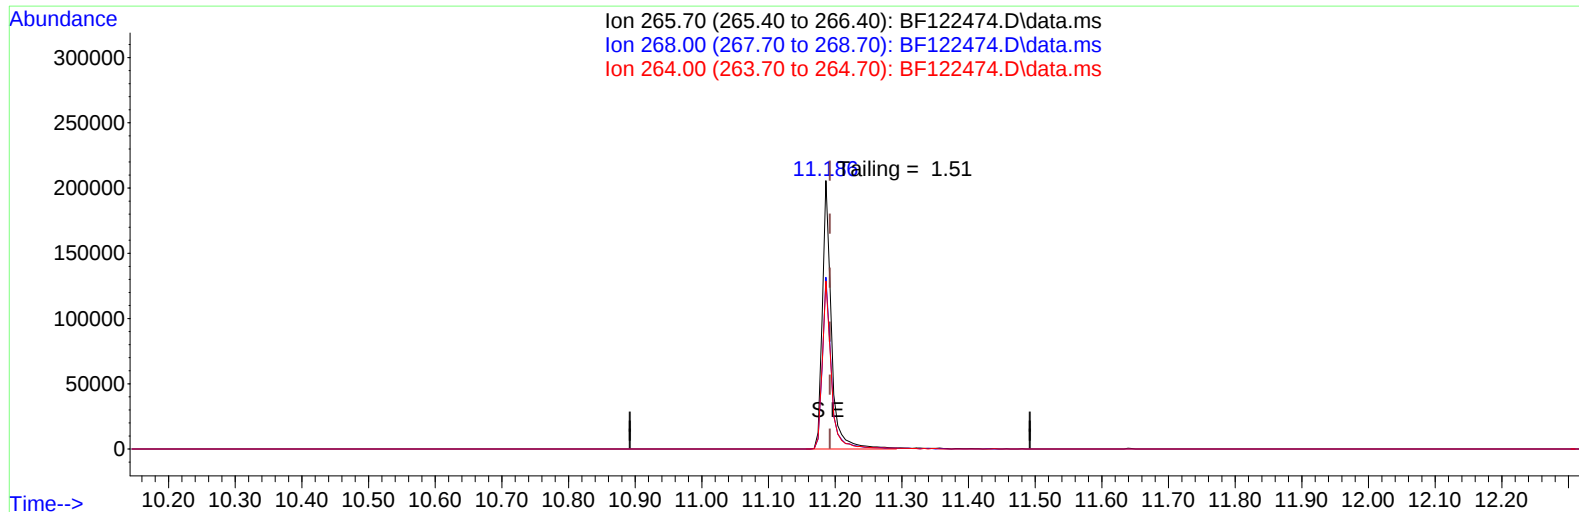

TIC: BF122474.D\data.ms

(70) Pentachlorophenol (C)




11.186min (-0.006) 30999.07 ng

response 195685

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	64.00
264.00	62.40	62.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112520\
Data File : BF122474.D
Acq On : 25 Nov 2020 9:04
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 26 01:56:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 24 14:38:56 2020
Response via : Initial Calibration

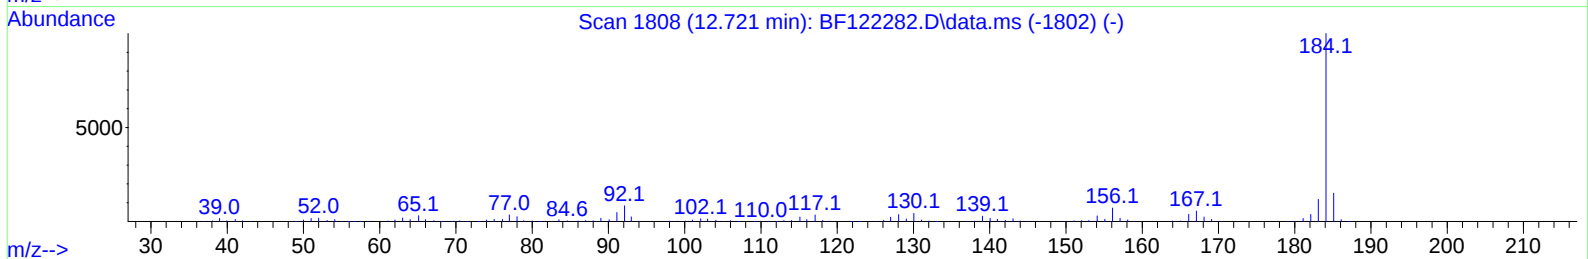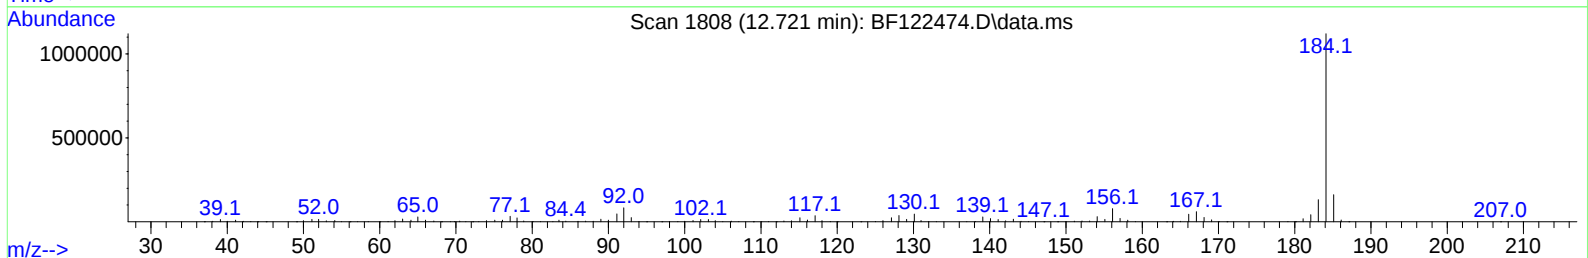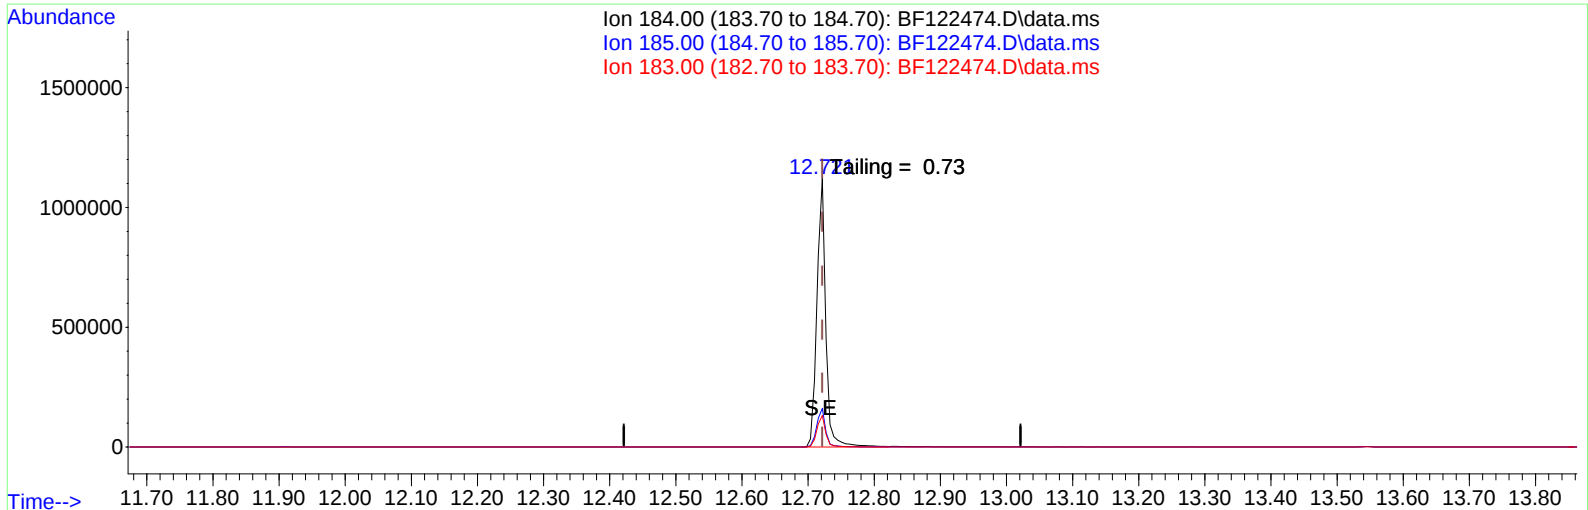

TIC: BF122474.D\data.ms

(77) Benzidine

12.721min (-0.000) 0.00 ng

response 1044001

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.38
183.00	11.70	11.79
0.00	0.00	0.00