

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112520\
 Data File : BF122476.D
 Acq On : 25 Nov 2020 10:11
 Operator : JU/CG
 Sample : PB133227BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB133227BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122476.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.204	17	20	35	rVB	74733	122657	1.15%	0.215%
2	5.092	504	511	516	rVB	96590	125555	1.18%	0.220%
3	5.487	573	578	581	rBV	4241911	4272332	40.04%	7.487%
4	6.492	743	749	752	rBV	3849020	4349618	40.76%	7.623%
5	6.857	807	811	814	rBV	1628605	1451663	13.60%	2.544%
6	7.016	833	838	841	rBV	6142264	5866512	54.98%	10.281%
7	7.422	900	907	910	rBV	4249753	4893269	45.86%	8.575%
8	8.139	1024	1029	1047	rBV	2155940	1937117	18.15%	3.395%
9	9.222	1206	1213	1216	rBV	7908263	8965509	84.02%	15.712%
10	9.898	1322	1328	1331	rBV	2580261	2347969	22.00%	4.115%
11	10.686	1456	1462	1482	rBV	3810677	3964038	37.15%	6.947%
12	11.380	1574	1580	1588	rBV	2584342	2539080	23.80%	4.450%
13	12.980	1844	1852	1855	rBV	8963378	10670572	100.00%	18.700%
14	14.021	2025	2029	2037	rBV	2758591	2715368	25.45%	4.759%
15	15.492	2273	2279	2295	rBV	1912896	2709746	25.39%	4.749%
16	16.927	2516	2523	2537	rVB4	38327	131317	1.23%	0.230%




Sum of corrected areas: 57062322

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112520\
Data File : BF122476.D
Acq On : 25 Nov 2020 10:11
Operator : JU/CG
Sample : PB133227BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133227BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

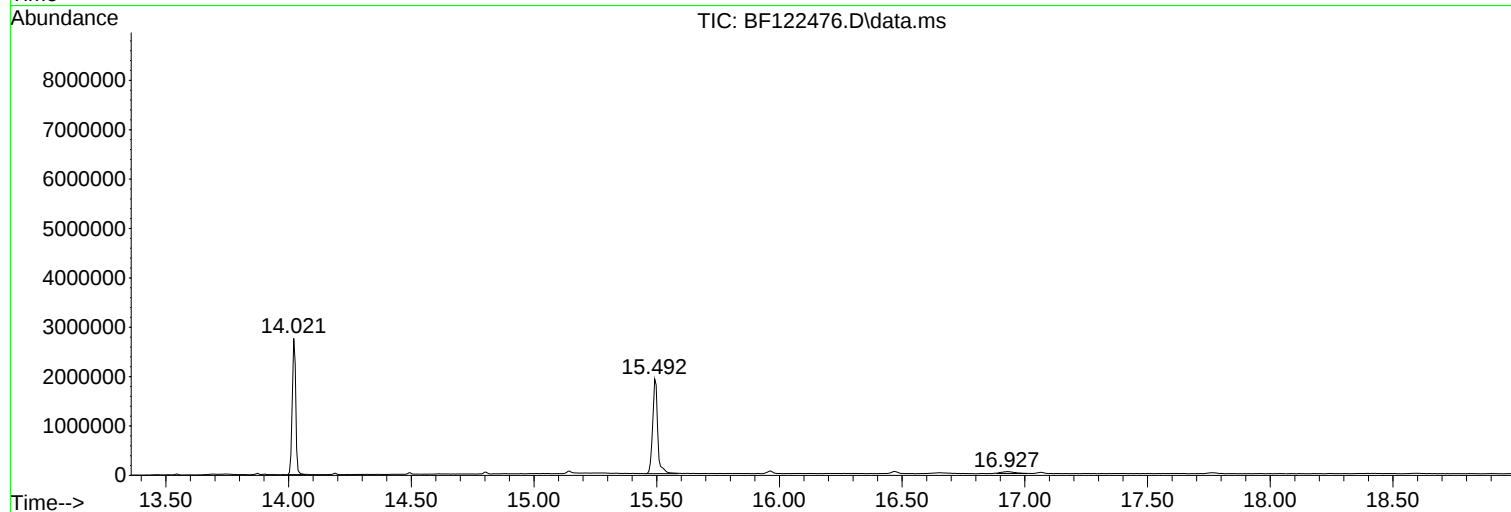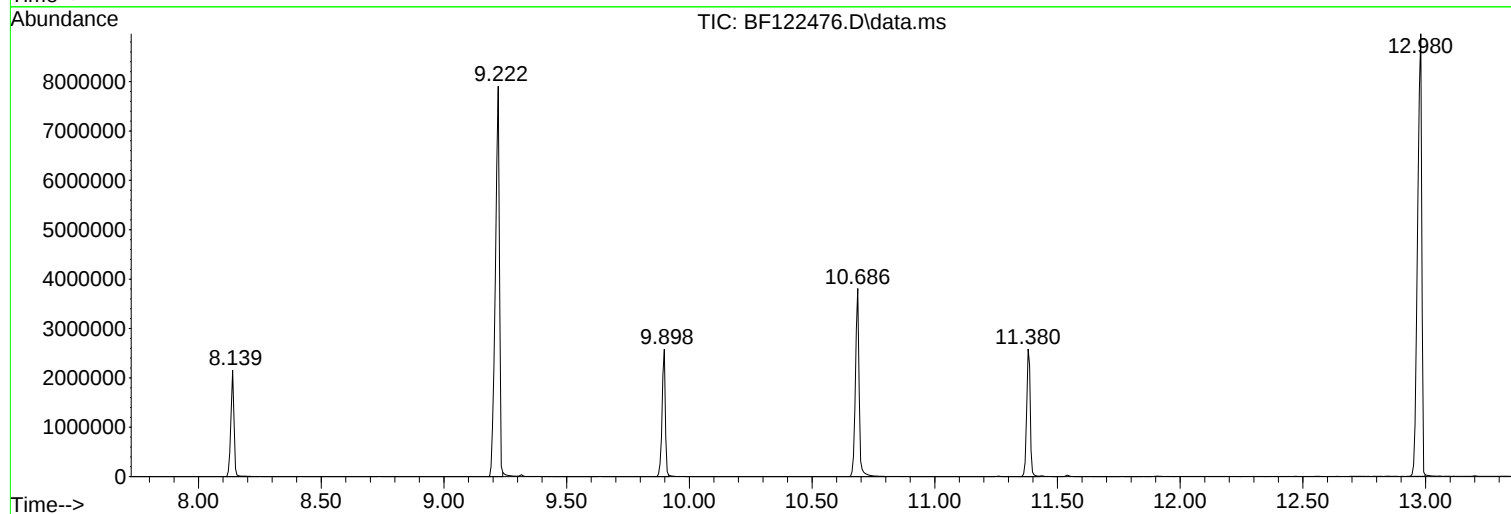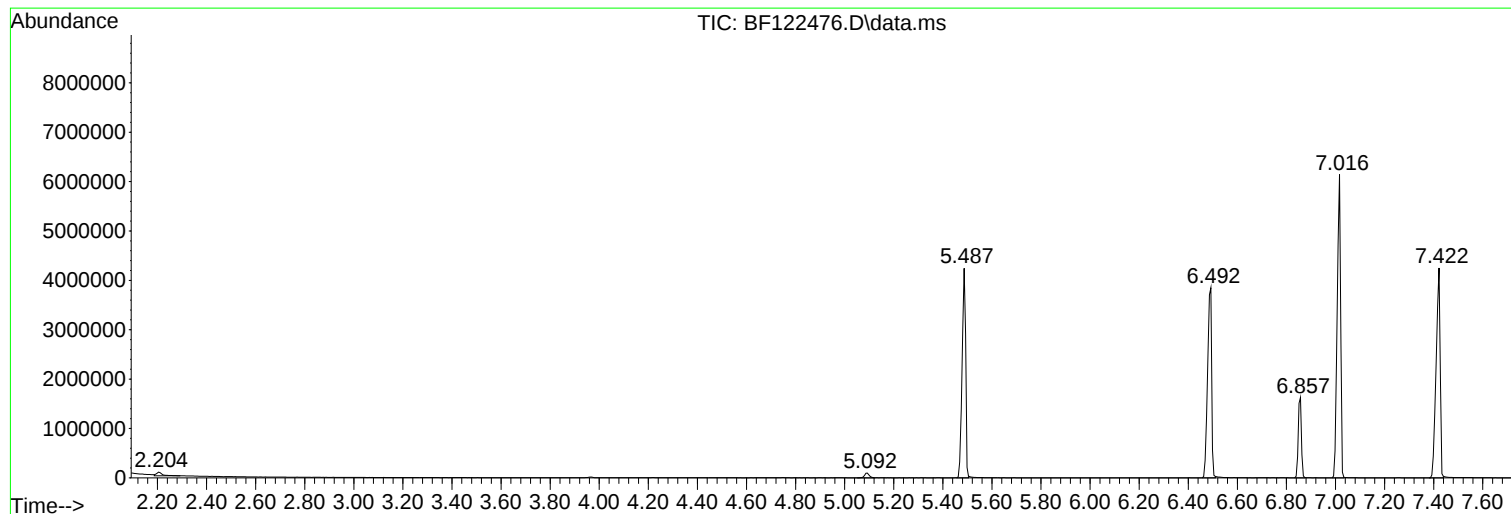

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112520\
Data File : BF122476.D
Acq On : 25 Nov 2020 10:11
Operator : JU/CG
Sample : PB133227BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133227BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112520\
Data File : BF122476.D
Acq On : 25 Nov 2020 10:11
Operator : JU/CG
Sample : PB133227BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133227BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------