

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112520\
 Data File : BF122483.D
 Acq On : 25 Nov 2020 14:20
 Operator : JU/CG
 Sample : L4891-03 2X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PAV-B3-112420-0-10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122483.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.122	3	6	12	rVB	222149	280418	4.83%	0.396%
2	5.475	572	576	588	rBV	2389004	2082722	35.87%	2.938%
3	6.487	743	748	762	rBV	2489051	2174732	37.45%	3.068%
4	6.681	778	781	787	rBV	98319	100819	1.74%	0.142%
5	6.857	807	811	814	rBV	1490225	1222572	21.06%	1.725%
6	7.416	901	906	909	rBV	1609779	1386518	23.88%	1.956%
7	8.139	1025	1029	1031	rBV	1946704	1688724	29.08%	2.382%
8	8.163	1031	1033	1036	rVB	1168283	865092	14.90%	1.220%
9	8.851	1146	1150	1156	rBV	489605	425007	7.32%	0.600%
10	8.951	1162	1167	1171	rBB	400698	326361	5.62%	0.460%
11	9.216	1208	1212	1215	rBV	3270312	2622175	45.16%	3.699%
12	9.316	1222	1229	1235	rVB	217946	203262	3.50%	0.287%
13	9.410	1243	1245	1251	rVB	72809	78519	1.35%	0.111%
14	9.480	1251	1257	1261	rBV2	137196	201065	3.46%	0.284%
15	9.551	1265	1269	1272	rBV	241398	260421	4.49%	0.367%
16	9.580	1272	1274	1276	rVV	198886	151025	2.60%	0.213%
17	9.610	1276	1279	1283	rVV	459832	377424	6.50%	0.532%
18	9.669	1284	1289	1294	rVV2	118204	158915	2.74%	0.224%
19	9.757	1298	1304	1308	rVB	382326	313976	5.41%	0.443%
20	9.898	1322	1328	1331	rVV	2301320	2049732	35.30%	2.891%
21	9.928	1331	1333	1336	rVV	947188	752825	12.97%	1.062%
22	9.963	1336	1339	1342	rVB	78149	73125	1.26%	0.103%
23	10.051	1349	1354	1359	rBV2	73024	87298	1.50%	0.123%
24	10.098	1359	1362	1366	rBV	820918	746193	12.85%	1.053%
25	10.139	1366	1369	1377	rVB	86360	92058	1.59%	0.130%
26	10.210	1377	1381	1384	rBV3	81462	87043	1.50%	0.123%
27	10.304	1393	1397	1399	rBV	78343	102877	1.77%	0.145%
28	10.445	1417	1421	1426	rVB	931184	880448	15.16%	1.242%
29	10.527	1433	1435	1438	rVB2	86768	72178	1.24%	0.102%
30	10.598	1445	1447	1451	rVB	283353	249352	4.29%	0.352%
31	10.680	1453	1461	1466	rVV	1919683	2047011	35.25%	2.887%
32	10.733	1467	1470	1474	rVB2	75255	81853	1.41%	0.115%
33	10.810	1479	1483	1489	rVB2	93603	114785	1.98%	0.162%
34	10.992	1505	1514	1516	rBV4	181254	275231	4.74%	0.388%
35	11.016	1516	1518	1521	rVB2	76720	71293	1.23%	0.101%
36	11.075	1525	1528	1531	rVB2	72854	72063	1.24%	0.102%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112520\
 Data File : BF122483.D
 Acq On : 25 Nov 2020 14:20
 Operator : JU/CG
 Sample : L4891-03 2X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PAV-B3-112420-0-10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.122	1531	1536	1538	rBV2	138670	176175	3.03%	0.249%
38	11.186	1544	1547	1551	rVB	424710	367528	6.33%	0.518%
39	11.233	1551	1555	1559	rBV3	145851	245665	4.23%	0.347%
40	11.280	1559	1563	1568	rVB	480035	455331	7.84%	0.642%

41	11.386	1575	1581	1583	rBV	1968532	2247002	38.70%	3.170%
42	11.416	1583	1586	1588	rVV	6282042	5806343	100.00%	8.190%
43	11.457	1588	1593	1596	rVV	1212128	1253967	21.60%	1.769%
44	11.492	1596	1599	1602	rVB	159729	153315	2.64%	0.216%
45	11.610	1613	1619	1622	rBV2	620504	675193	11.63%	0.952%

46	11.680	1627	1631	1634	rVV2	187097	184163	3.17%	0.260%
47	11.716	1634	1637	1642	rVB5	103375	120571	2.08%	0.170%
48	11.886	1660	1666	1668	rBV	658271	626023	10.78%	0.883%
49	11.910	1668	1670	1675	rVV	947558	909779	15.67%	1.283%
50	11.957	1675	1678	1681	rVV	250600	236464	4.07%	0.334%

51	11.998	1681	1685	1687	rVV	935320	949093	16.35%	1.339%
52	12.022	1687	1689	1693	rVB	375504	309254	5.33%	0.436%
53	12.086	1698	1700	1703	rVB2	92861	74723	1.29%	0.105%
54	12.180	1713	1716	1718	rBV	594220	497932	8.58%	0.702%
55	12.204	1718	1720	1723	rVB	823706	616539	10.62%	0.870%

56	12.327	1736	1741	1744	rBV3	142081	157424	2.71%	0.222%
57	12.357	1744	1746	1749	rVV	89199	85151	1.47%	0.120%
58	12.386	1749	1751	1753	rVB	95592	75306	1.30%	0.106%
59	12.433	1755	1759	1763	rBV2	220938	281809	4.85%	0.398%
60	12.474	1763	1766	1768	rVV	162142	175701	3.03%	0.248%

61	12.521	1771	1774	1779	rVB	231122	262451	4.52%	0.370%
62	12.604	1783	1788	1791	rBV	5043670	4740725	81.65%	6.687%
63	12.657	1796	1797	1800	rVB2	92805	72294	1.25%	0.102%
64	12.692	1800	1803	1805	rVB	160872	121789	2.10%	0.172%
65	12.727	1805	1809	1811	rBV	142338	192344	3.31%	0.271%

66	12.745	1811	1812	1816	rVB	173503	141451	2.44%	0.200%
67	12.833	1820	1827	1831	rBV2	4083448	4890053	84.22%	6.898%
68	12.874	1831	1834	1839	rVB2	221142	245273	4.22%	0.346%
69	12.945	1842	1846	1847	rBV	306605	267523	4.61%	0.377%
70	12.968	1847	1850	1857	rVB	2954787	2646549	45.58%	3.733%

71	13.045	1857	1863	1866	rBV2	251899	426884	7.35%	0.602%
72	13.127	1874	1877	1879	rBV3	190204	217040	3.74%	0.306%
73	13.151	1879	1881	1884	rVB	469355	412674	7.11%	0.582%
74	13.221	1890	1893	1895	rVB	263294	226479	3.90%	0.319%
75	13.257	1895	1899	1902	rBV2	400976	408973	7.04%	0.577%

76	13.351	1912	1915	1917	rBV	169312	140918	2.43%	0.199%
----	--------	------	------	------	-----	--------	--------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112520\
 Data File : BF122483.D
 Acq On : 25 Nov 2020 14:20
 Operator : JU/CG
 Sample : L4891-03 2X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PAV-B3-112420-0-10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	13.380	1917	1920	1924	rBV2	198540	198655	3.42%	0.280%
78	13.451	1929	1932	1938	rVB4	136337	169820	2.92%	0.240%
79	13.551	1943	1949	1952	rBV6	84496	206283	3.55%	0.291%
80	13.657	1964	1967	1972	rVB	231540	246057	4.24%	0.347%
81	13.768	1982	1986	1989	rBV2	216822	296180	5.10%	0.418%
82	13.798	1989	1991	1993	rVV	300016	270212	4.65%	0.381%
83	13.821	1993	1995	2000	rVV2	248692	367520	6.33%	0.518%
84	13.868	2000	2003	2011	rVB2	474575	642213	11.06%	0.906%
85	14.021	2021	2029	2032	rBV3	2224653	3316584	57.12%	4.678%
86	14.051	2032	2034	2040	rVB	1745516	1472195	25.35%	2.077%
87	14.127	2045	2047	2050	rVV	236563	191288	3.29%	0.270%
88	14.251	2064	2068	2071	rBV2	107505	147087	2.53%	0.207%
89	14.410	2092	2095	2098	rVB	243325	212836	3.67%	0.300%
90	14.445	2098	2101	2105	rVB2	164949	160910	2.77%	0.227%
91	14.533	2114	2116	2118	rVV	103502	74005	1.27%	0.104%
92	14.557	2118	2120	2123	rVB3	122597	109933	1.89%	0.155%
93	15.068	2202	2207	2210	rBV	1174303	1842752	31.74%	2.599%
94	15.174	2222	2225	2229	rBV	194422	188275	3.24%	0.266%
95	15.368	2254	2258	2264	rVB	711650	963913	16.60%	1.360%
96	15.433	2264	2269	2274	rBV	1136881	1362922	23.47%	1.922%
97	15.498	2275	2280	2283	rVV	1164563	1537520	26.48%	2.169%
98	15.527	2283	2285	2291	rVB2	348537	404084	6.96%	0.570%
99	16.956	2523	2528	2536	rVB2	481318	942481	16.23%	1.329%
100	17.398	2598	2603	2616	rVB	344264	700509	12.06%	0.988%




Sum of corrected areas: 70893217

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112520\
Data File : BF122483.D
Acq On : 25 Nov 2020 14:20
Operator : JU/CG
Sample : L4891-03 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PAV-B3-112420-0-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

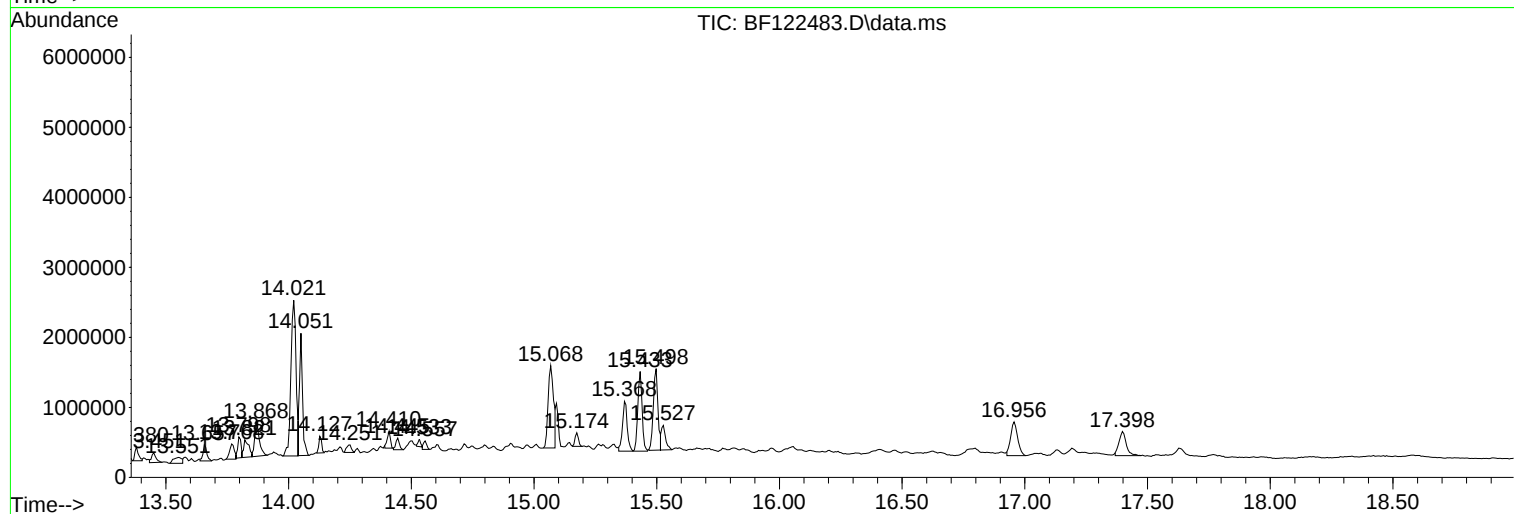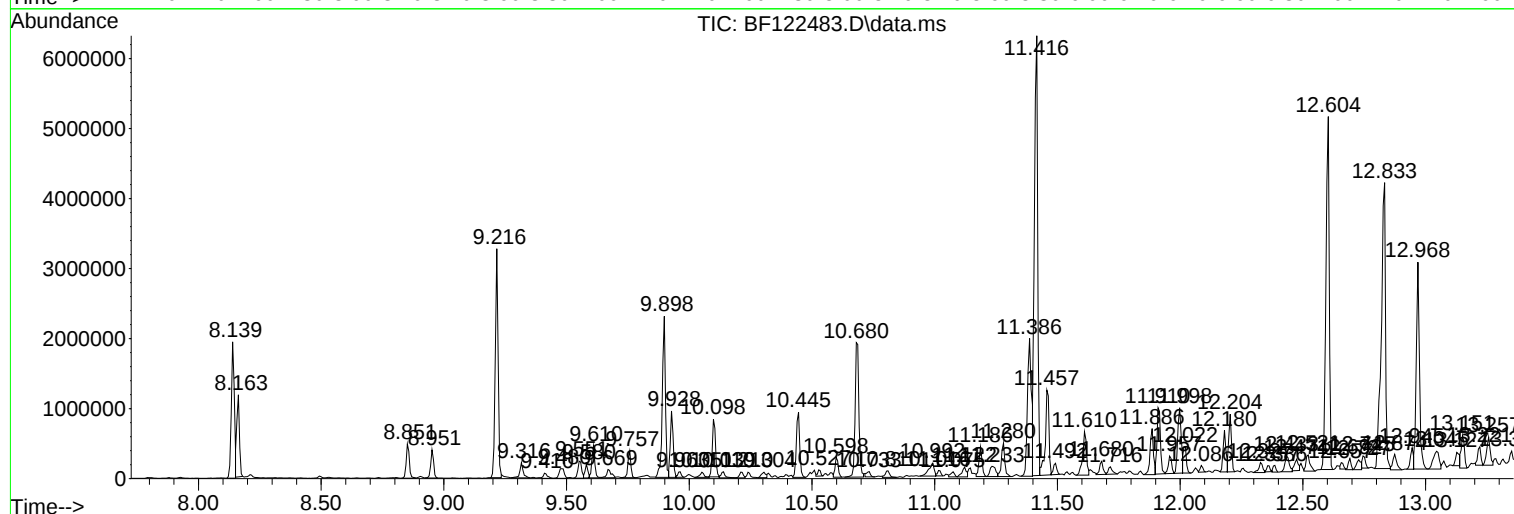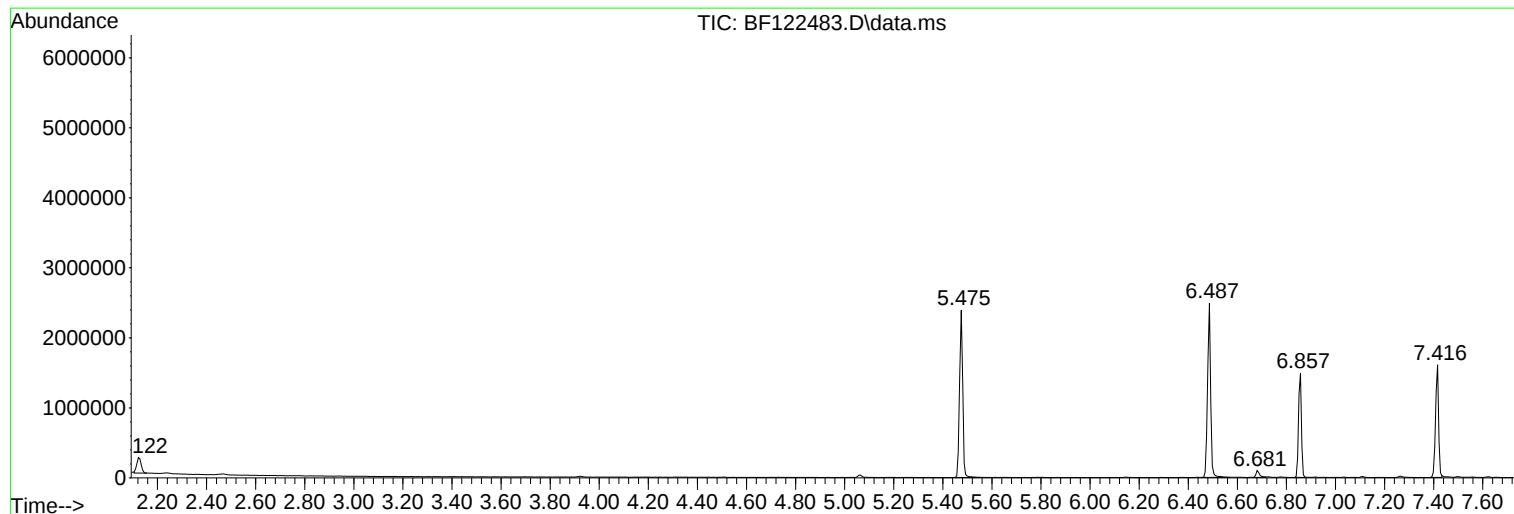

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112520\
Data File : BF122483.D
Acq On : 25 Nov 2020 14:20
Operator : JU/CG
Sample : L4891-03 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PAV-B3-112420-0-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112520\
Data File : BF122483.D
Acq On : 25 Nov 2020 14:20
Operator : JU/CG
Sample : L4891-03 2X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PAV-B3-112420-0-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
