


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112520\
 Data File : BF122474.D
 Acq On : 25 Nov 2020 9:04
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 24 14:38:56 2020

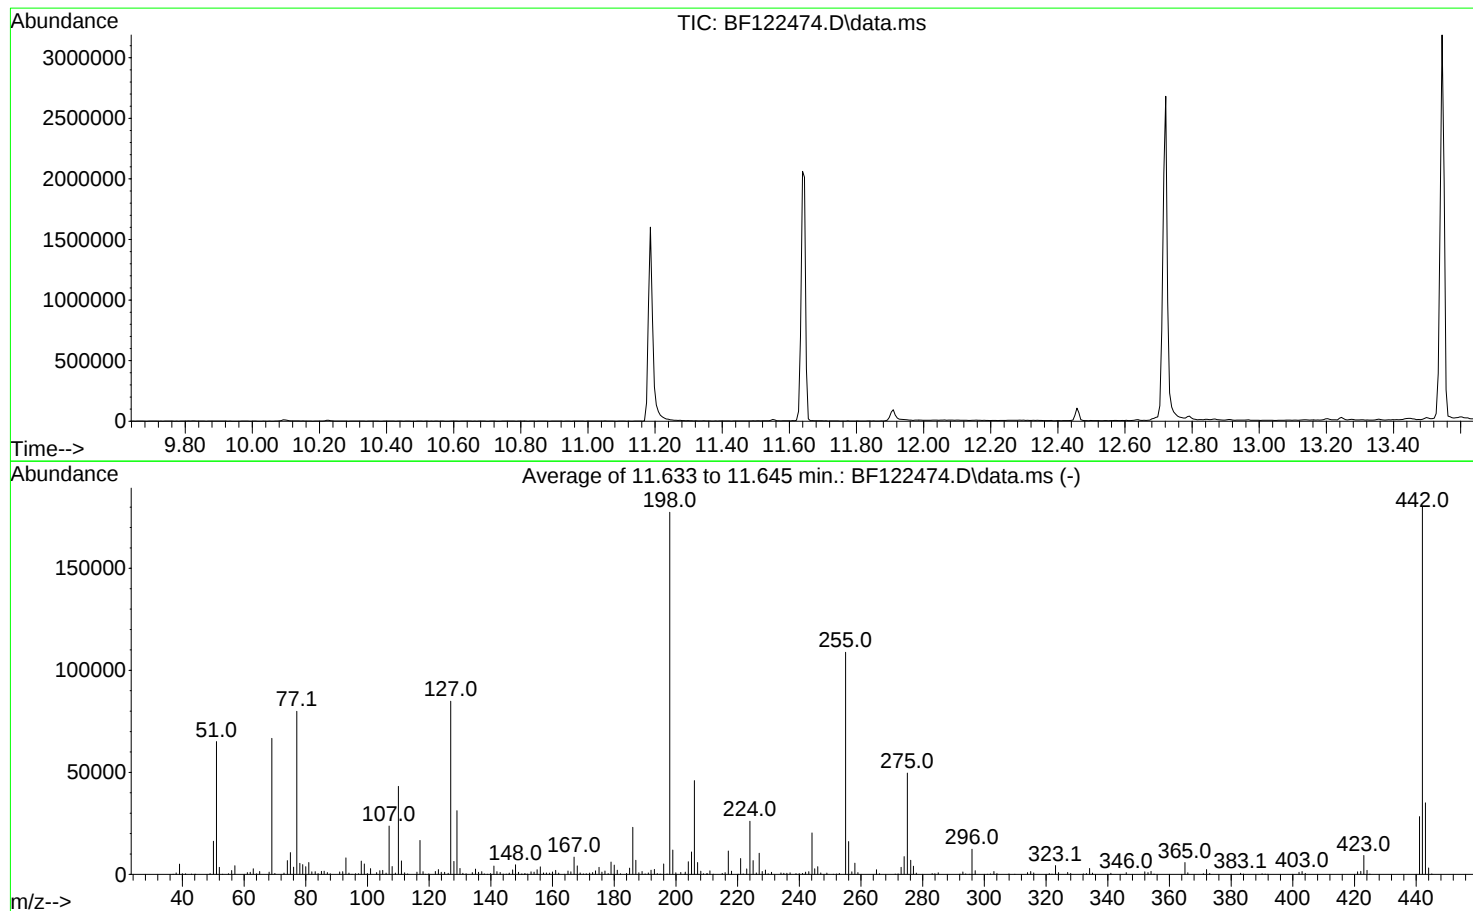

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	65083	PASS
68	69	0.00	2	1.7	1142	PASS
69	198	0.00	100	37.6	66680	PASS
70	69	0.00	2	0.7	455	PASS
127	198	10	80	47.8	84835	PASS
197	198	0.00	2	0.1	210	PASS
198	198	100	100	100.0	177507	PASS
199	198	5	9	6.7	11957	PASS
275	198	10	60	28.0	49643	PASS
365	198	1	100	3.3	5780	PASS
441	198	0.01	100	16.0	28315	PASS
442	442	100	100	100.0	180317	PASS
443	442	15	24	19.5	35086	PASS