
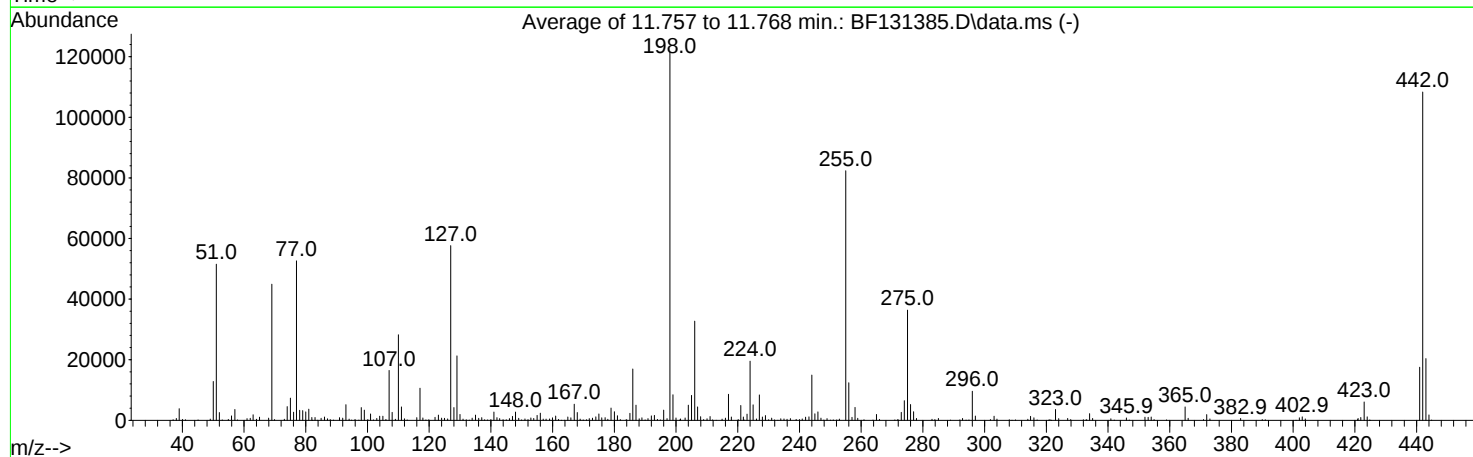


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112522\
 Data File : BF131385.D
 Acq On : 25 Nov 2022 09:01
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 01 12:46:17 2022

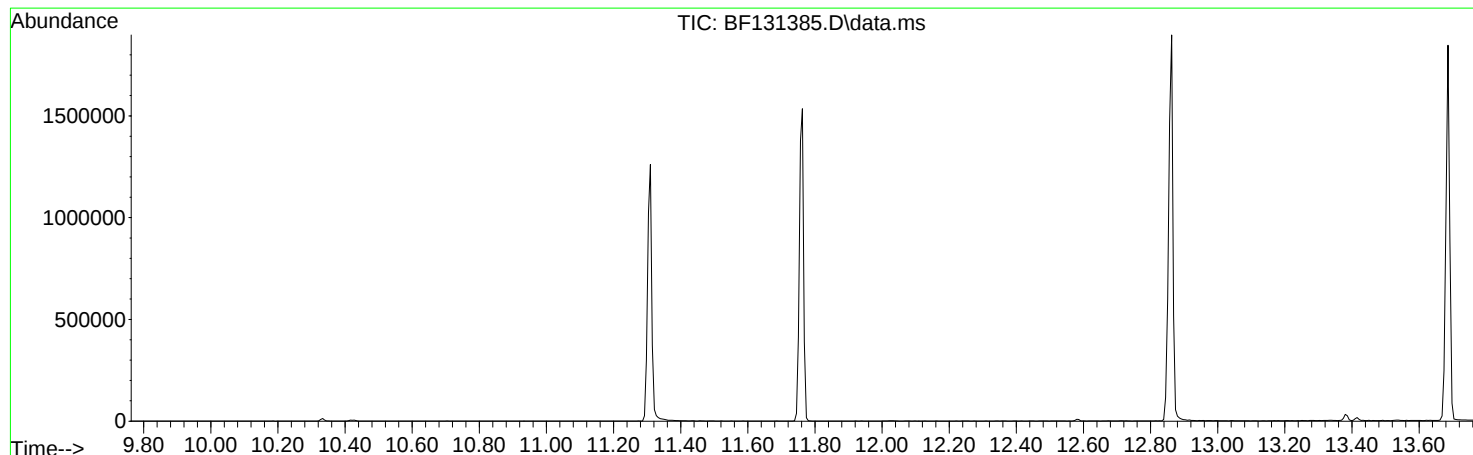




AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1638

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	51543	PASS
68	69	0.00	2	1.6	725	PASS
69	198	0.00	100	37.0	44912	PASS
70	69	0.00	2	0.5	234	PASS
127	198	10	80	47.5	57629	PASS
197	198	0.00	2	0.5	580	PASS
198	198	100	100	100.0	121408	PASS
199	198	5	9	6.9	8400	PASS
275	198	10	60	30.0	36385	PASS
365	198	1	100	3.6	4408	PASS
441	198	0.01	100	14.4	17514	PASS
442	442	50	100	100.0	108357	PASS
443	442	15	24	18.8	20348	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112522\
Data File : BF131385.D
Acq On : 25 Nov 2022 09:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 26 05:24:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 25 23:13:01 2022
Response via : Initial Calibration

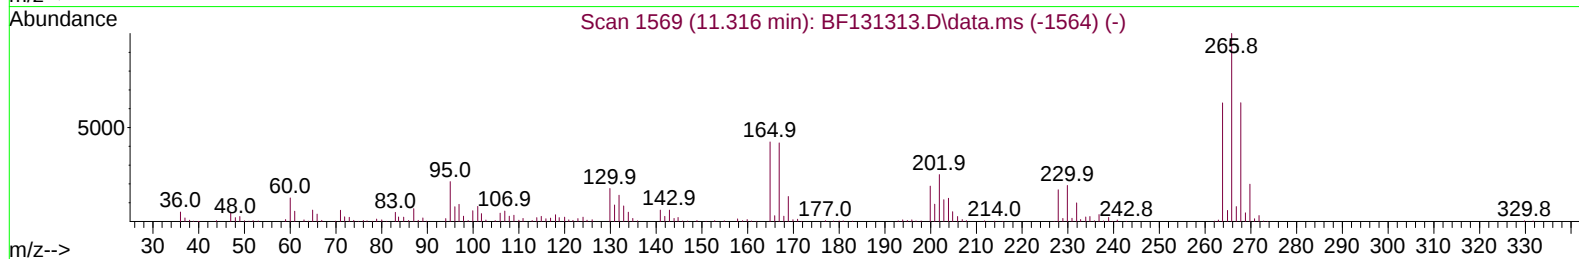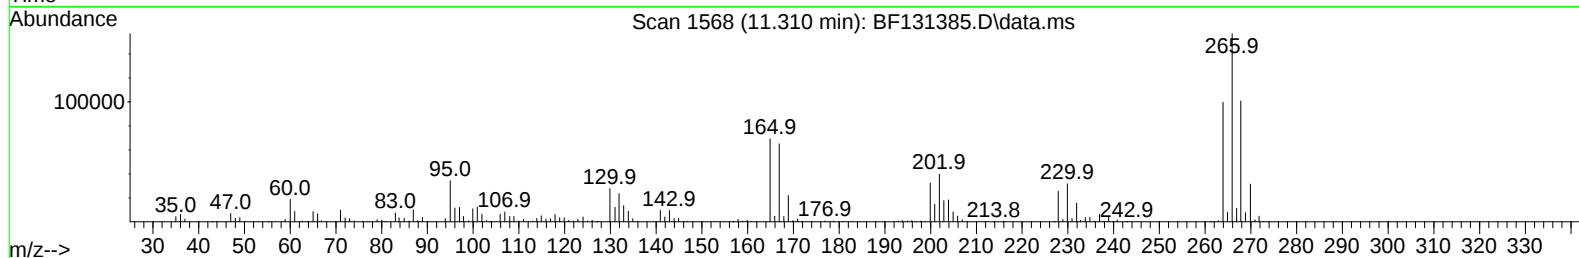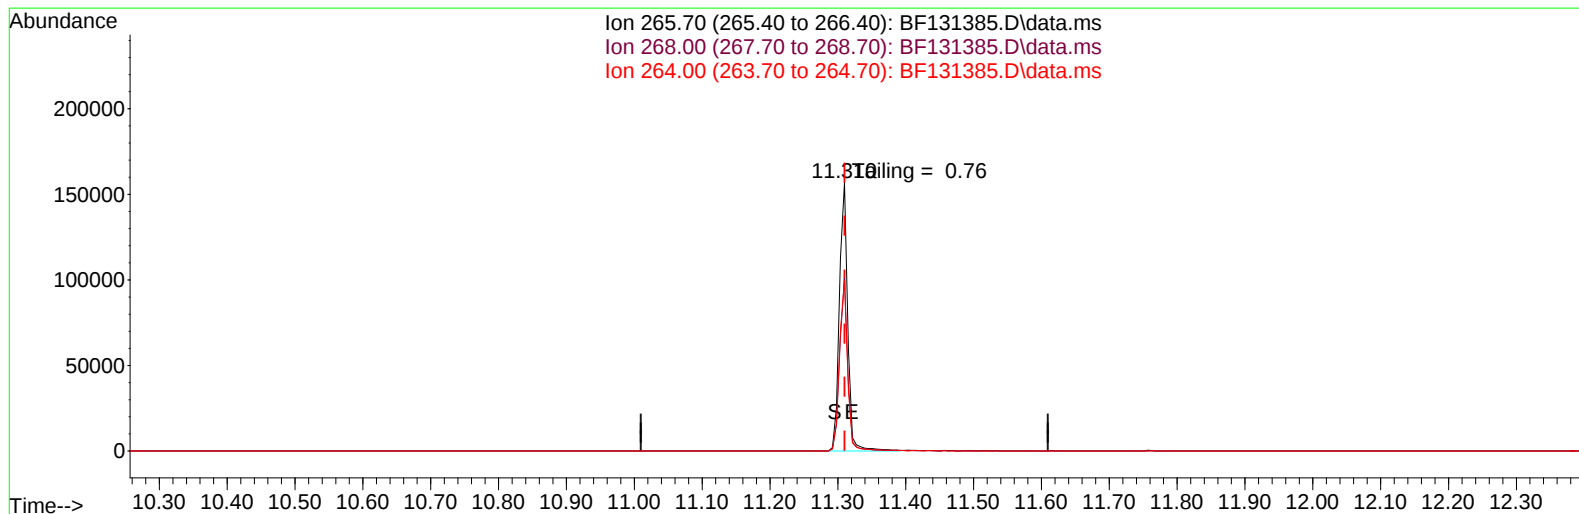

TIC: BF131385.D\data.ms

(70) Pentachlorophenol (C)

11.310min (-0.000) 26114.09 ng




response 133874

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	64.32
264.00	63.00	63.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112522\
Data File : BF131385.D
Acq On : 25 Nov 2022 09:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 26 05:24:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 25 23:13:01 2022
Response via : Initial Calibration

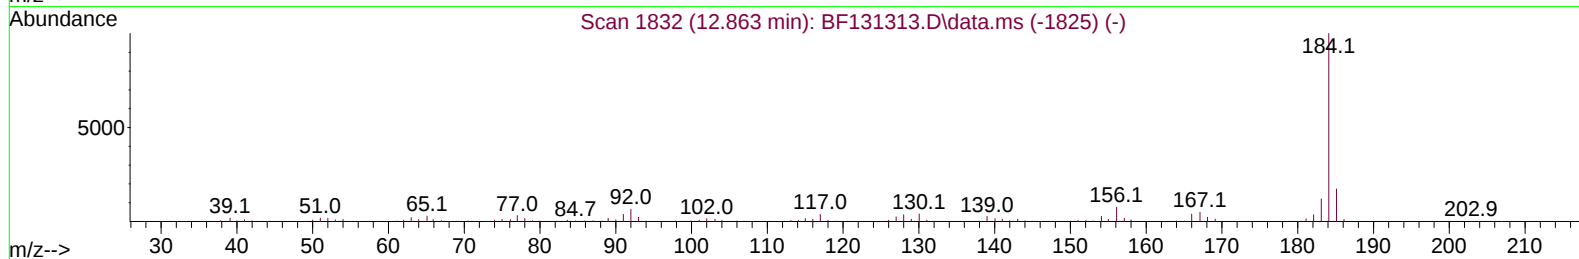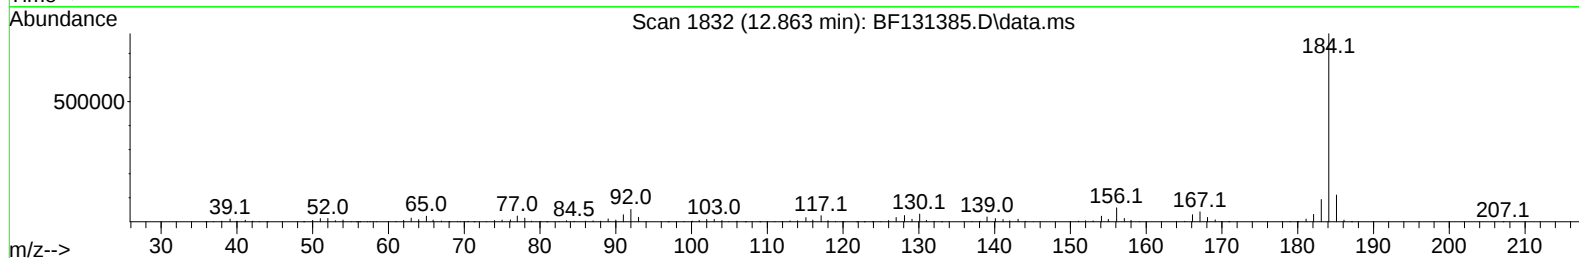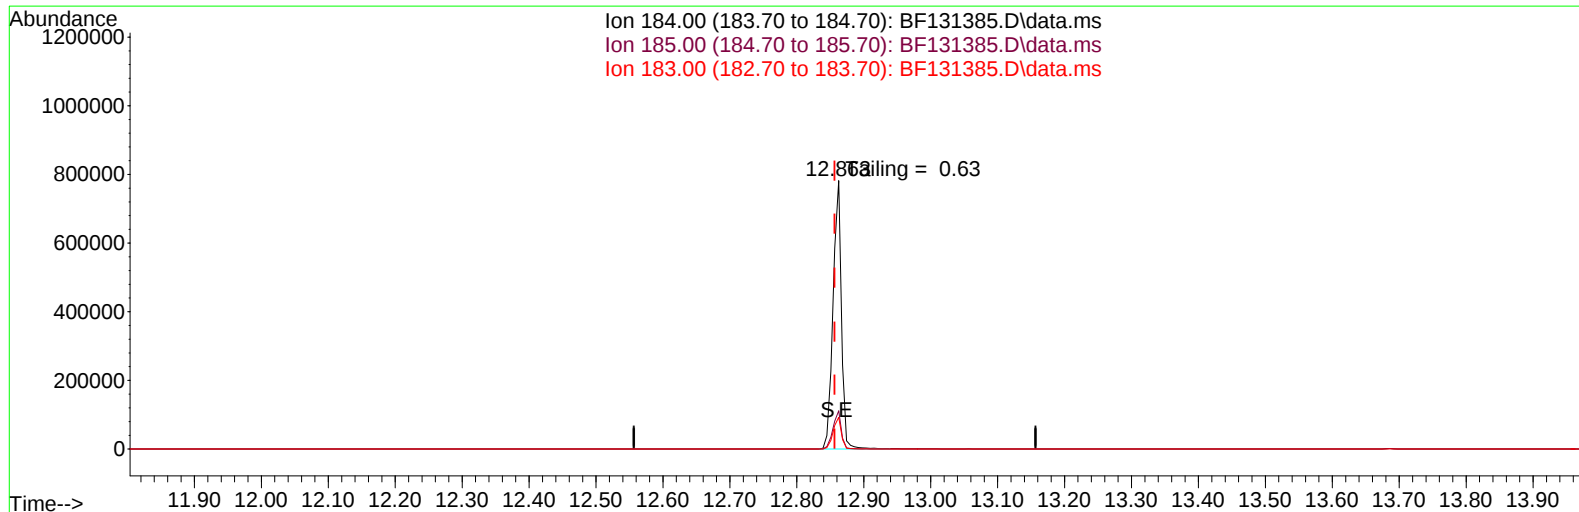

TIC: BF131385.D\data.ms

(77) Benzidine

12.863min (+ 0.006) 0.00 ng

response 686705

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	14.28
183.00	12.00	11.83
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/25/2022	BNA_F	<u>BF131385.D</u>
Compound Name	Response	Retention Time
DDT	291329	13.686
DDD	8428	13.38
DDE	291	13.045
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8719	300048	2.91

Instrument :
BNA_F
ClientSampleId :
DFTPP