


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112522\
 Data File : BF131397.D
 Acq On : 25 Nov 2022 15:50
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 01 12:46:17 2022

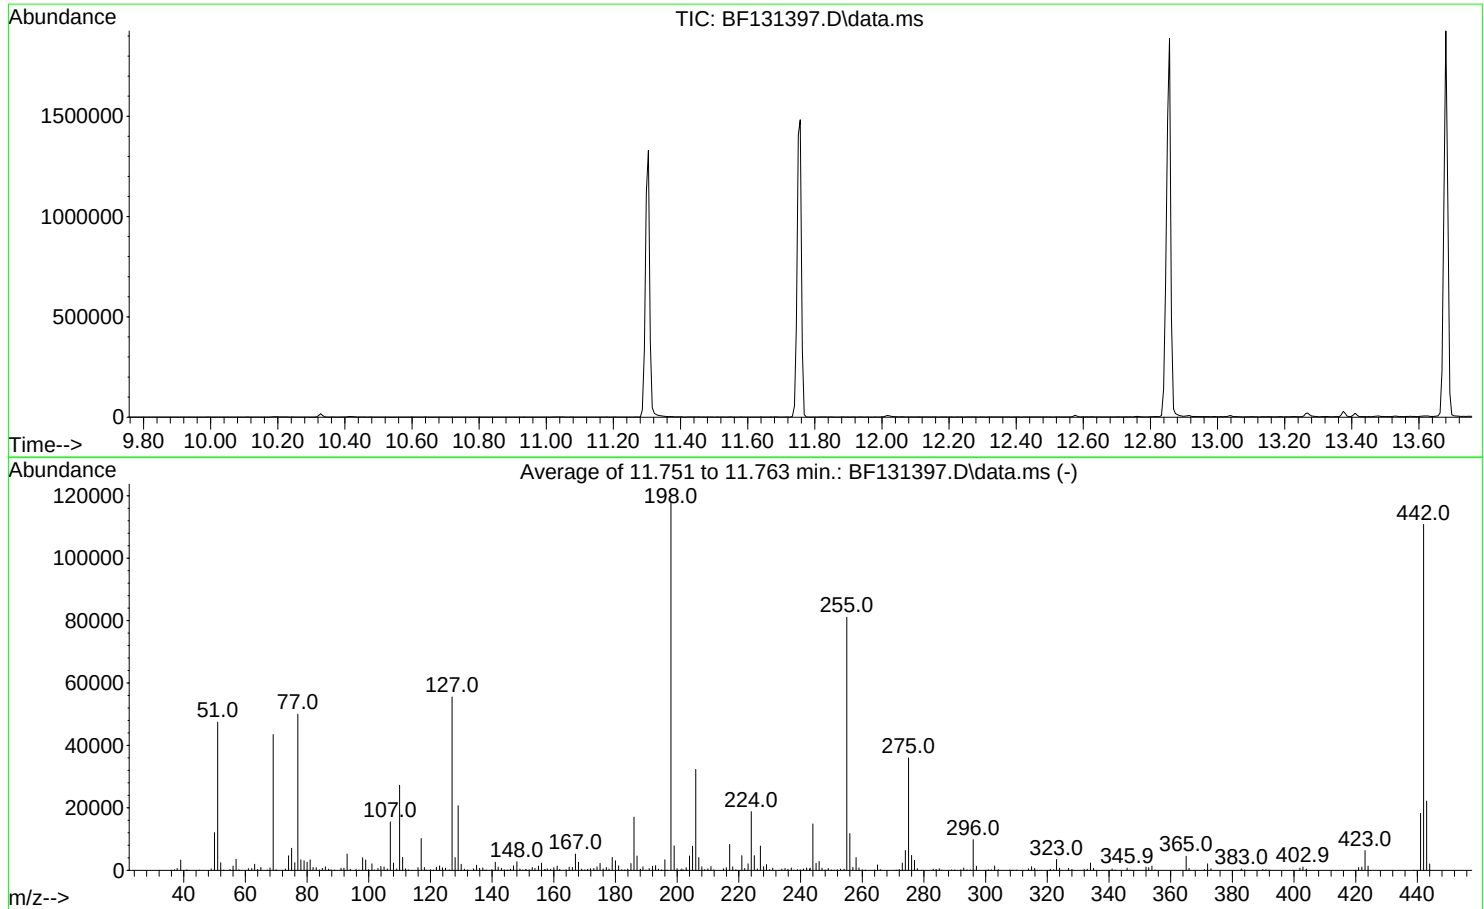




AutoFind: Scans 1643, 1644, 1645; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	47436	PASS
68	69	0.00	2	1.8	792	PASS
69	198	0.00	100	36.9	43507	PASS
70	69	0.00	2	0.4	186	PASS
127	198	10	80	47.1	55557	PASS
197	198	0.00	2	0.1	64	PASS
198	198	100	100	100.0	117864	PASS
199	198	5	9	6.6	7832	PASS
275	198	10	60	30.6	36022	PASS
365	198	1	100	3.8	4514	PASS
441	198	0.01	100	15.5	18213	PASS
442	442	50	100	100.0	110811	PASS
443	442	15	24	20.0	22168	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112522\
Data File : BF131397.D
Acq On : 25 Nov 2022 15:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 26 05:26:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 25 23:13:01 2022
Response via : Initial Calibration

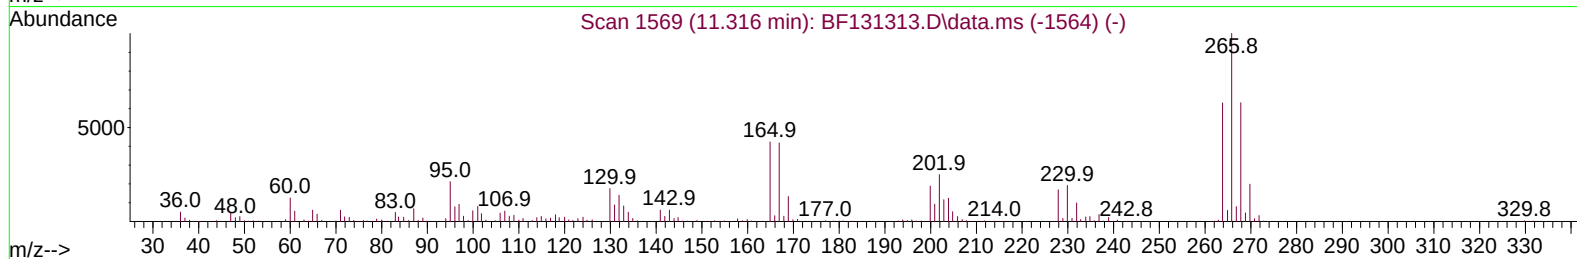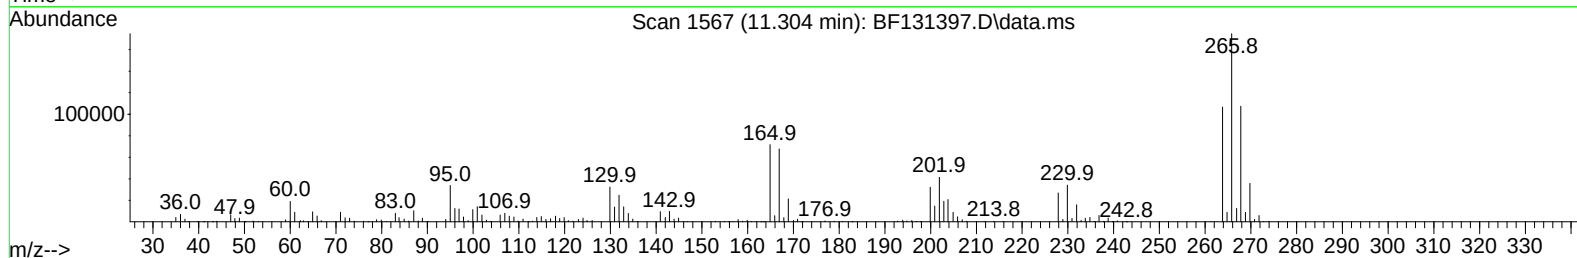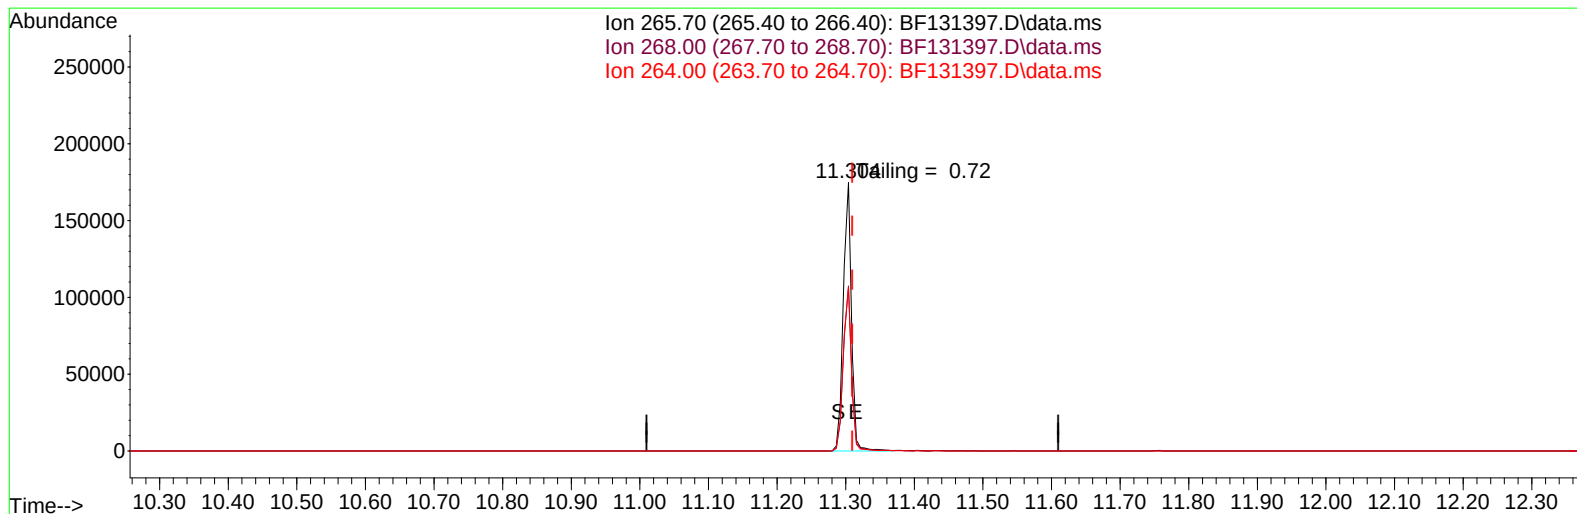

TIC: BF131397.D\data.ms

(70) Pentachlorophenol (C)

11.304min (-0.006) 36218.67 ng




response 144292

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	61.45
264.00	63.00	61.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112522\
Data File : BF131397.D
Acq On : 25 Nov 2022 15:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 26 05:26:16 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 25 23:13:01 2022
Response via : Initial Calibration

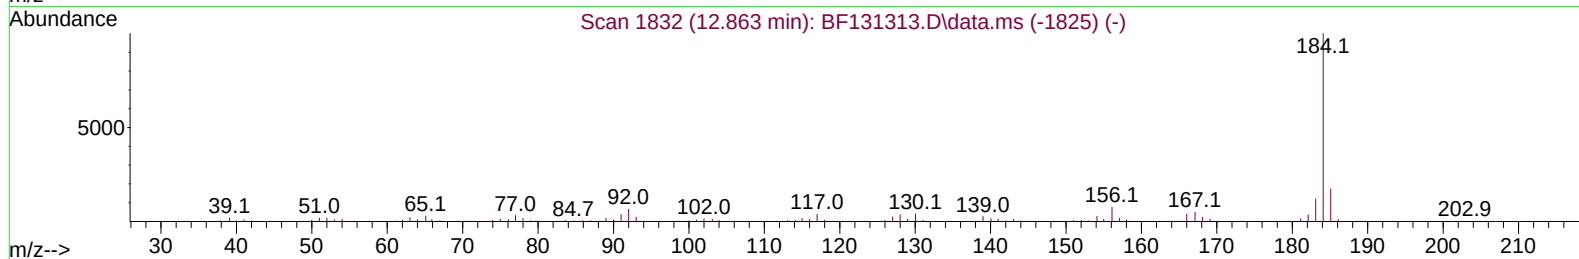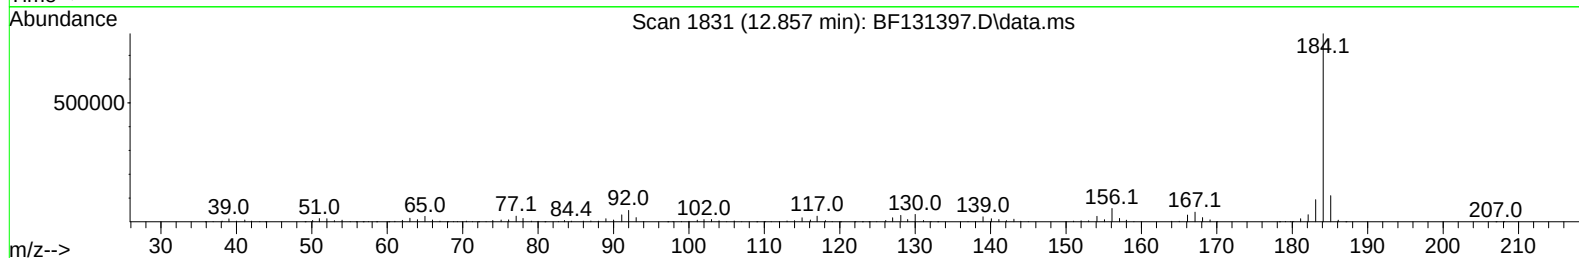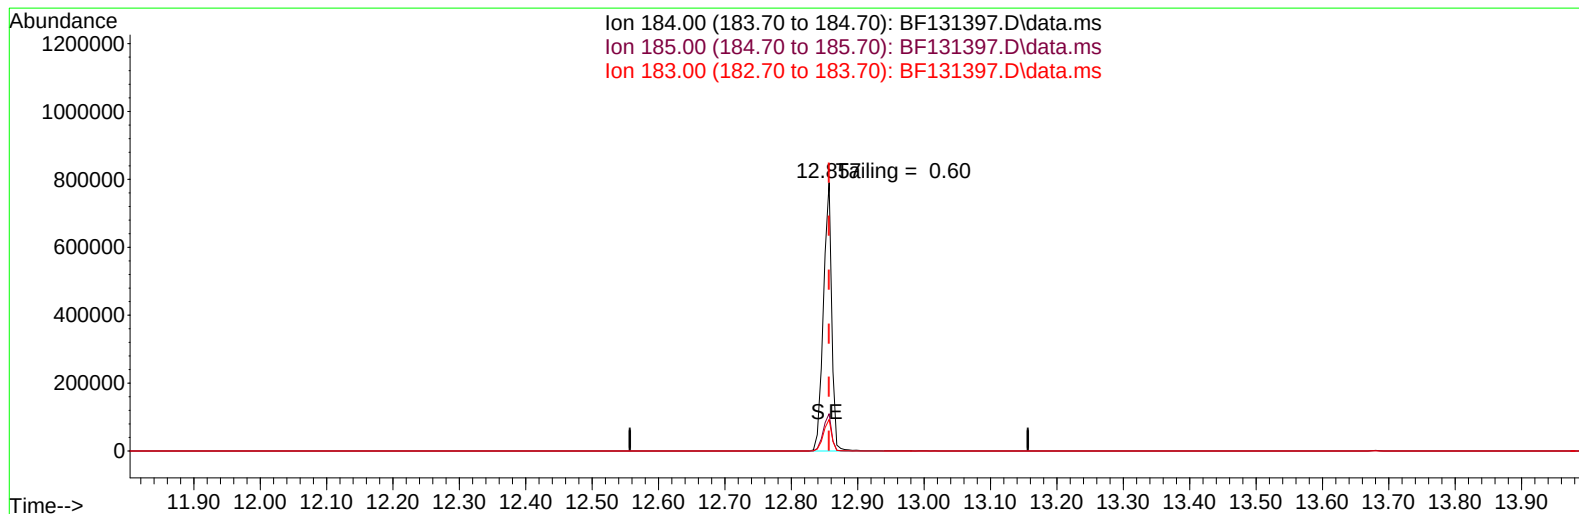

TIC: BF131397.D\data.ms

(77) Benzidine

12.857min (+ 0.000) 0.00 ng

response 688880

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	13.89
183.00	12.00	11.74
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/25/2022	BNA_F	<u>BF131397.D</u>
Compound Name	Response	Retention Time
DDT	313941	13.68
DDD	7650	13.374
DDE	1046	13.039
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8696	322637	2.70

Instrument :
BNA_F
ClientSampleId :
DFTPP